
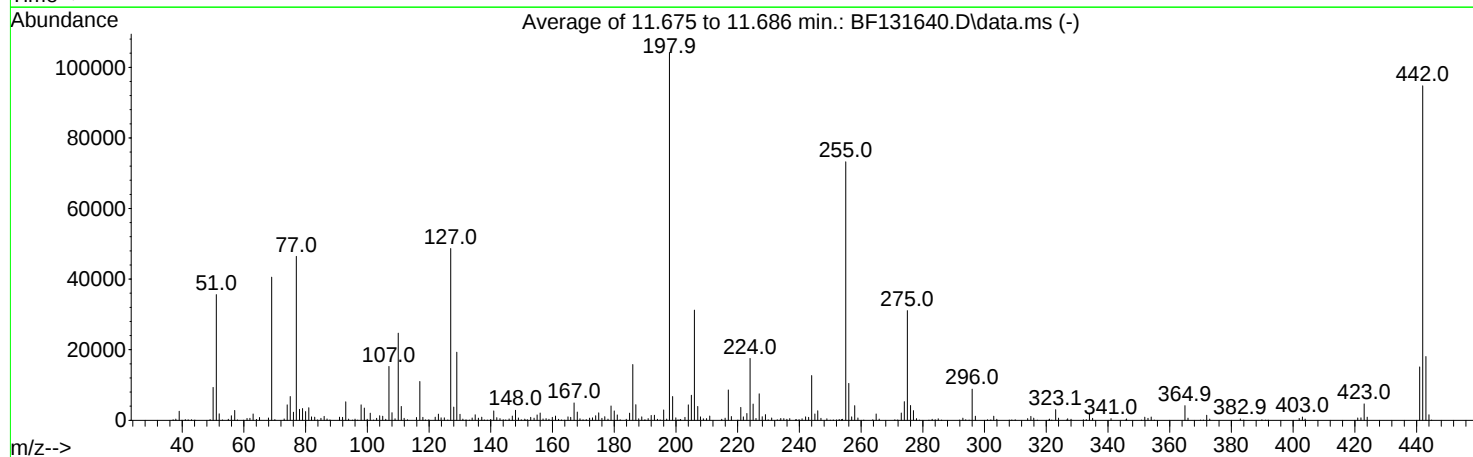


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121522\
 Data File : BF131640.D
 Acq On : 15 Dec 2022 10:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 16 01:44:46 2022

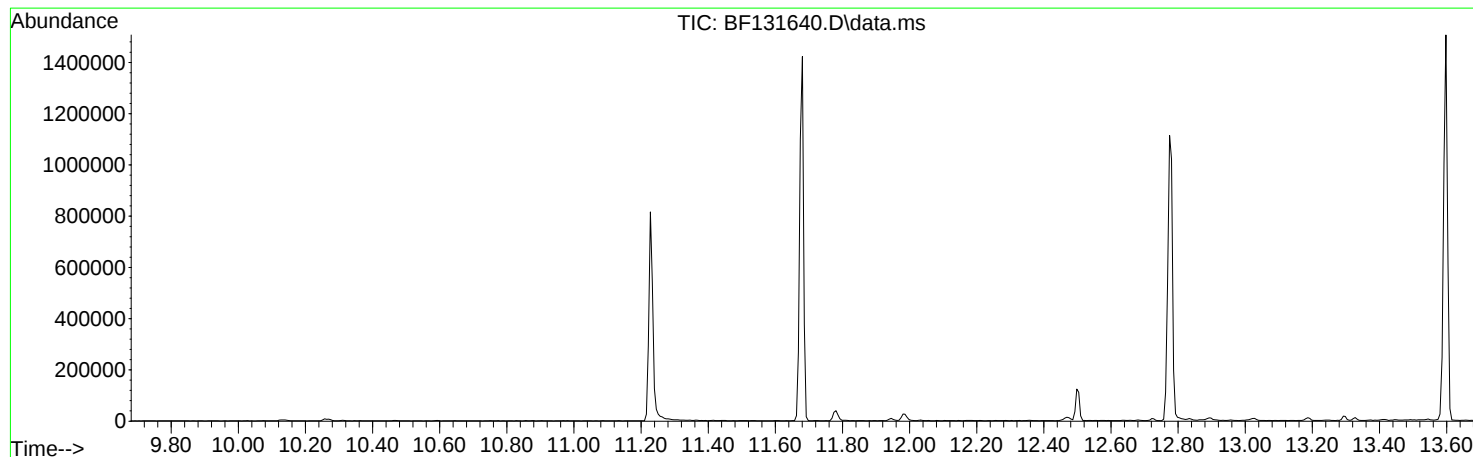




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	35597	PASS
68	69	0.00	2	1.7	680	PASS
69	198	0.00	100	38.9	40543	PASS
70	69	0.00	2	0.5	214	PASS
127	198	10	80	46.7	48664	PASS
197	198	0.00	2	0.4	366	PASS
198	198	100	100	100.0	104221	PASS
199	198	5	9	6.5	6745	PASS
275	198	10	60	29.8	31089	PASS
365	198	1	100	4.0	4147	PASS
441	198	0.01	100	14.5	15106	PASS
442	442	50	100	100.0	94779	PASS
443	442	15	24	19.1	18080	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121522\
Data File : BF131640.D
Acq On : 15 Dec 2022 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 07:43:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration

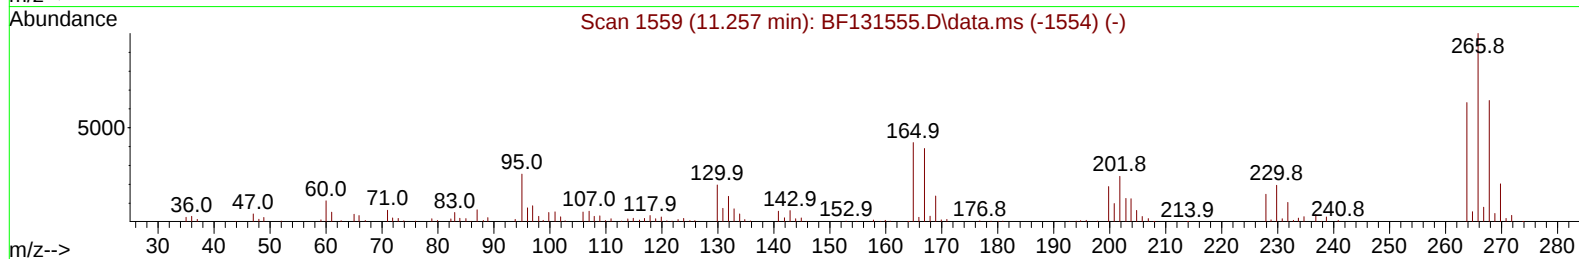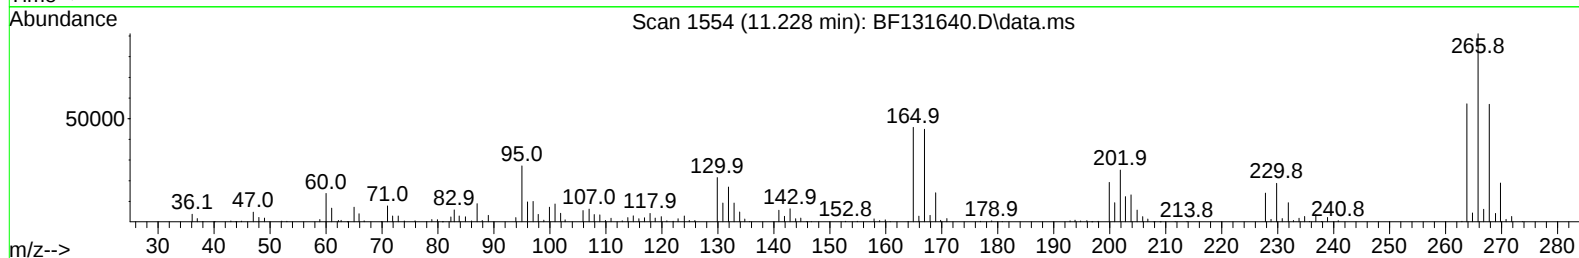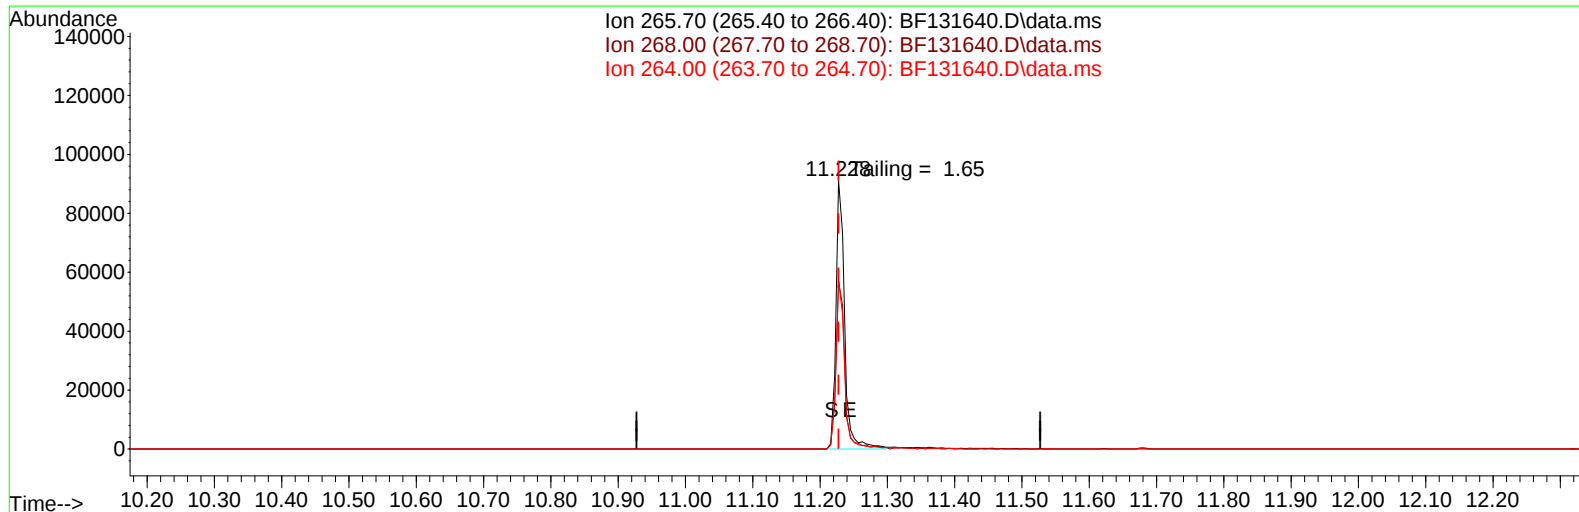

TIC: BF131640.D\data.ms

(70) Pentachlorophenol (C)

11.228min (+ 0.000) 195097.32 ng




response 82457

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.52
264.00	63.40	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121522\
Data File : BF131640.D
Acq On : 15 Dec 2022 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 07:43:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration

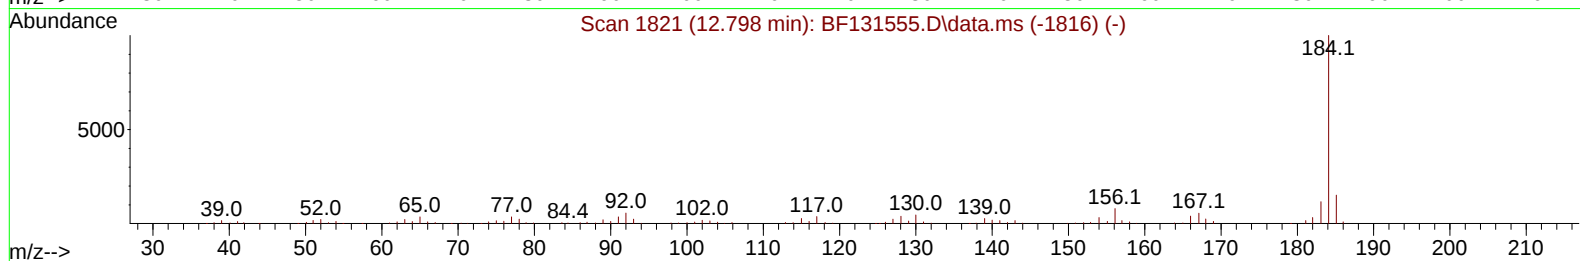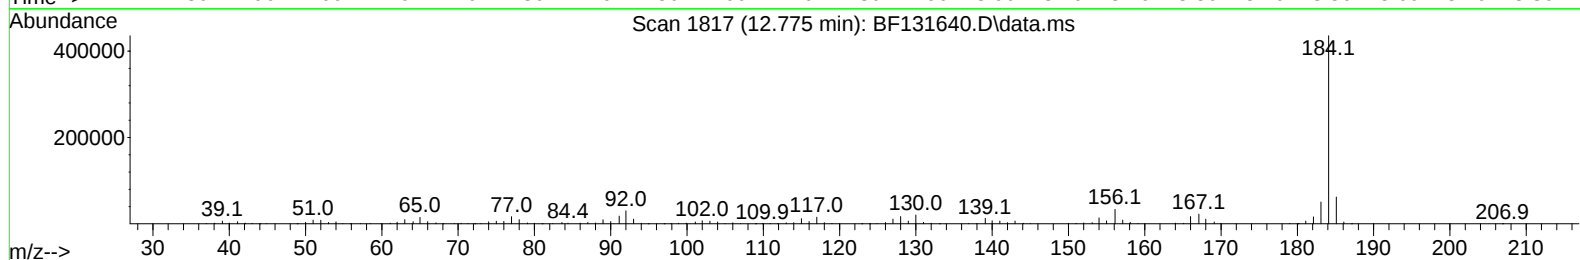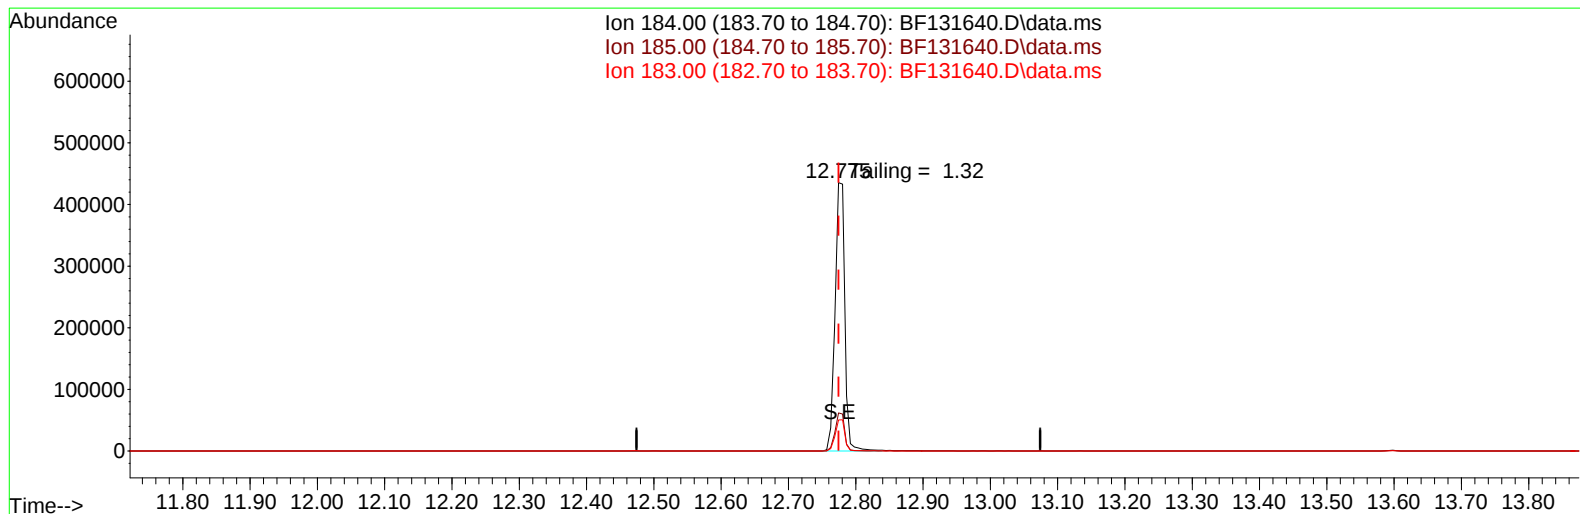

TIC: BF131640.D\data.ms

(77) Benzidine

12.775min (+ 0.000) 75840.19 ng

response 436891

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.20
183.00	11.60	11.57
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2022	BNA_F	<u>BF131640.D</u>
Compound Name	Response	Retention Time
DDT	238558	13.598
DDD	5509	13.298
DDE	441	12.957
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5950	244508	2.43

Instrument :
BNA_F
ClientSampleId :
DFTPP