
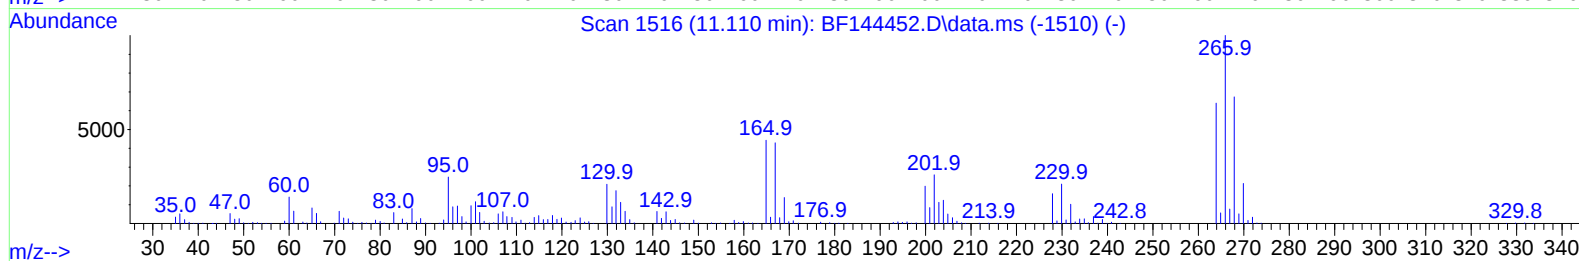
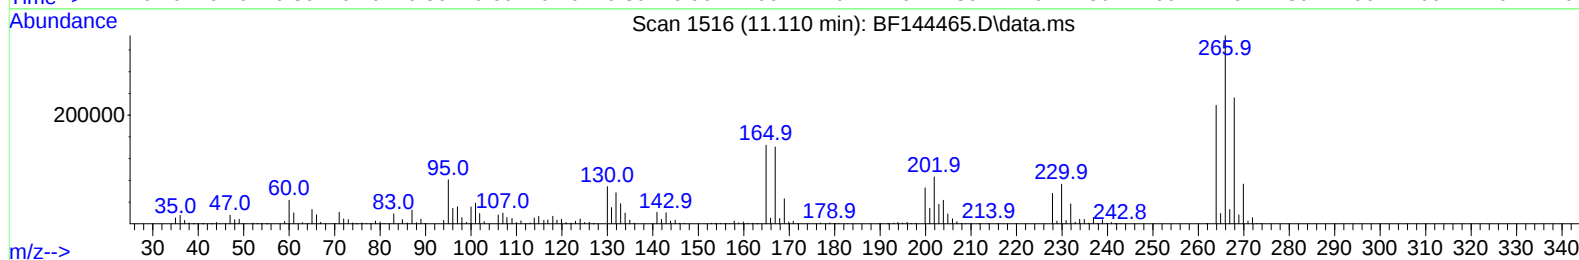


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121525\
Data File : BF144465.D
Acq On : 15 Dec 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 10:11:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

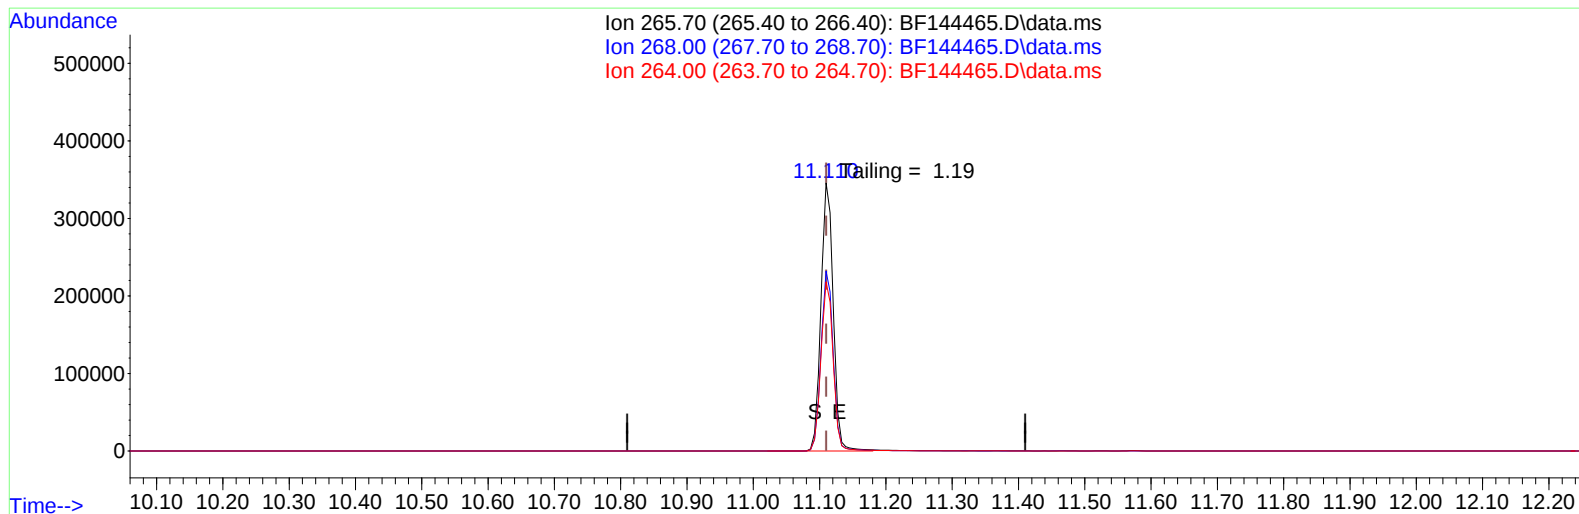

TIC: BF144465.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.000) 1131111.26 ng

response 448982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.30	67.00
264.00	64.00	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121525\
Data File : BF144465.D
Acq On : 15 Dec 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 10:11:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

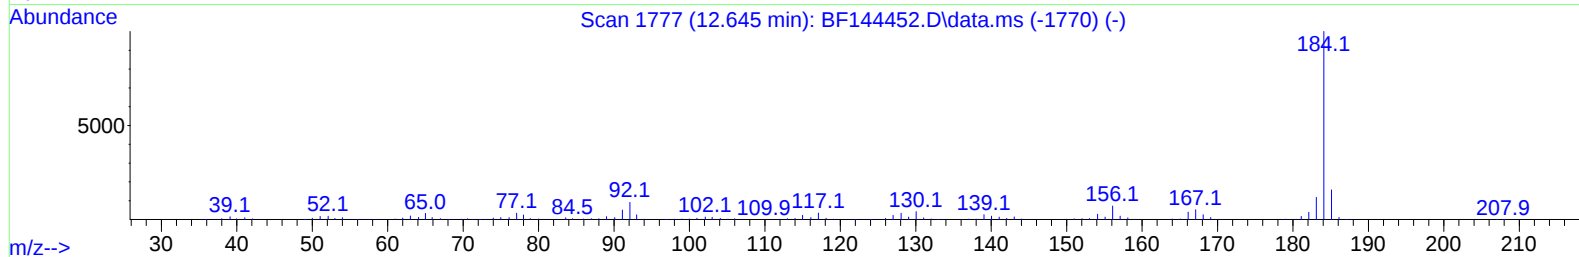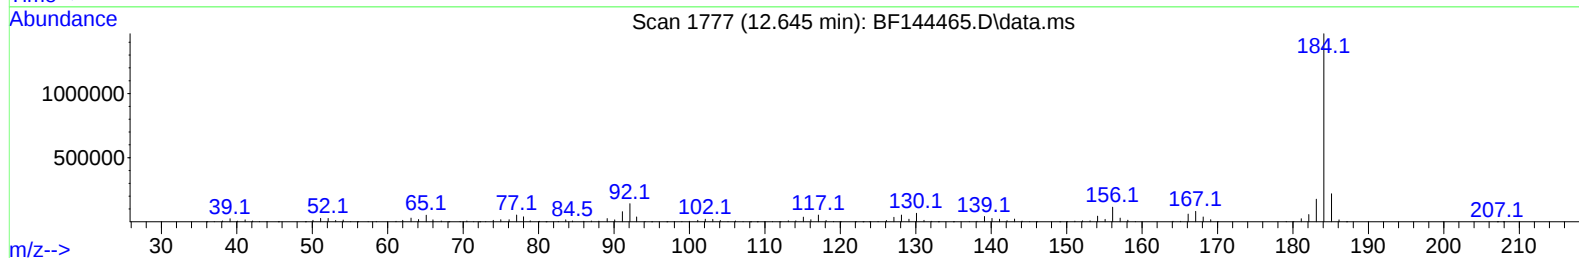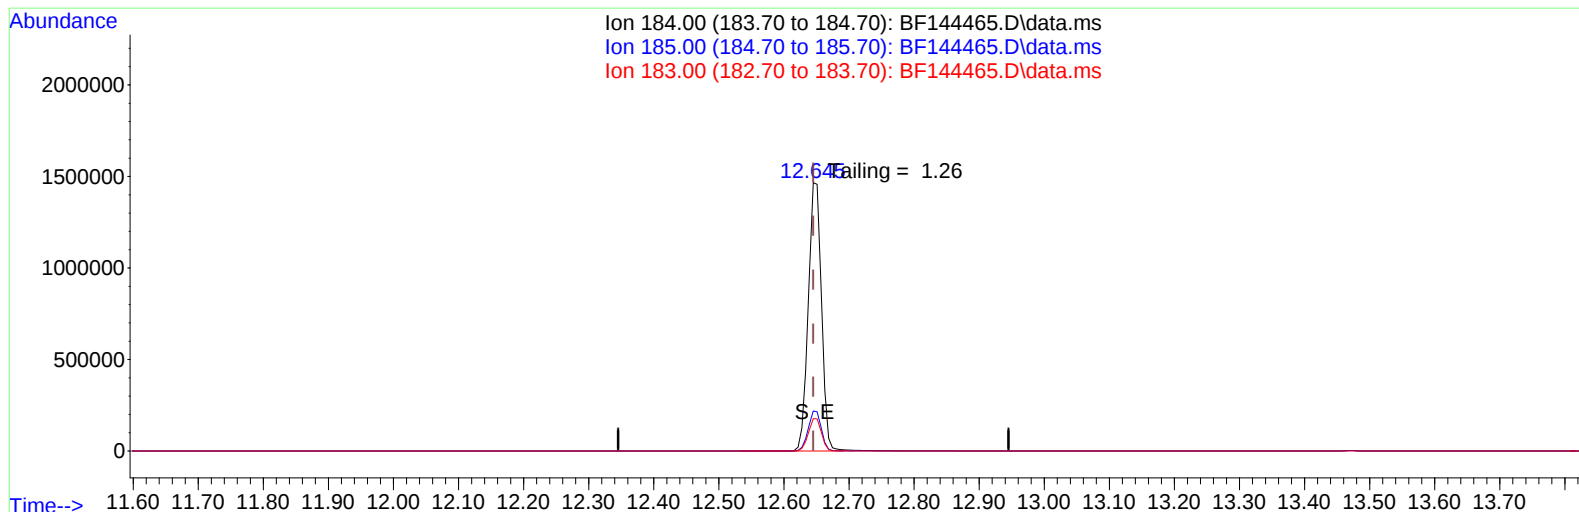

TIC: BF144465.D\data.ms

(77) Benzidine

12.645min (-0.000) 249322.52 ng

response 2077367

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.95
183.00	11.70	12.05
0.00	0.00	0.00