
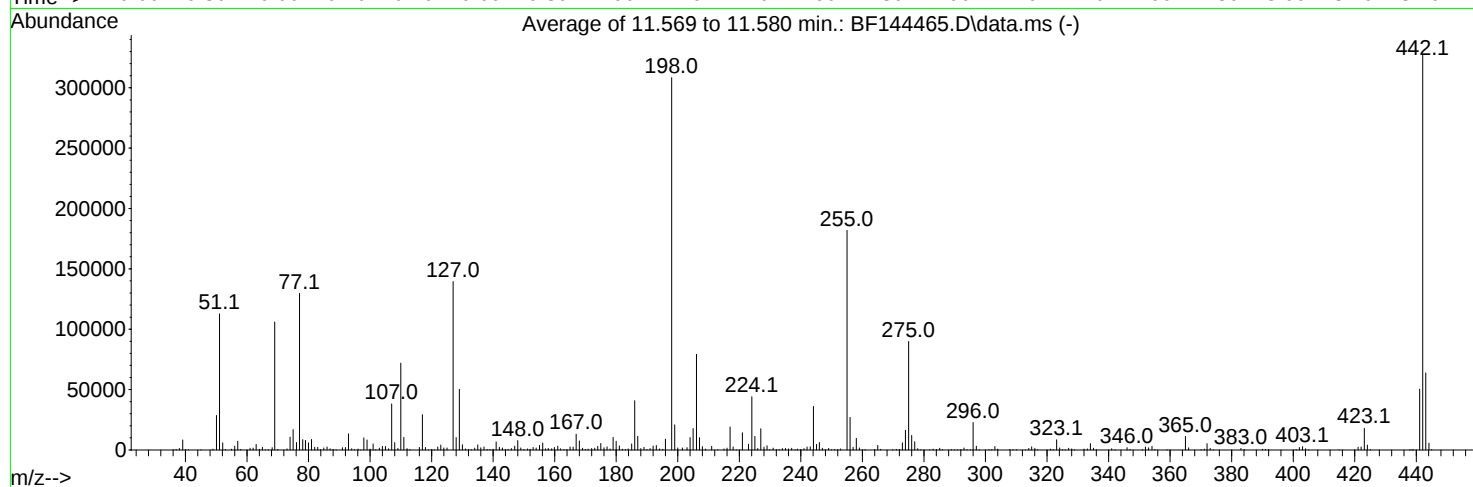


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121525\
Data File : BF144465.D
Acq On : 15 Dec 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 12 15:57:03 2025

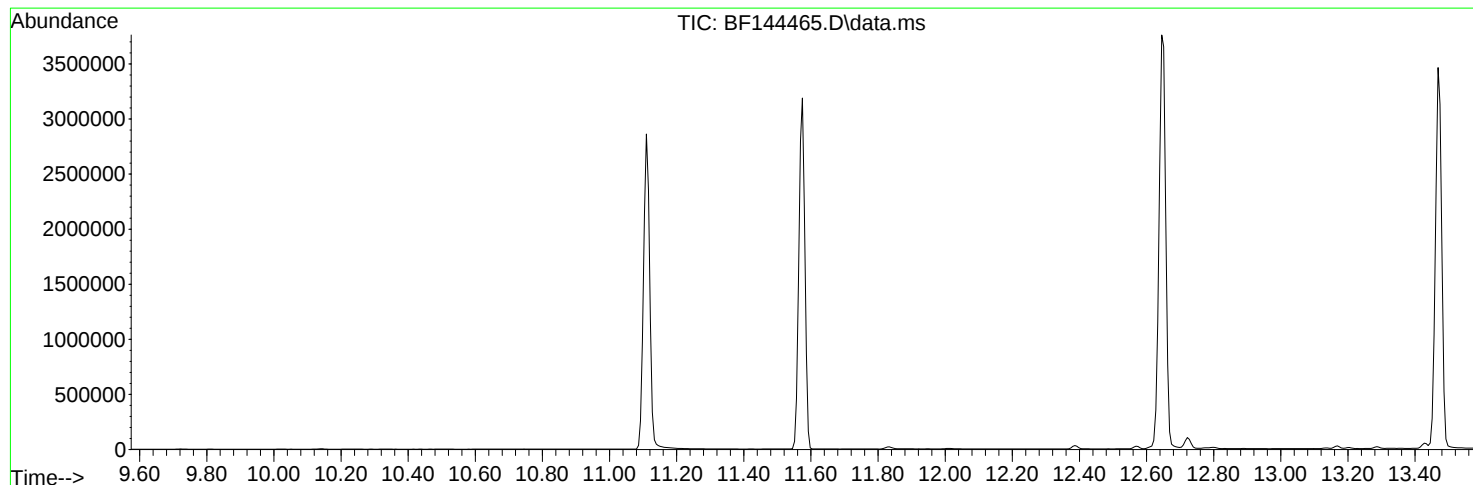




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1587

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1971	PASS
69	69	100	100	100.0	106013	PASS
70	69	0.00	2	0.5	532	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	308437	PASS
199	198	5	9	6.7	20735	PASS
365	198	1	100	3.6	11206	PASS
441	443	0.01	150	78.8	50352	PASS
442	442	100	100	100.0	327083	PASS
443	442	15	24	19.5	63888	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121525\
Data File : BF144465.D
Acq On : 15 Dec 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 15 10:11:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

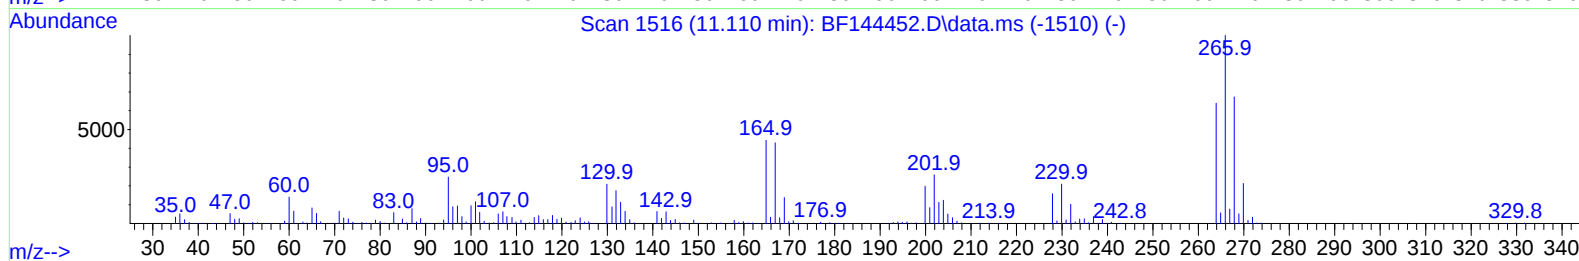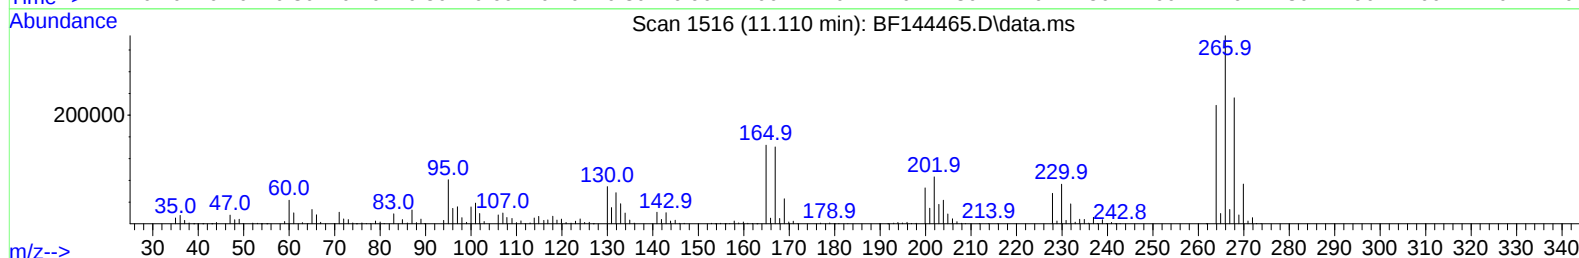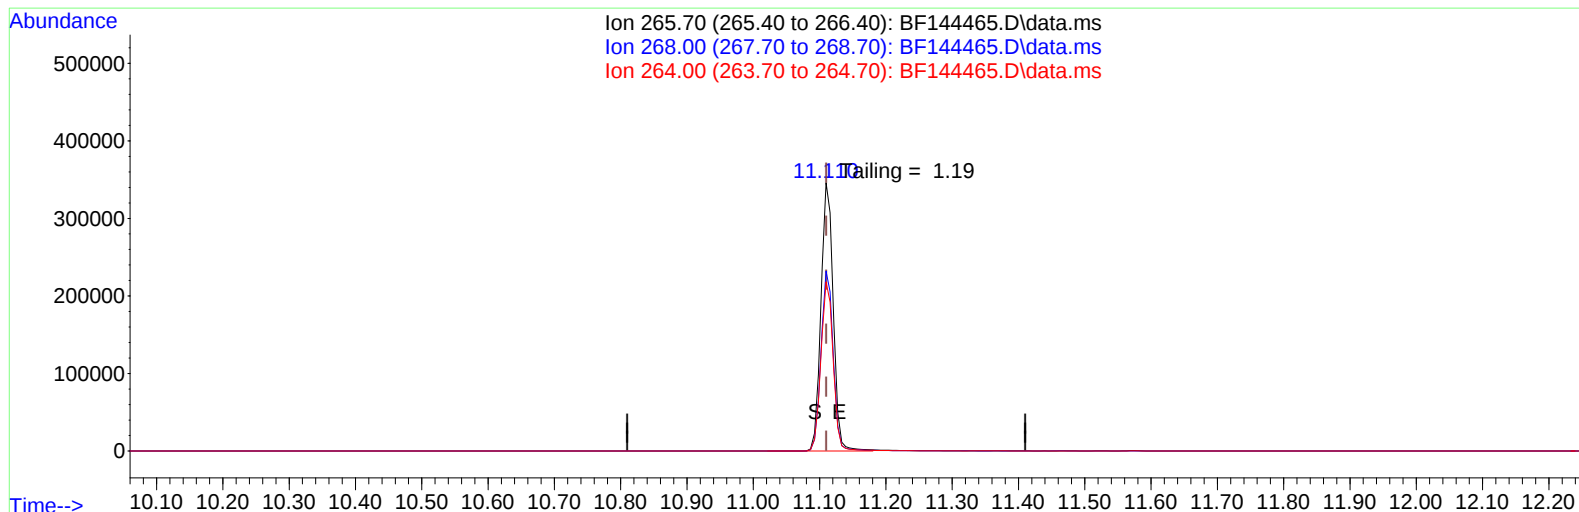

TIC: BF144465.D\data.ms

(70) Pentachlorophenol (C)

11.110min (-0.000) 1131111.26 ng




response 448982

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.30	67.00
264.00	64.00	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121525\
Data File : BF144465.D
Acq On : 15 Dec 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 15 10:11:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 12 15:57:03 2025
Response via : Initial Calibration

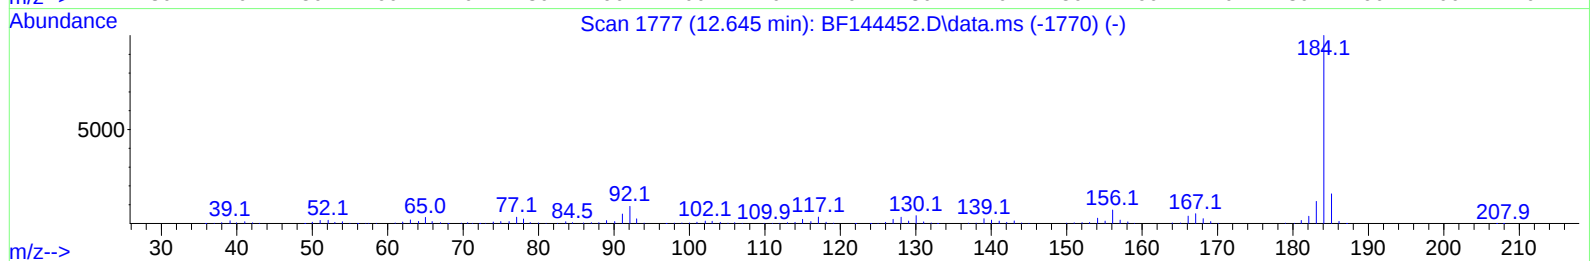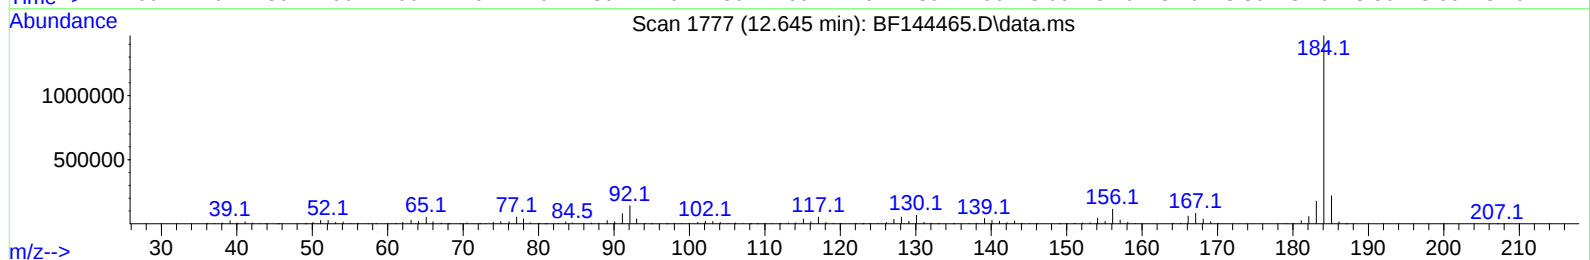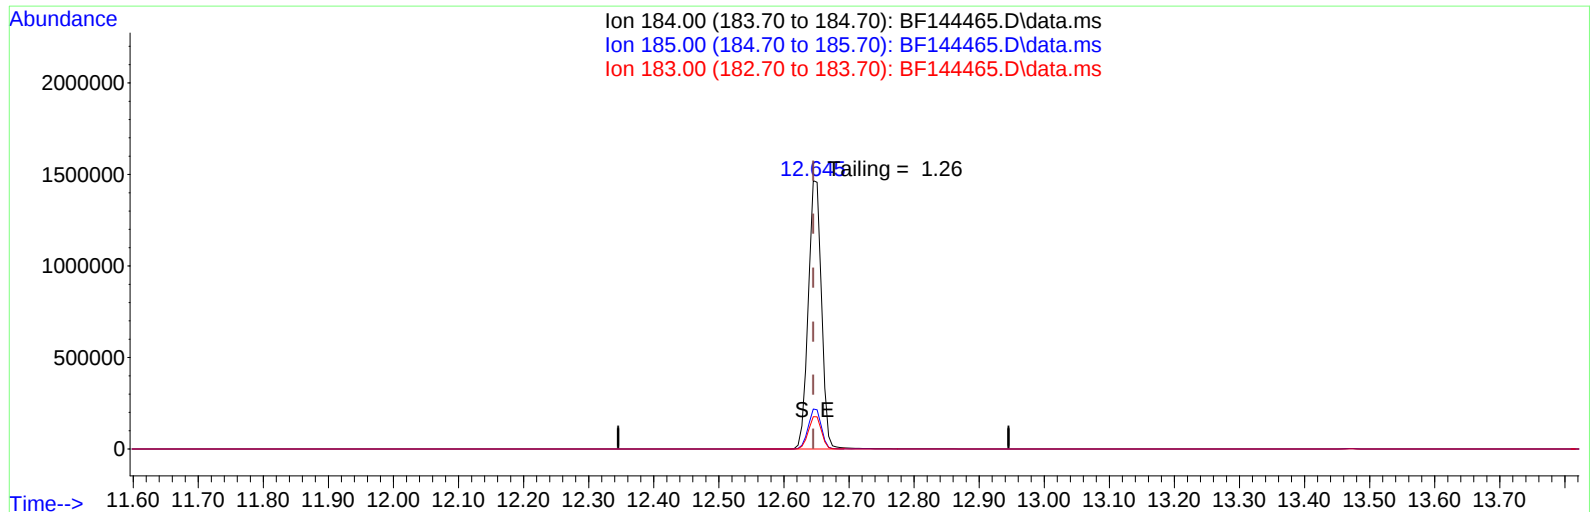

TIC: BF144465.D\data.ms

(77) Benzidine

12.645min (-0.000) 249322.52 ng

response 2077367

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.95
183.00	11.70	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2025	BNA_F	<u>BF144465.D</u>
Compound Name	Response	Retention Time
DDT	825993	13.469
DDD	8571	13.169
DDE	59	12.833
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8630	834623	1.03

Instrument :
BNA_F
ClientSampleId :
DFTPP