

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121618\
 Data File : BF111507.D
 Acq On : 16 Dec 2018 14:35
 Operator : JU/SJ
 Sample : J6373-10 10X
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OILY-WATER

Quant Time: Dec 17 06:57:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121418.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 14 13:26:17 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.79	152	252176	20.00	ng	0.00
21) Naphthalene-d8	8.07	136	1069991	20.00	ng	-0.01
39) Acenaphthene-d10	9.83	164	505108	20.00	ng	0.00
64) Phenanthrene-d10	11.30	188	830428	20.00	ng	-0.01
76) Chrysene-d12	13.94	240	542657	20.00	ng	-0.01
87) Perylene-d12	15.37	264	543999	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	55816	3.68	ng	-0.02
7) Phenol-d6	6.42	99	69018	3.42	ng	-0.02
23) Nitrobenzene-d5	7.34	82	140627	7.83	ng	-0.02
42) 2,4,6-Tribromophenol	10.61	330	52545	11.61	ng	-0.01
45) 2-Fluorobiphenyl	9.15	172	307659	9.41	ng	-0.01
79) Terphenyl-d14	12.89	244	227461	9.84	ng	-0.01
Target Compounds						
10) Phenol	6.43	94	484383	21.571	ng	89
22) Acetophenone	7.19	105	72990	3.056	ng	# 82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121618\
Data File : BF111507.D
Acq On : 16 Dec 2018 14:35
Operator : JU/SJ
Sample : J6373-10 10X
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OILY-WATER

Quant Time: Dec 17 06:57:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121418.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 14 13:26:17 2018
Response via : Initial Calibration

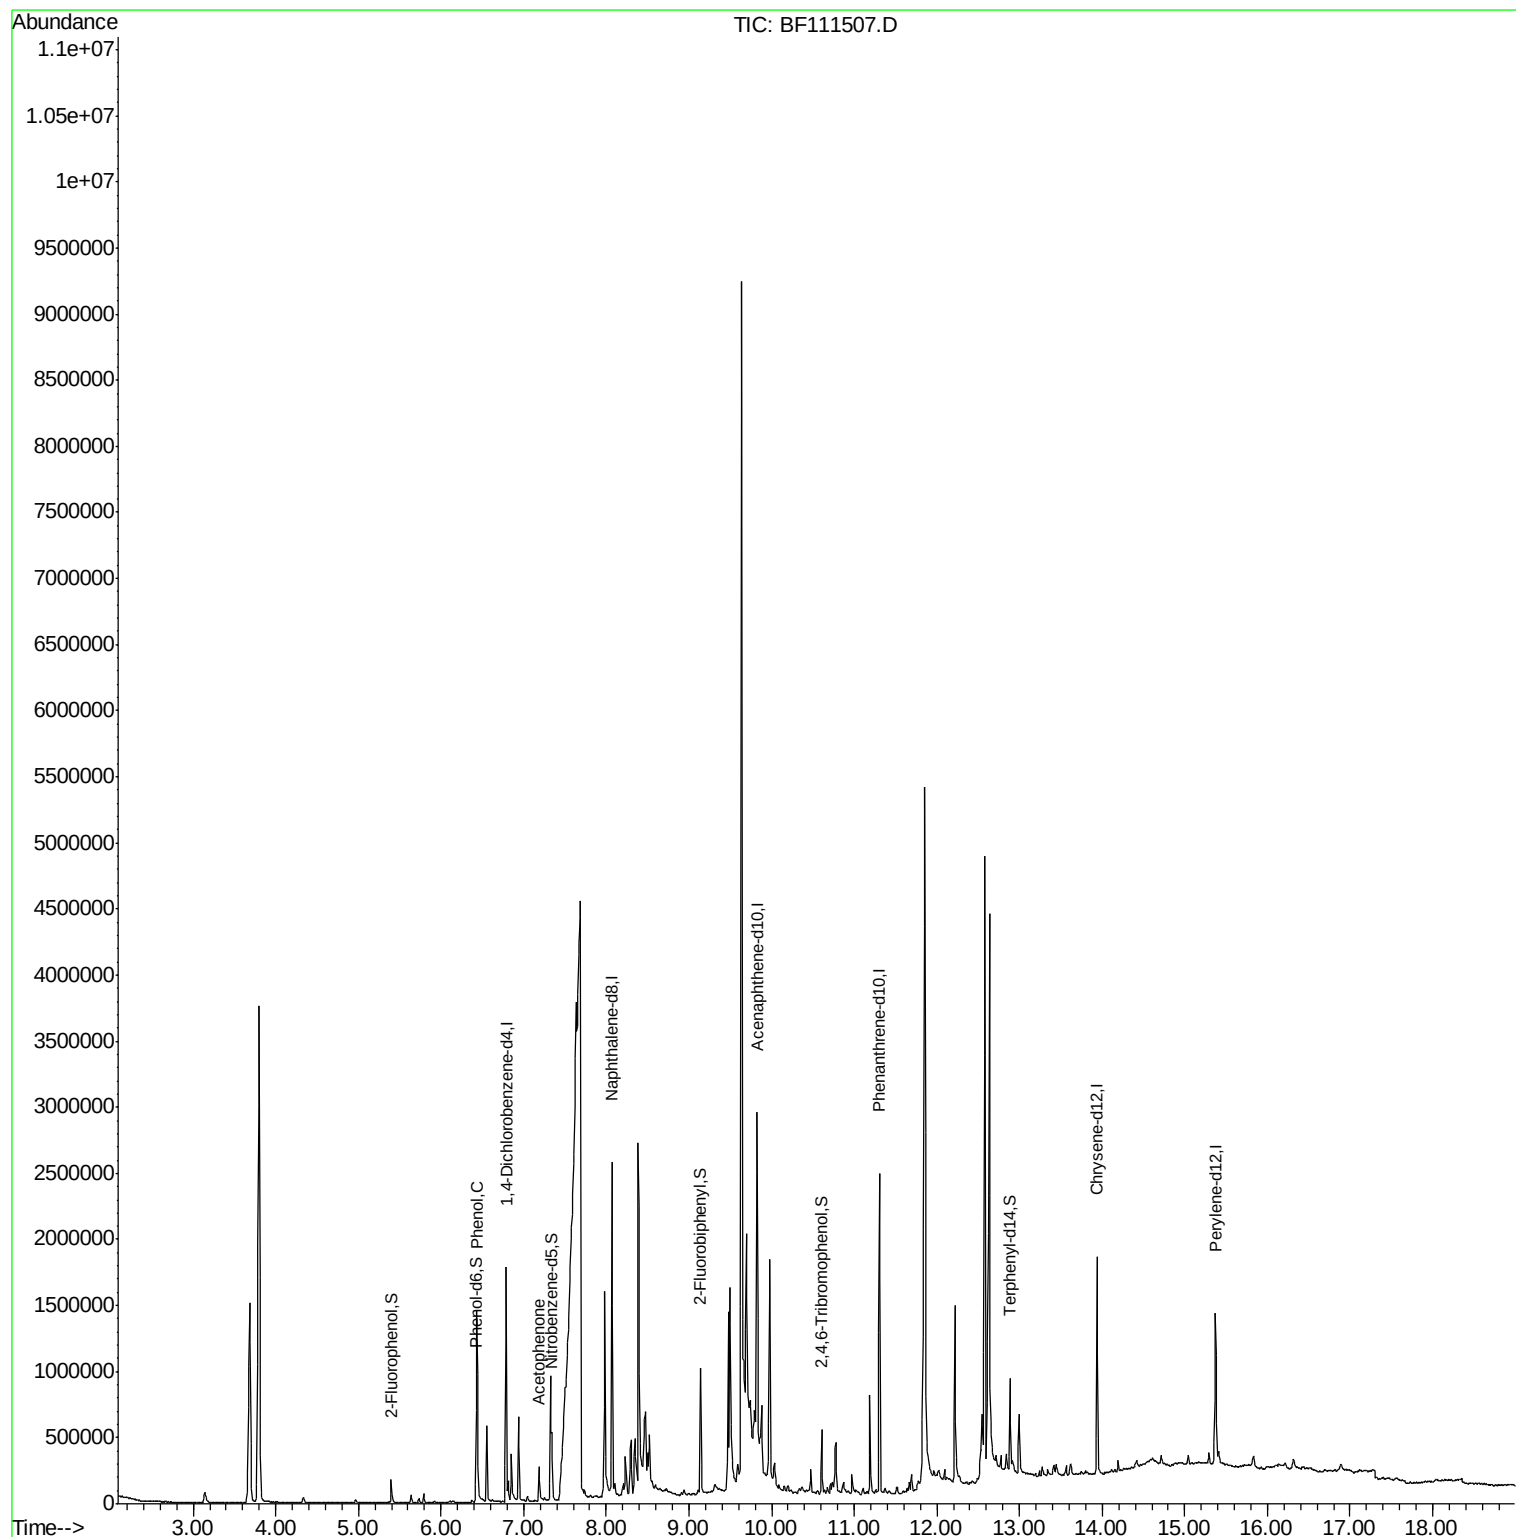

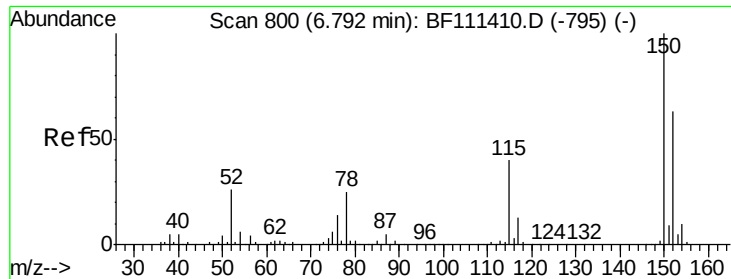


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.79 min Scan# 799
 Delta R.T. -0.01 min
 Lab File: BF111507.D
 Acq: 16 Dec 2018 14:35

Instrument :
 BNA_F
 ClientSampleId :
 OILY-WATER

Tot Ion	Ratio	Lower	Upper
152	100		
150	160.1	126.6	189.8
115	59.7	50.7	76.1



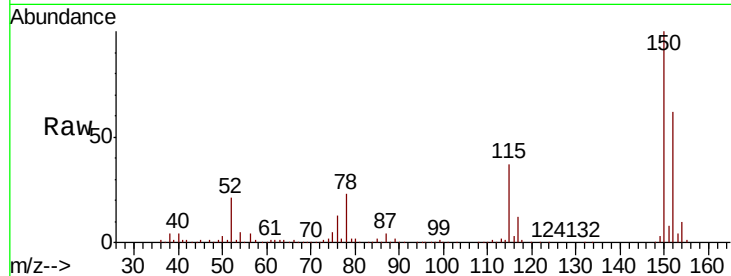


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

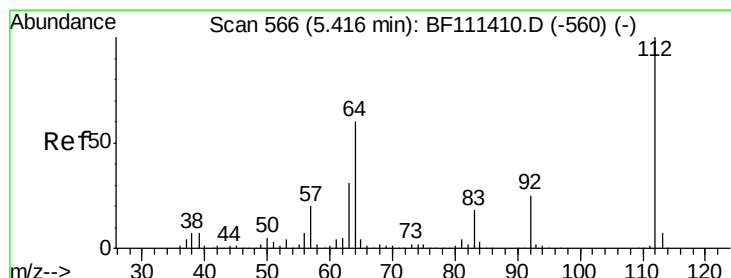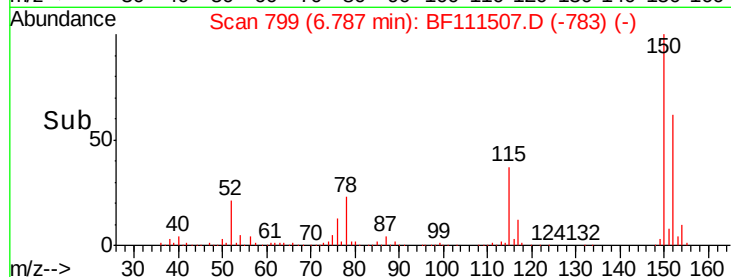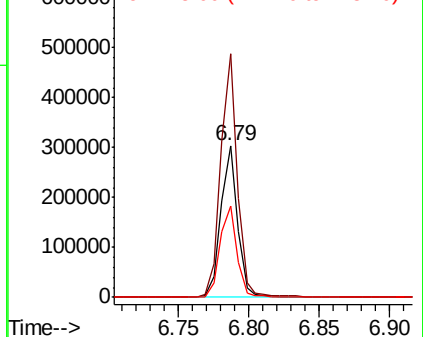

#5

2-Fluorophenol
 Concen: 3.683 ng
 RT: 5.40 min Scan# 563
 Delta R.T. -0.02 min
 Lab File: BF111507.D
 Acq: 16 Dec 2018 14:35

Tgt Ion	Ratio	Lower	Upper
112	100		
64	60.2	51.8	77.6
63	29.7	26.8	40.2


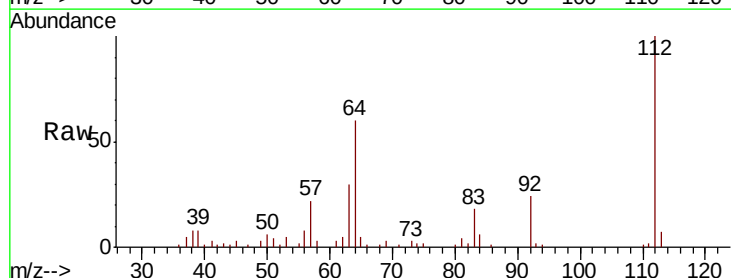



Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

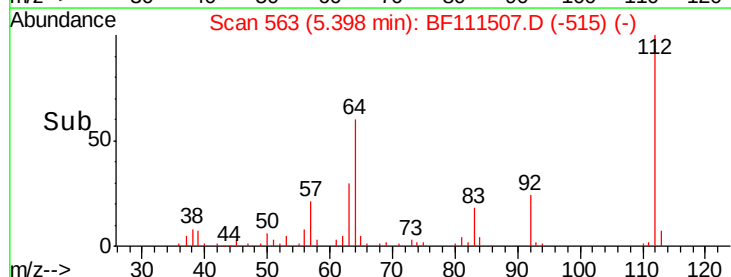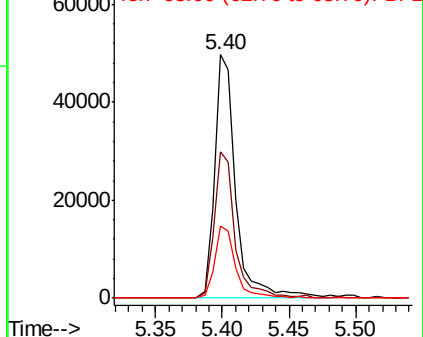

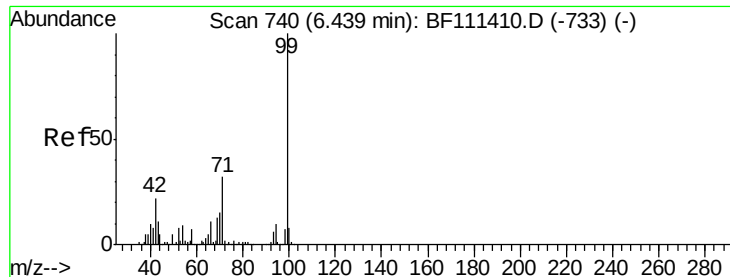

#7

Phenol-d6

Concen: 3.424 ng

RT: 6.42 min Scan# 737

Delta R.T. -0.02 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35

Instrument :

BNA_F

ClientSampleId :

OILY-WATER


Tot Ion: 99 Resp: 69018

Ion Ratio Lower Upper

99 100

42 18.4 17.4 26.0




71 28.5 26.1 39.1



Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

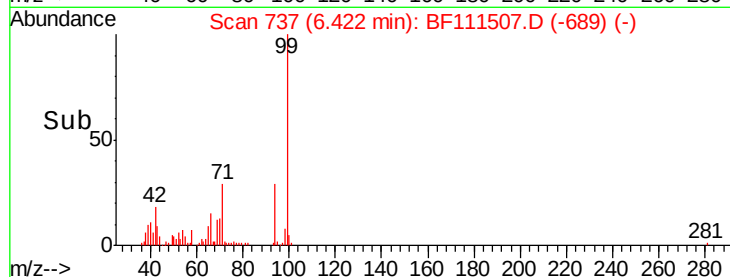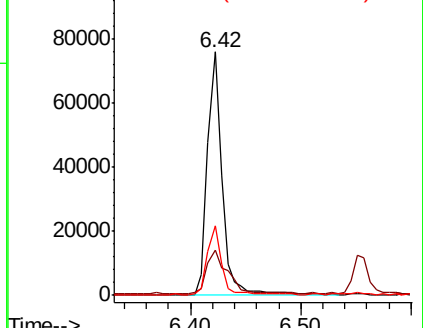

#10

Phenol

Concen: 21.571 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.02 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35


Tgt Ion: 94 Resp: 484383

Ion Ratio Lower Upper

94 100

65 26.3 11.7 51.7



66 33.6 21.0 61.0




Abundance Ion 94.00 (93.70 to 94.70): BF1

Ion 65.00 (64.70 to 65.70): BF1

Ion 66.00 (65.70 to 66.70): BF1



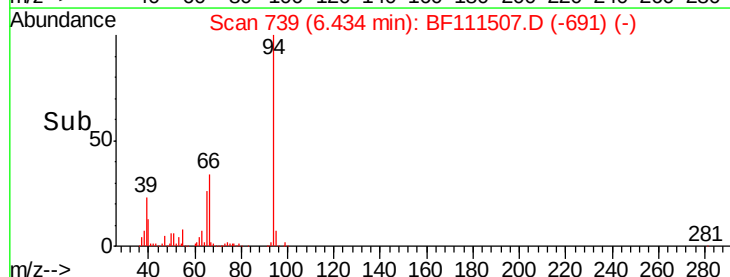
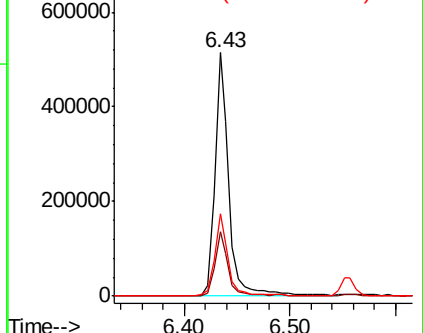


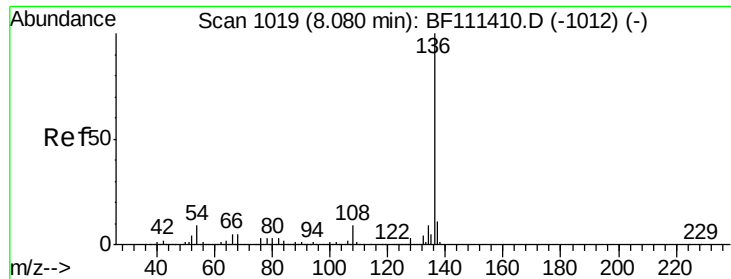

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.07 min Scan# 1017
Delta R.T. -0.01 min
Lab File: BF111507.D
Acq: 16 Dec 2018 14:35




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tot Ion:136	Resp: 1069991
Ion Ratio	Lower Upper
136 100	
137 11.1	9.1 13.7
54 9.0	7.7 11.5
68 5.7	4.9 7.3

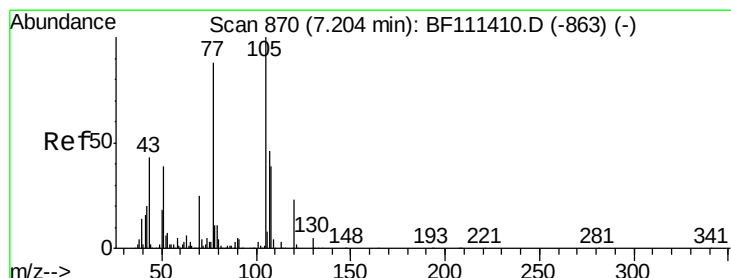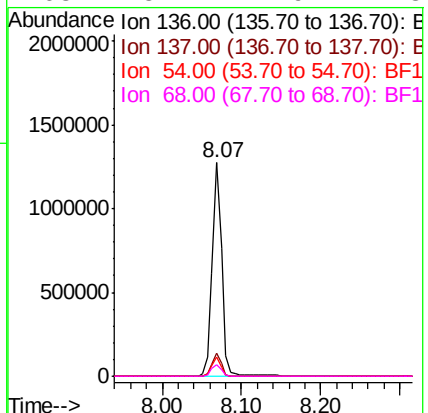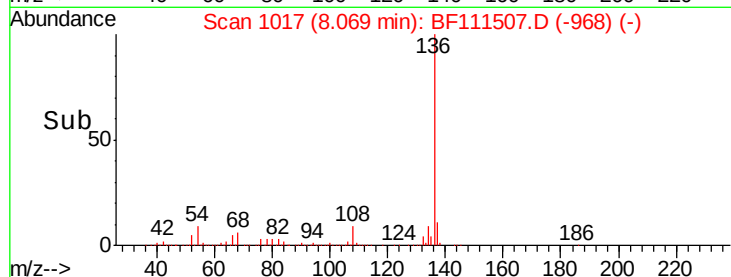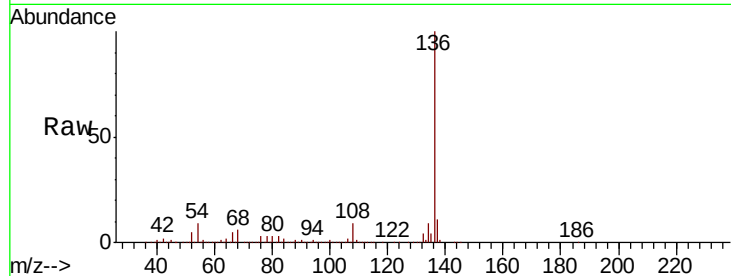

#22
Acetophenone
Concen: 3.056 ng
RT: 7.19 min Scan# 867
Delta R.T. -0.02 min
Lab File: BF111507.D
Acq: 16 Dec 2018 14:35

Tgt	Ion:105	Resp:	72990
Ion	Ratio	Lower	Upper
105	100		
71	0.7	3.1	4.7#
51	29.0	36.6	54.8#
120	20.0	18.2	27.4


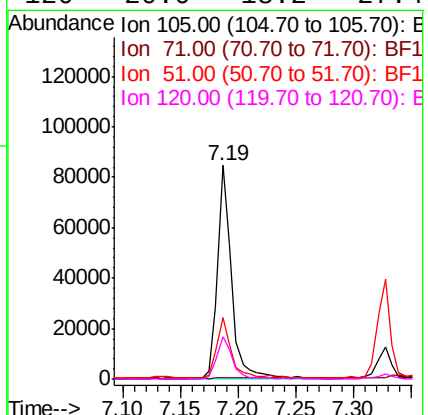
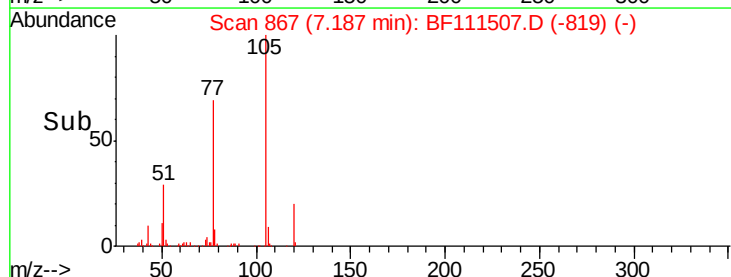
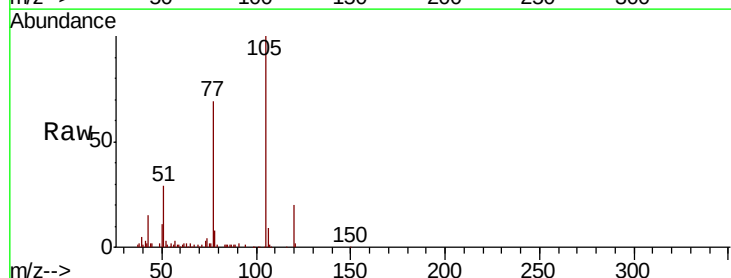


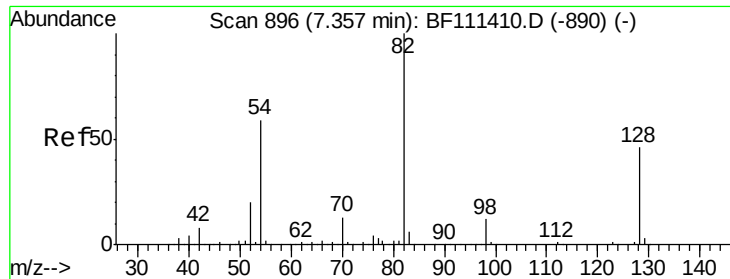

#23
Nitrobenzene-d5
Concen: 7.826 ng
RT: 7.34 min Scan# 893
Delta R.T. -0.02 min
Lab File: BF111507.D
Acq: 16 Dec 2018 14:35




Instrument :
BNA_F
ClientSampleId :
OILY-WATER


Tot Ion: 82 Resp: 140627
Ion Ratio Lower Upper
82 100
128 45.1 37.4 56.2
54 54.5 47.6 71.4

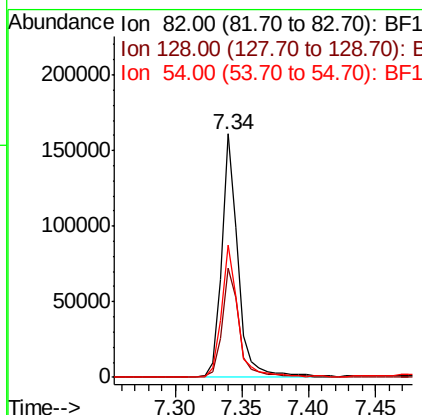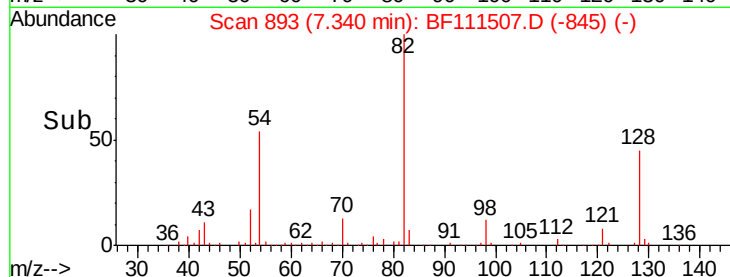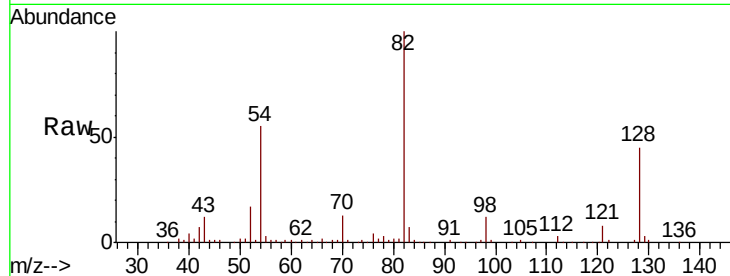

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.83 min Scan# 1316
Delta R.T. -0.01 min
Lab File: BF111507.D
Acq: 16 Dec 2018 14:35

Tgt Ion:164 Resp: 505108
Ion Ratio Lower Upper
164 100
162 100.3 81.4 122.0
160 44.4 35.7 53.5

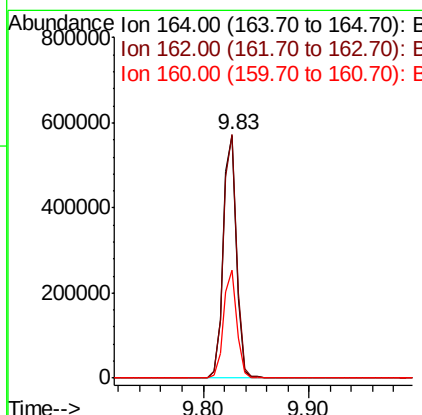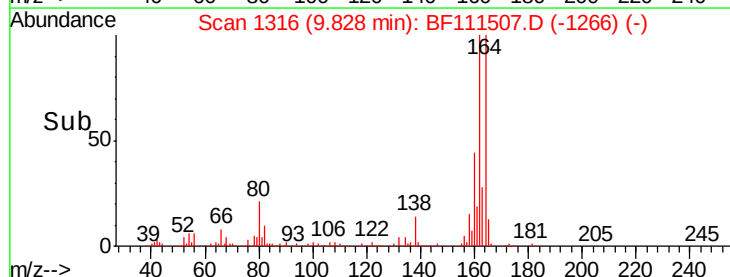


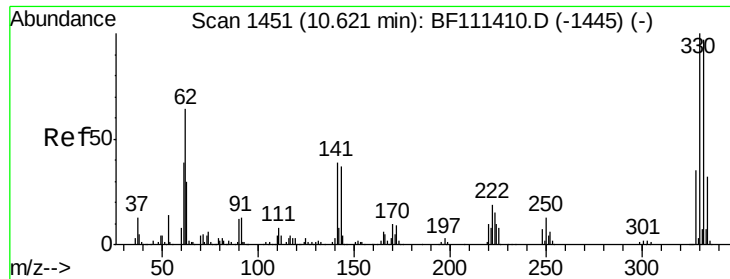




#42
 2,4,6-Tribromophenol
 Concen: 11.613 ng
 RT: 10.61 min Scan# 1449
 Delta R.T. -0.01 min
 Lab File: BF111507.D
 Acq: 16 Dec 2018 14:35

Instrument :
 BNA_F
 ClientSampleId :
 OILY-WATER

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.6	76.0	114.0
141	36.2	31.0	46.6




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

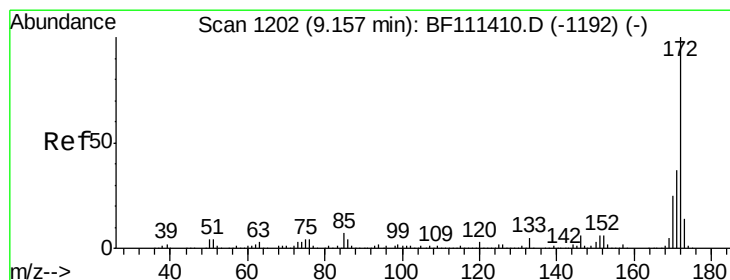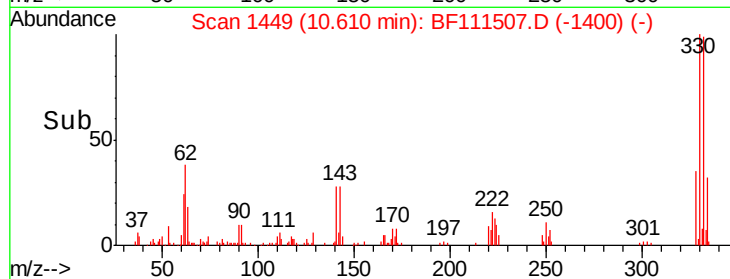
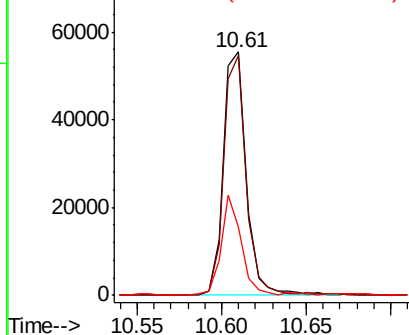



#45
 2-Fluorobiphenyl
 Concen: 9.408 ng
 RT: 9.15 min Scan# 1200
 Delta R.T. -0.01 min
 Lab File: BF111507.D
 Acq: 16 Dec 2018 14:35

Tgt Ion	Ratio	Lower	Upper
172	100		
171	34.7	33.0	49.4
170	22.6	22.3	33.5

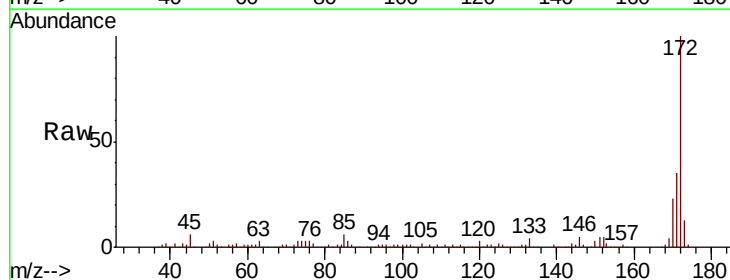

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

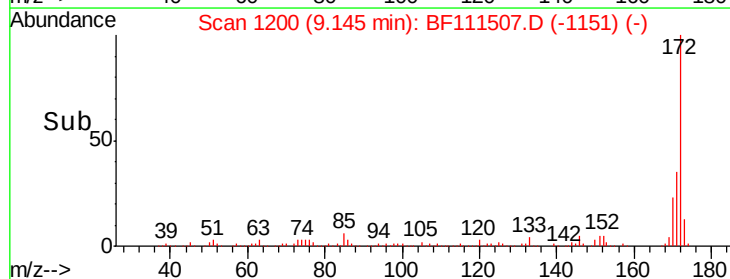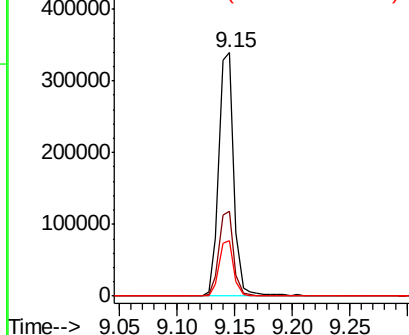

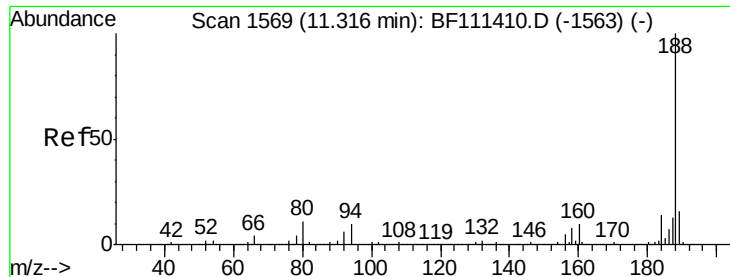

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.30 min Scan# 1567

Delta R.T. -0.01 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35

Instrument :

BNA_F

ClientSampleId :

OILY-WATER


Tot Ion:188 Resp: 830428

Ion Ratio Lower Upper

188 100

94 11.0 9.6 14.4




80 12.7 9.8 14.6

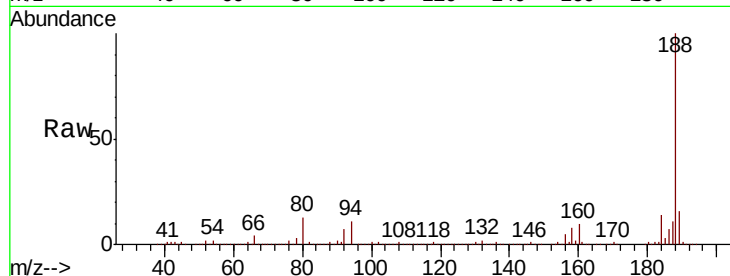

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

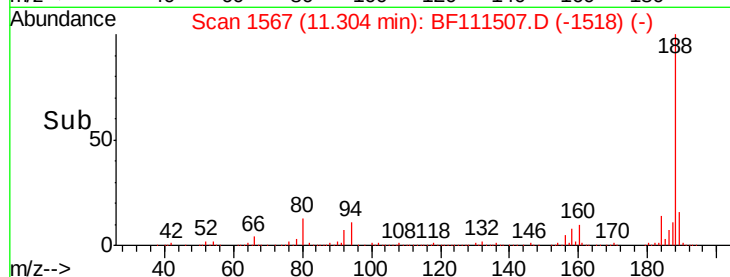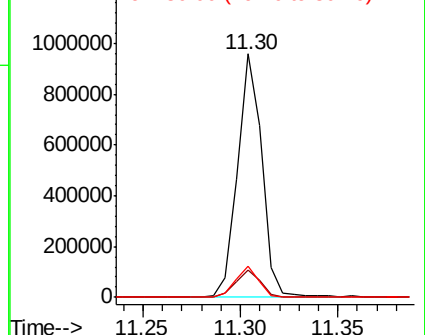

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.94 min Scan# 2015

Delta R.T. -0.01 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35


Tgt Ion:240 Resp: 542657

Ion Ratio Lower Upper

240 100

120 13.8 12.2 18.2



236 24.2 20.2 30.2




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

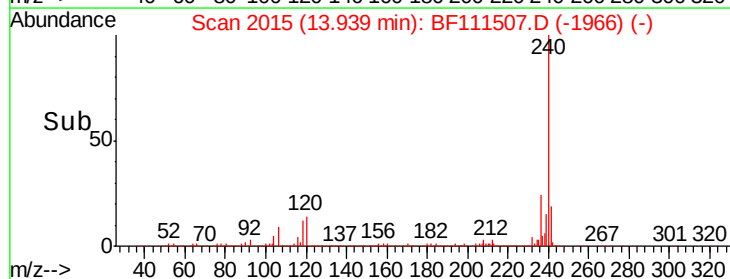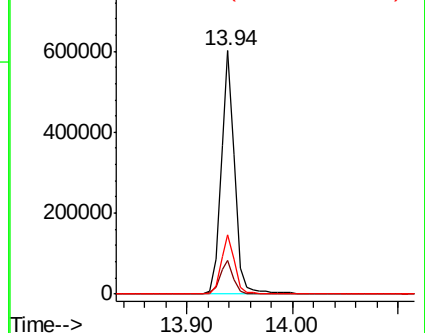

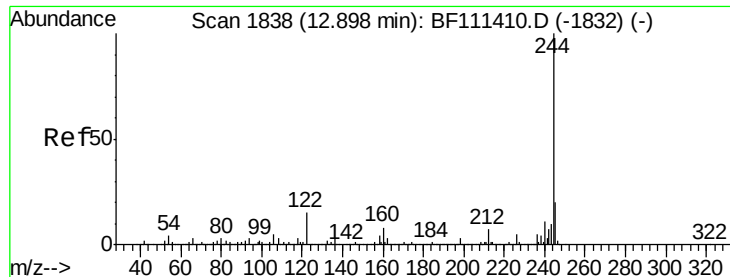

#79

Terphenyl-d14

Concen: 9.843 ng

RT: 12.89 min Scan# 1836

Delta R.T. -0.01 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35

Instrument :

BNA_F

ClientSampleId :

OILY-WATER


Tot Ion:244 Resp: 227461

Ion Ratio Lower Upper

244 100

212 6.2 5.7 8.5




122 12.1 13.1 19.7#



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

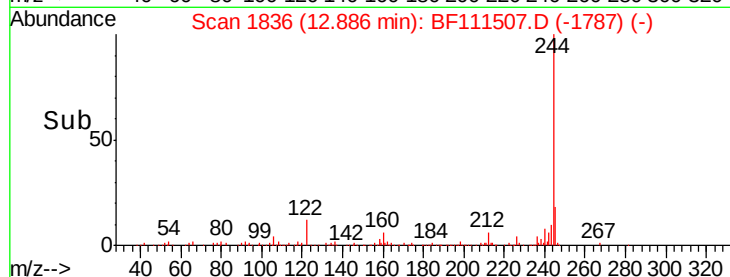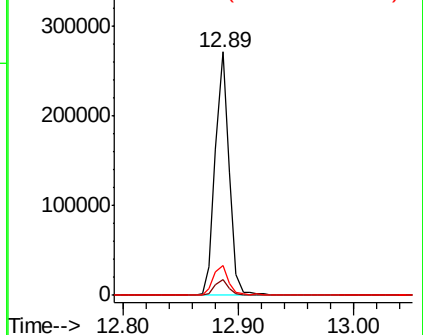

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.37 min Scan# 2259

Delta R.T. -0.01 min

Lab File: BF111507.D

Acq: 16 Dec 2018 14:35


Tgt Ion:264 Resp: 543999

Ion Ratio Lower Upper

264 100

260 23.3 18.3 27.5

265 21.2 17.7 26.5



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

