


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121618\
 Data File : BF111504.D
 Acq On : 16 Dec 2018 11:51
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

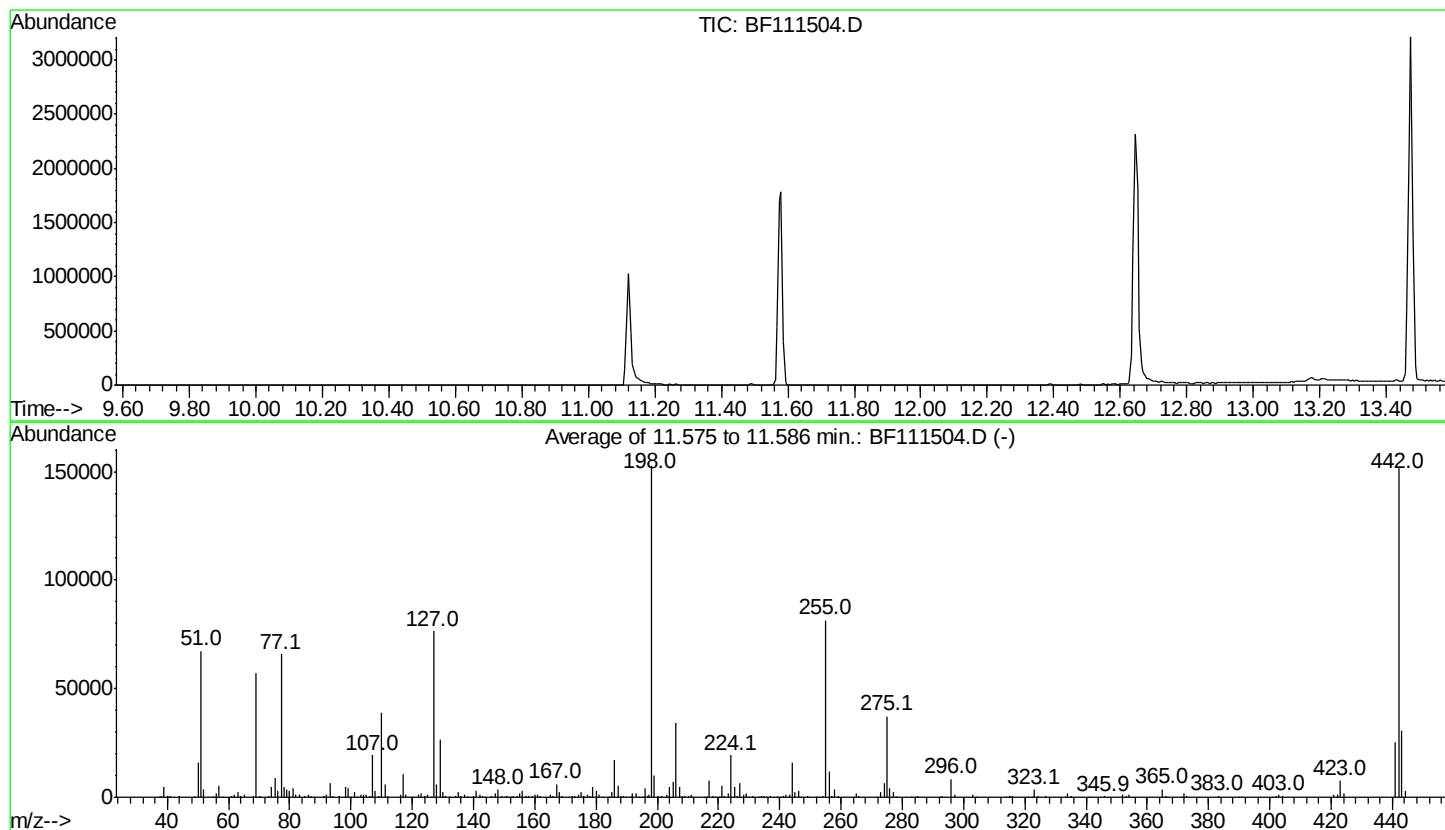

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.1	67354	PASS
68	69	0.00	2	1.2	696	PASS
69	198	0.00	100	37.4	57119	PASS
70	69	0.00	2	0.6	323	PASS
127	198	10	80	50.1	76537	PASS
197	198	0.00	2	0.8	1192	PASS
198	198	100	100	100.0	152760	PASS
199	198	5	9	6.5	9983	PASS
275	198	10	60	24.5	37430	PASS
365	198	1	100	2.5	3823	PASS
441	198	0.01	100	16.6	25424	PASS
442	198	50	100	99.3	151680	PASS
443	442	15	24	20.1	30474	PASS