

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121622\
 Data File : BF131677.D
 Acq On : 16 Dec 2022 20:56
 Operator : CG\JU
 Sample : N6037-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RB-24-(7-9)

Quant Time: Dec 17 03:58:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 16 01:44:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.881	152	58798	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	205514	20.000	ng	0.00
39) Acenaphthene-d10	9.928	164	116283	20.000	ng	-0.01
64) Phenanthrene-d10	11.428	188	225728	20.000	ng	0.00
76) Chrysene-d12	14.074	240	133952	20.000	ng	# 0.00
86) Perylene-d12	15.580	264	139380	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.493	112	409914	116.306	ng	0.00
7) Phenol-d6	6.510	99	536078	116.071	ng	0.00
23) Nitrobenzene-d5	7.445	82	368406	67.773	ng	0.00
42) 2,4,6-Tribromophenol	10.728	330	139507	107.983	ng	0.00
45) 2-Fluorobiphenyl	9.251	172	630434	68.359	ng	0.00
79) Terphenyl-d14	13.022	244	739286	75.688	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121622\
Data File : BF131677.D
Acq On : 16 Dec 2022 20:56
Operator : CG\JU
Sample : N6037-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RB-24-(7-9)

Quant Time: Dec 17 03:58:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration




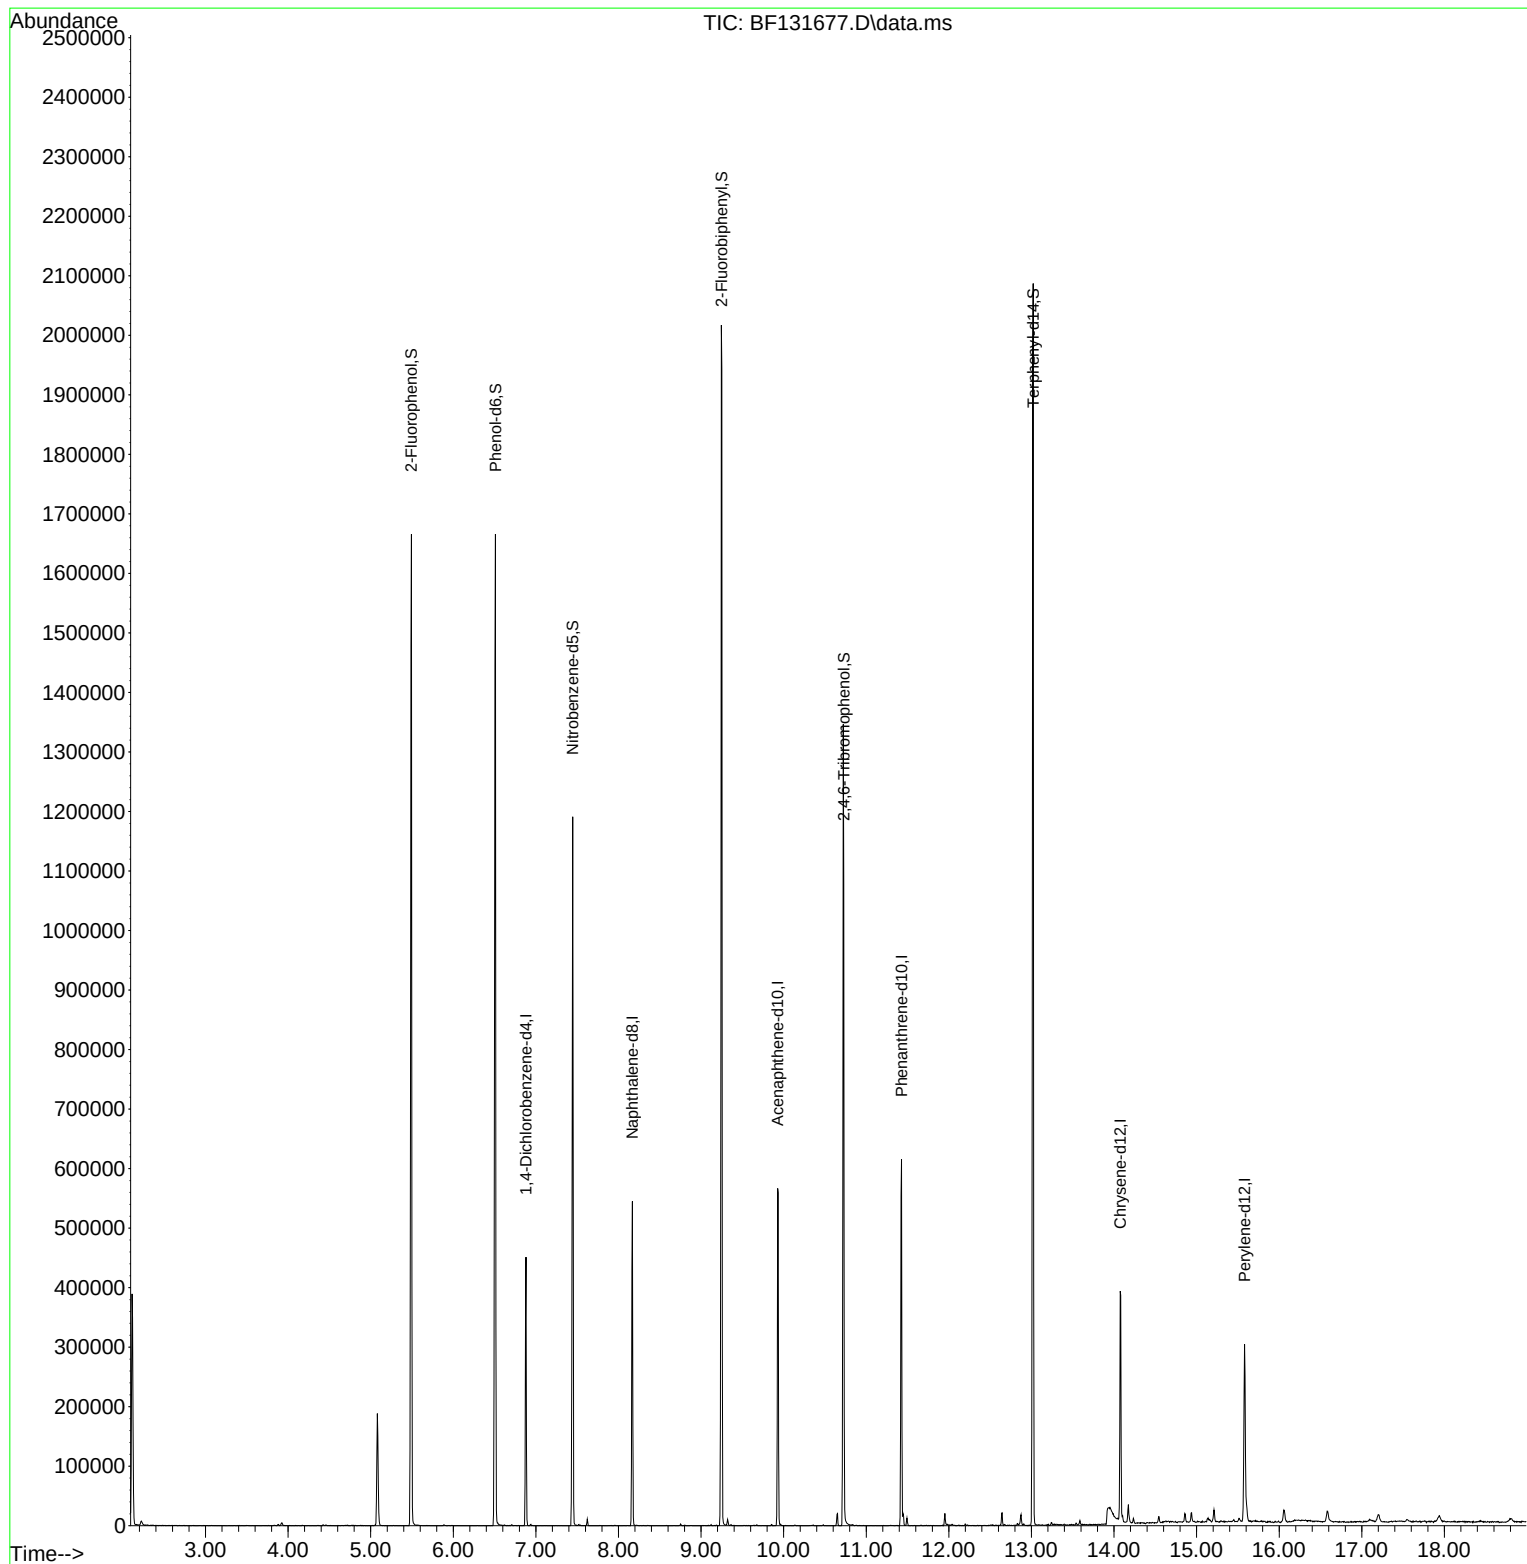


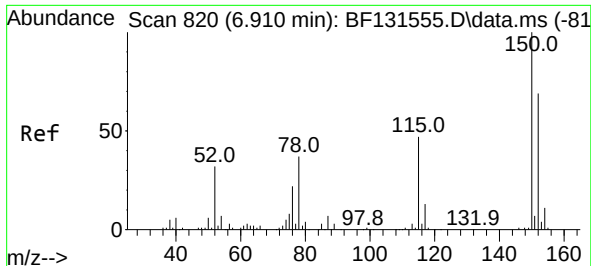

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.881 min Scan# 81
Delta R.T. -0.000 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56




Instrument :
BNA_F
ClientSampleId :
RB-24-(7-9)


Tgt Ion:152 Resp: 58798
Ion Ratio Lower Upper
152 100
150 147.0 116.7 175.1
115 64.6 54.6 82.0

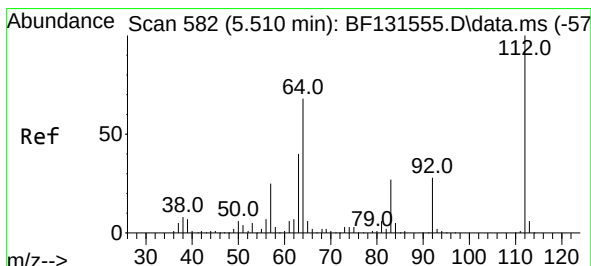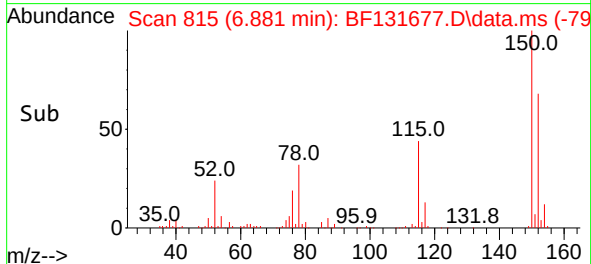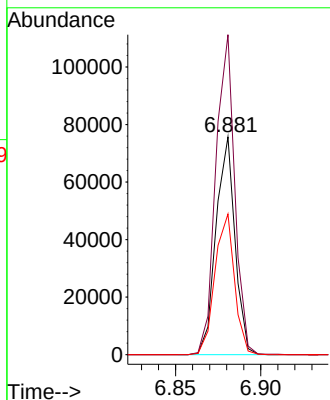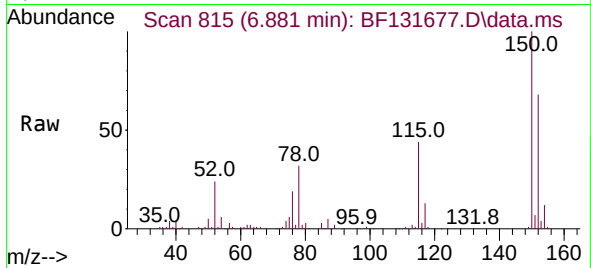

#5
2-Fluorophenol
Concen: 116.306 ng
RT: 5.493 min Scan# 579
Delta R.T. 0.000 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56

Tgt Ion:112 Resp: 409914
Ion Ratio Lower Upper
112 100
64 63.1 54.5 81.7
63 35.0 31.9 47.9


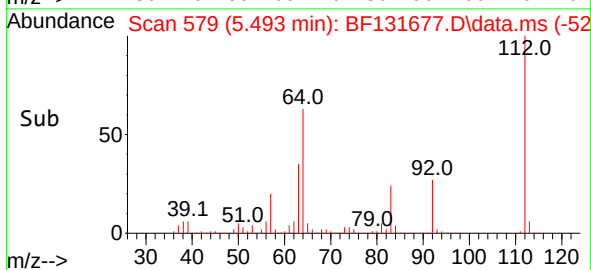
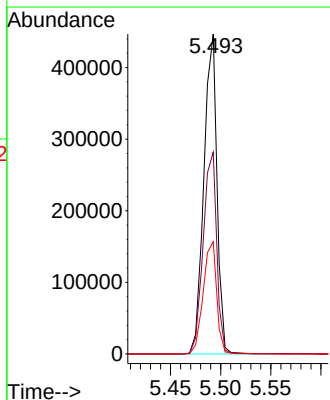
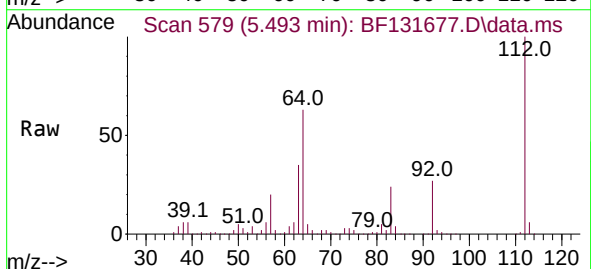


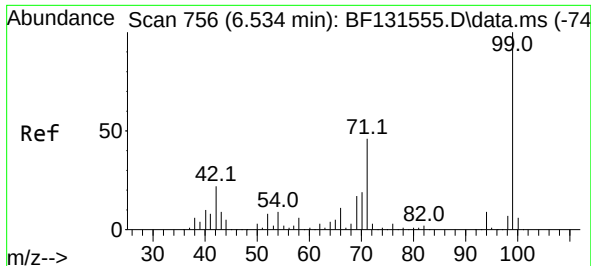

#7
Phenol-d6
Concen: 116.071 ng
RT: 6.510 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56




Instrument :
BNA_F
ClientSampleId :
RB-24-(7-9)


Tgt Ion: 99 Resp: 536078
Ion Ratio Lower Upper
99 100
42 18.4 17.9 26.9
71 41.9 37.2 55.8

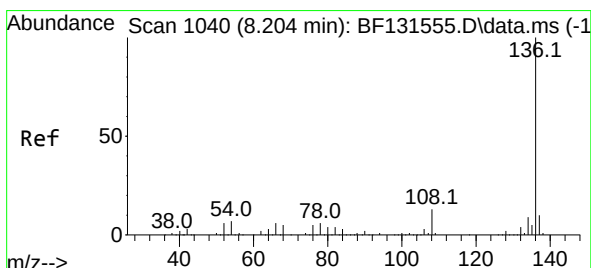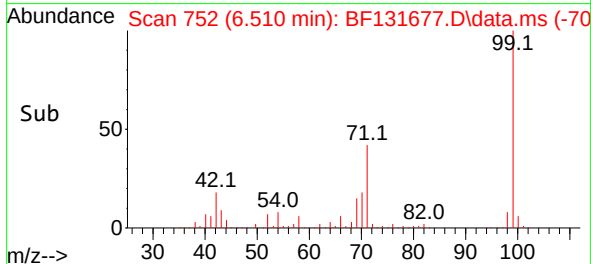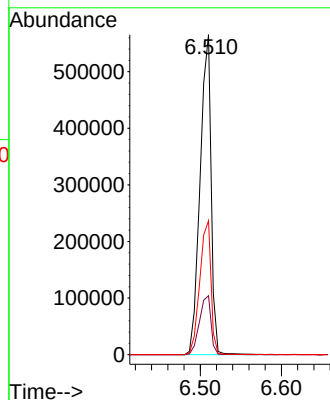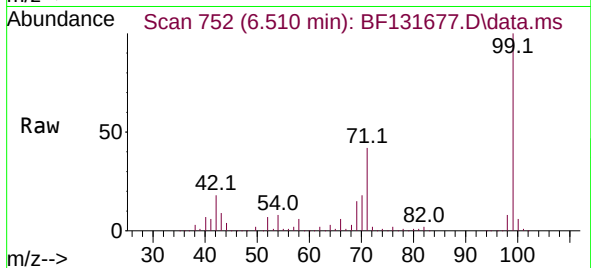

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56

Tgt Ion: 136 Resp: 205514
Ion Ratio Lower Upper
136 100
137 10.5 8.1 12.1
54 7.6 6.0 9.0
68 5.5 3.8 5.8

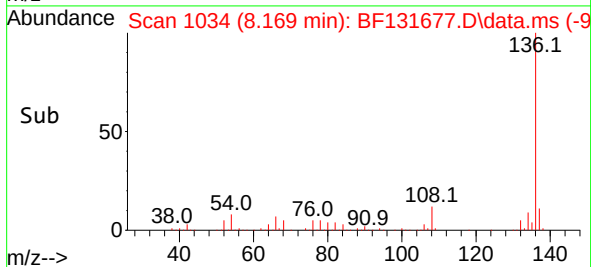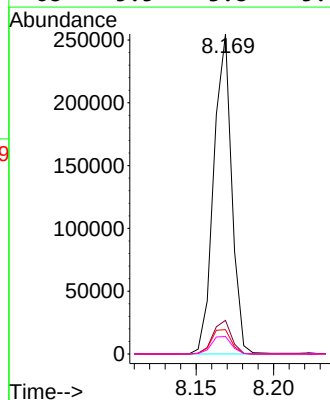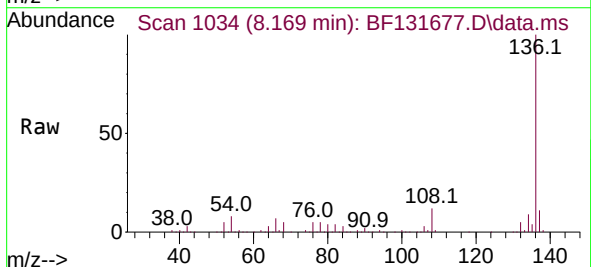

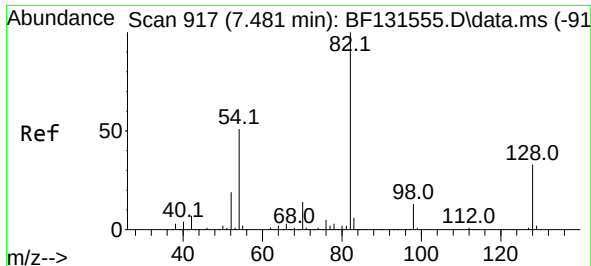

#23

Nitrobenzene-d5

Concen: 67.773 ng

RT: 7.445 min Scan# 91

Delta R.T. -0.006 min

Lab File: BF131677.D

Acq: 16 Dec 2022 20:56

Instrument :

BNA_F

ClientSampleId :

RB-24-(7-9)





Tgt Ion: 82 Resp: 368406

Ion Ratio Lower Upper

82 100

128 34.7 26.1 39.1

54 46.9 40.6 60.8

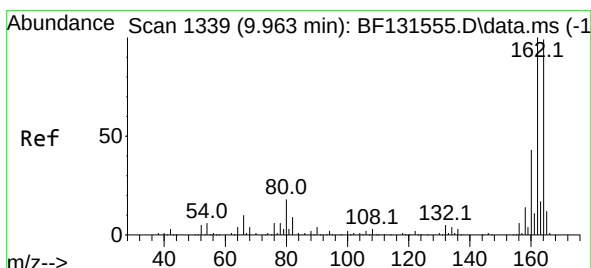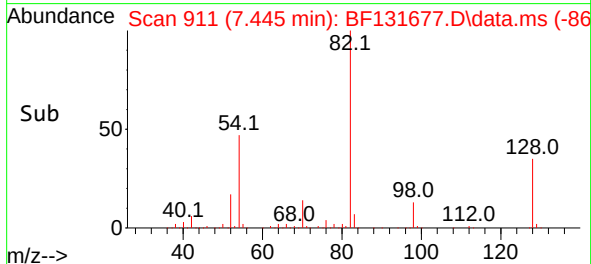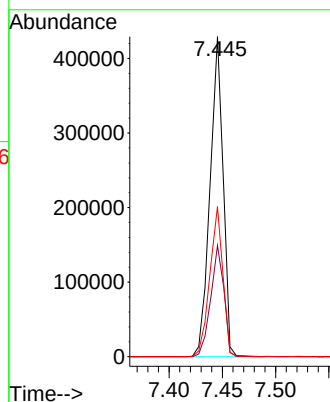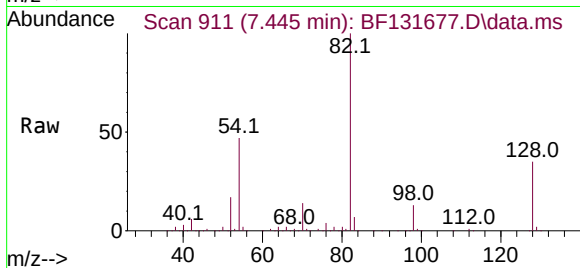

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.928 min Scan# 1333

Delta R.T. -0.012 min

Lab File: BF131677.D

Acq: 16 Dec 2022 20:56




Tgt Ion:164 Resp: 116283


Ion Ratio Lower Upper

164 100

162 102.3 81.0 121.6

160 43.6 35.0 52.6

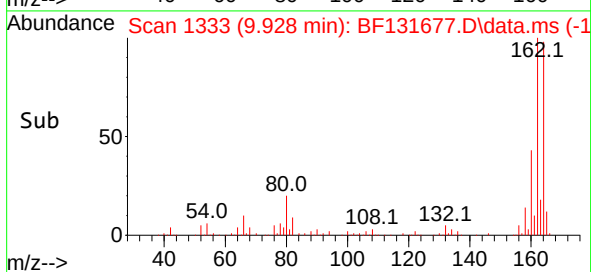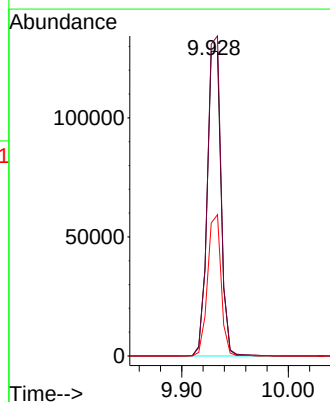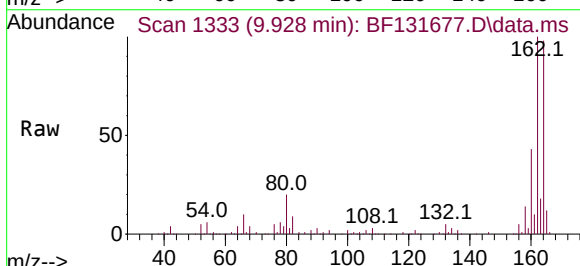

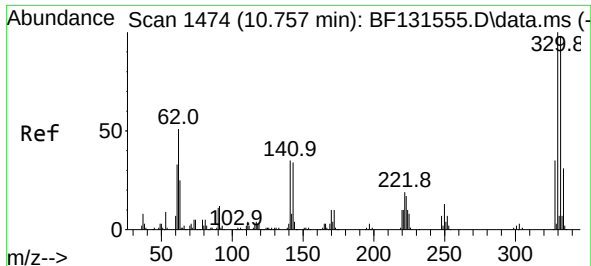

#42

2,4,6-Tribromophenol

Concen: 107.983 ng

RT: 10.728 min Scan# 1469

Delta R.T. -0.006 min

Lab File: BF131677.D

Acq: 16 Dec 2022 20:56

Instrument :

BNA_F

ClientSampleId :

RB-24-(7-9)





Tgt Ion:330 Resp: 139507

Ion Ratio Lower Upper

330 100

332 97.5 78.3 117.5

141 39.2 32.6 49.0

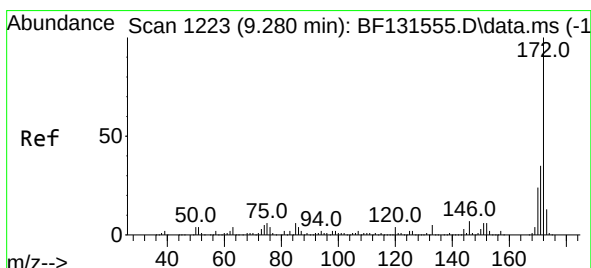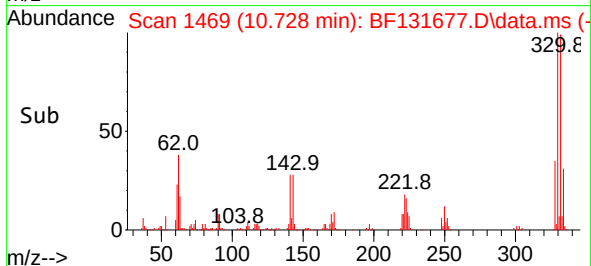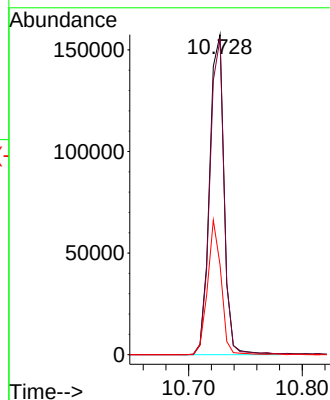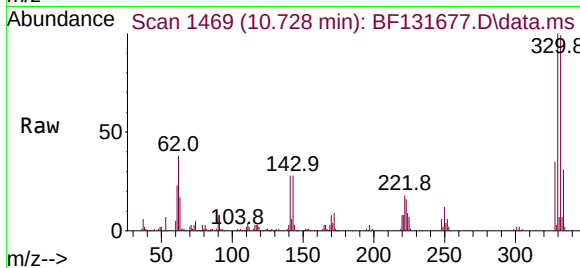

#45

2-Fluorobiphenyl

Concen: 68.359 ng

RT: 9.251 min Scan# 1218

Delta R.T. 0.000 min

Lab File: BF131677.D

Acq: 16 Dec 2022 20:56




Tgt Ion:172 Resp: 630434


Ion Ratio Lower Upper

172 100

171 35.7 28.3 42.5

170 23.3 19.3 28.9


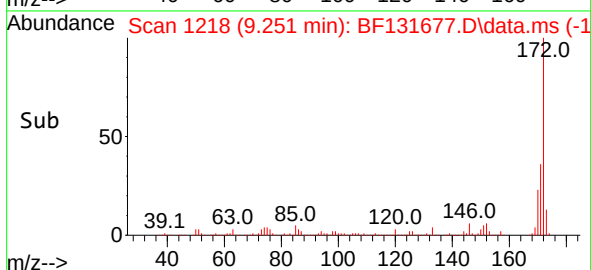
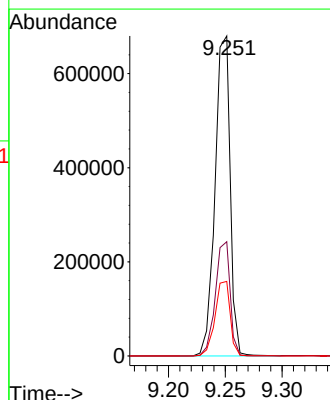
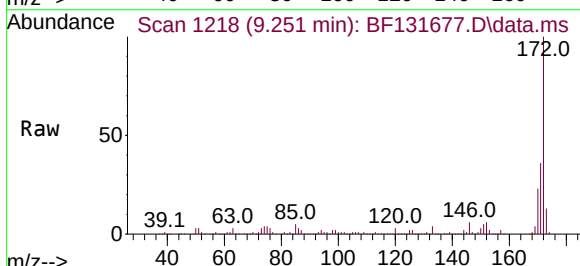


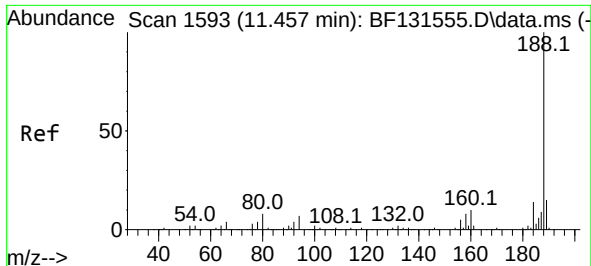

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.428 min Scan# 11
Delta R.T. 0.000 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56




Instrument :
BNA_F
ClientSampleId :
RB-24-(7-9)


Tgt Ion:188 Resp: 225728
Ion Ratio Lower Upper
188 100
94 6.7 5.5 8.3
80 8.1 6.6 10.0

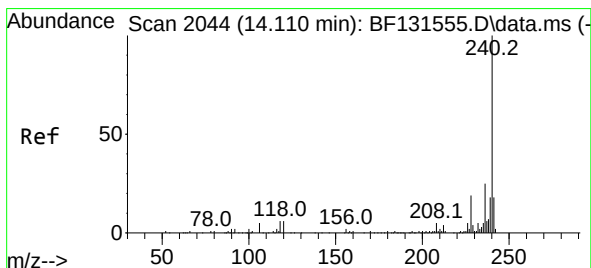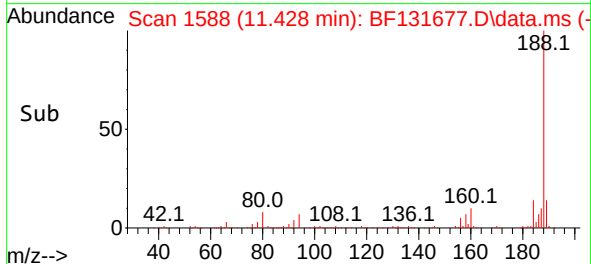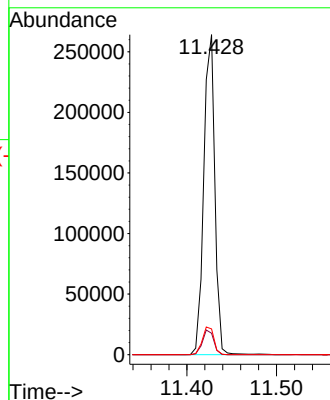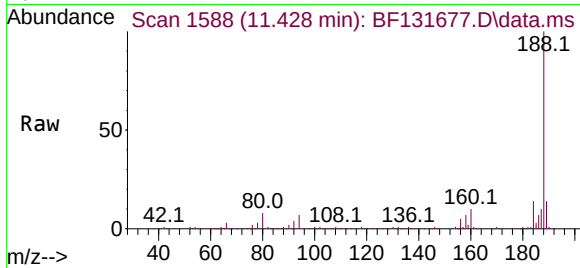

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.074 min Scan# 2038
Delta R.T. -0.006 min
Lab File: BF131677.D
Acq: 16 Dec 2022 20:56


Tgt Ion:240 Resp: 133952
Ion Ratio Lower Upper
240 100
120 8.6 4.6 7.0#
236 26.0 20.2 30.2

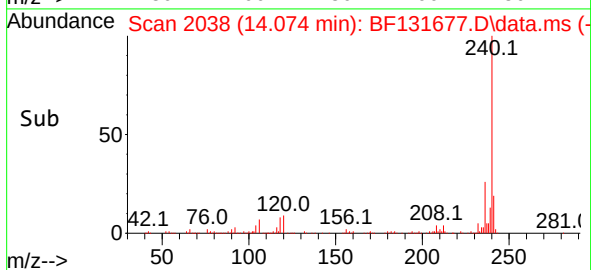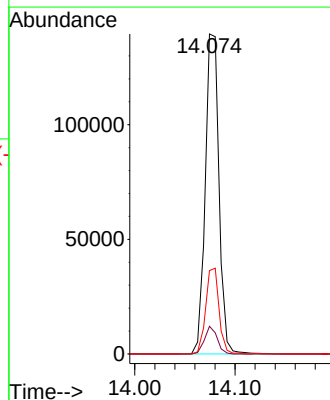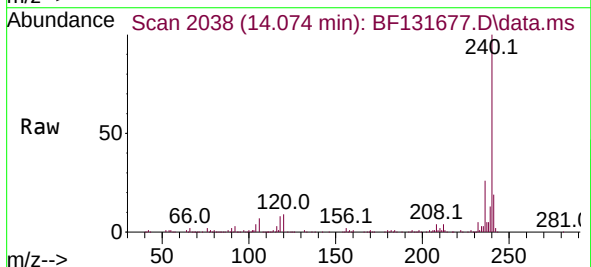



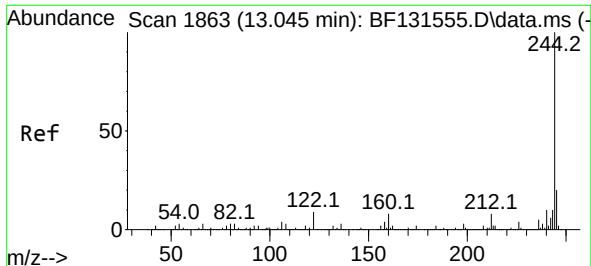


#79
 Terphenyl-d14
 Concen: 75.688 ng
 RT: 13.022 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BF131677.D
 Acq: 16 Dec 2022 20:56

Instrument :
 BNA_F
 ClientSampleId :
 RB-24-(7-9)

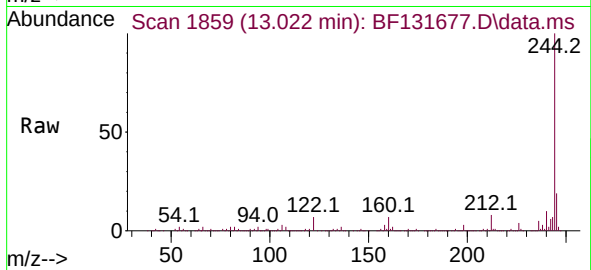

Tgt Ion:244 Resp: 739286
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.5 9.7
 122 7.1 7.1 10.7#

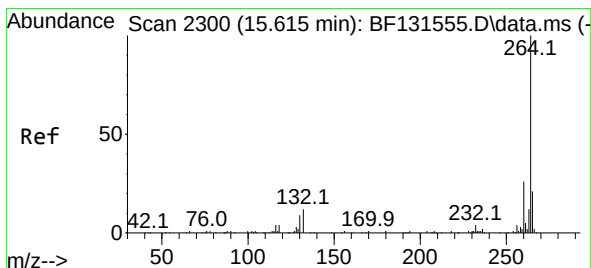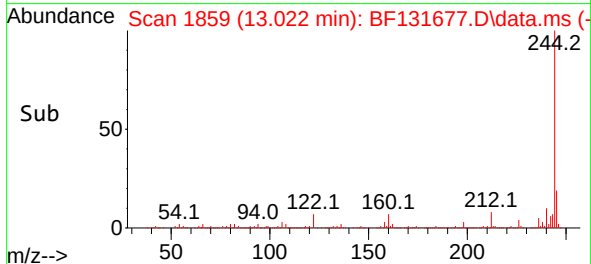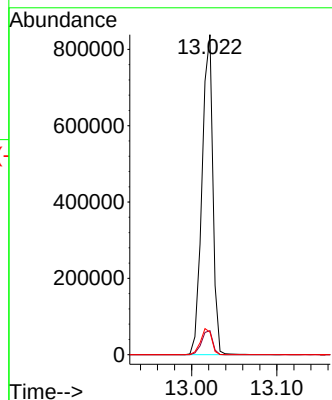

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.580 min Scan# 2294
 Delta R.T. 0.000 min
 Lab File: BF131677.D
 Acq: 16 Dec 2022 20:56

Tgt Ion:264 Resp: 139380
 Ion Ratio Lower Upper
 264 100
 260 23.5 20.6 30.8
 265 21.6 16.8 25.2

