


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121622\
Data File : BF131660.D
Acq On : 16 Dec 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 16 01:44:46 2022

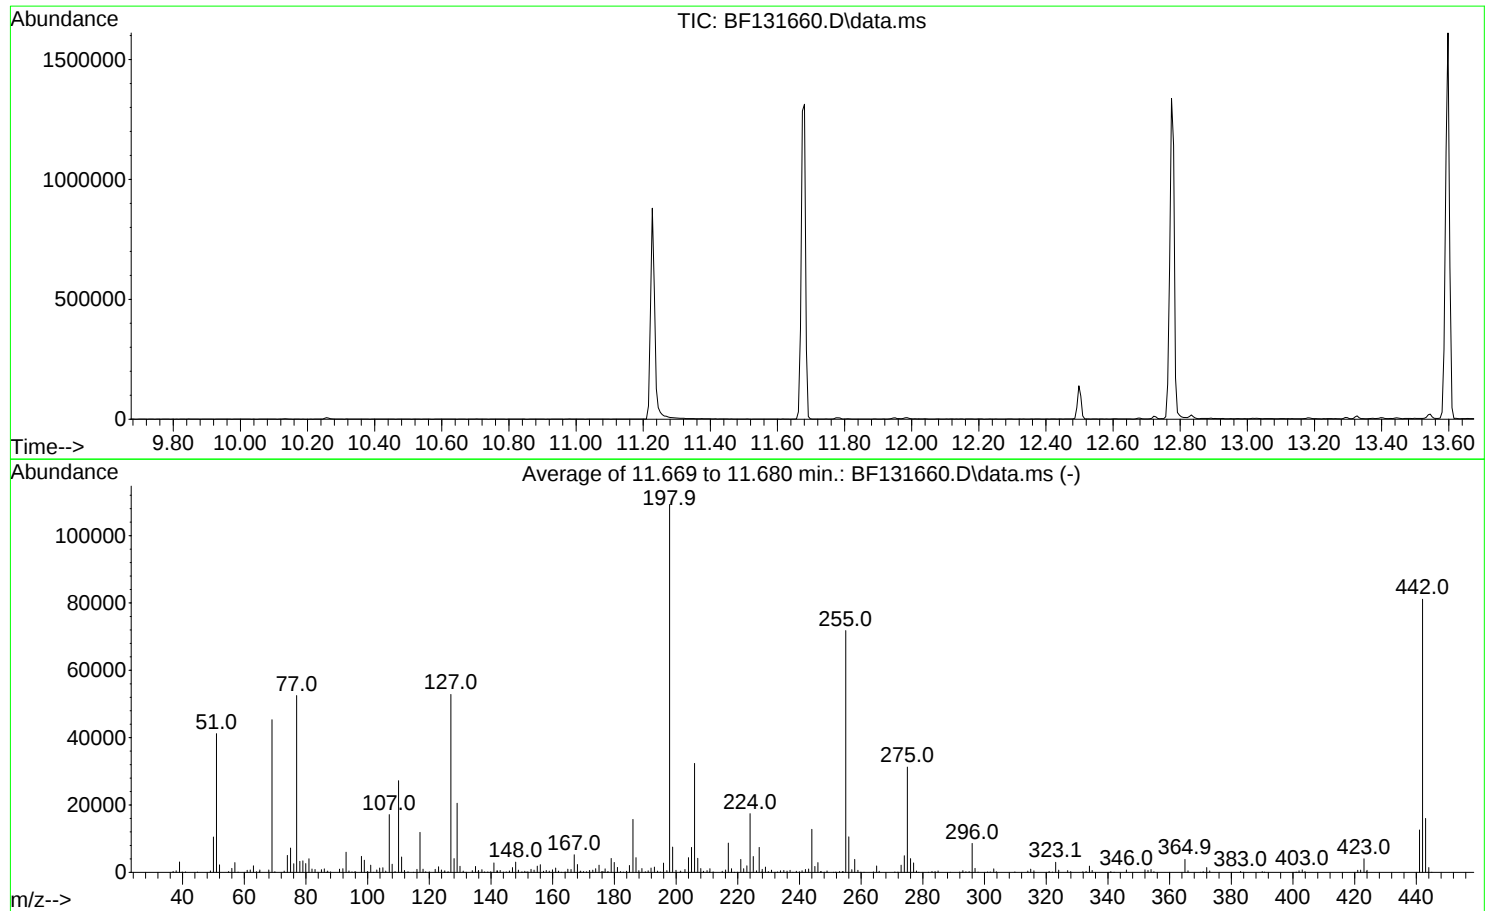

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1625

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	41192	PASS
68	69	0.00	2	1.5	694	PASS
69	198	0.00	100	41.5	45347	PASS
70	69	0.00	2	0.4	188	PASS
127	198	10	80	48.4	52861	PASS
197	198	0.00	2	0.5	541	PASS
198	198	100	100	100.0	109248	PASS
199	198	5	9	6.9	7516	PASS
275	198	10	60	28.6	31275	PASS
365	198	1	100	3.5	3872	PASS
441	198	0.01	100	11.5	12574	PASS
442	442	50	100	100.0	81139	PASS
443	442	15	24	19.8	16038	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/16/2022	BNA_F	<u>BF131660.D</u>
Compound Name	Response	Retention Time
DDT	259570	13.598
DDD	3480	13.327
DDE	132	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3612	263182	1.37

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121622\
Data File : BF131660.D
Acq On : 16 Dec 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 17 06:10:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration

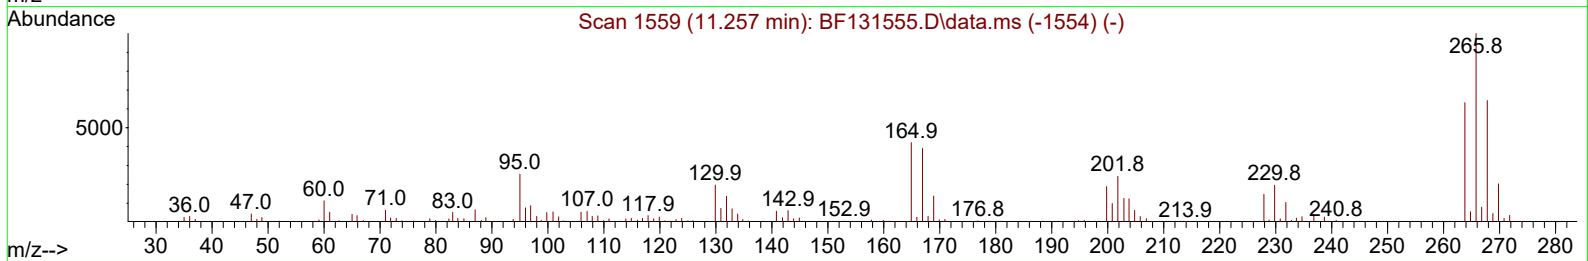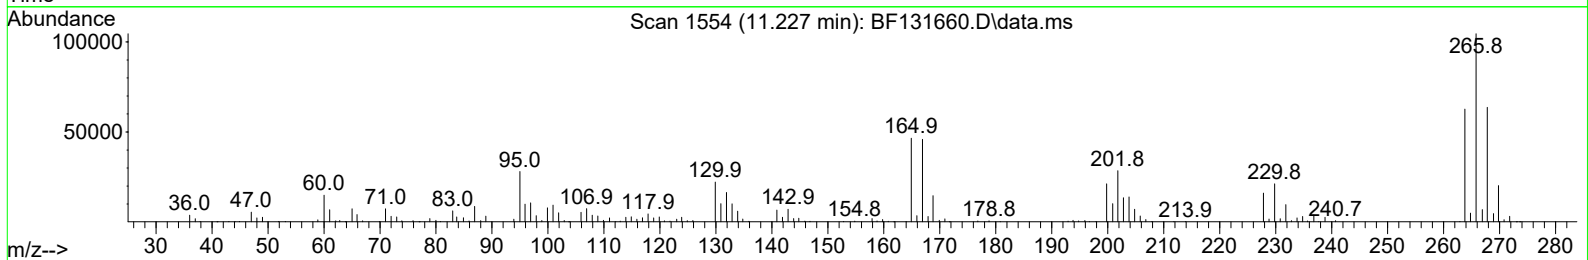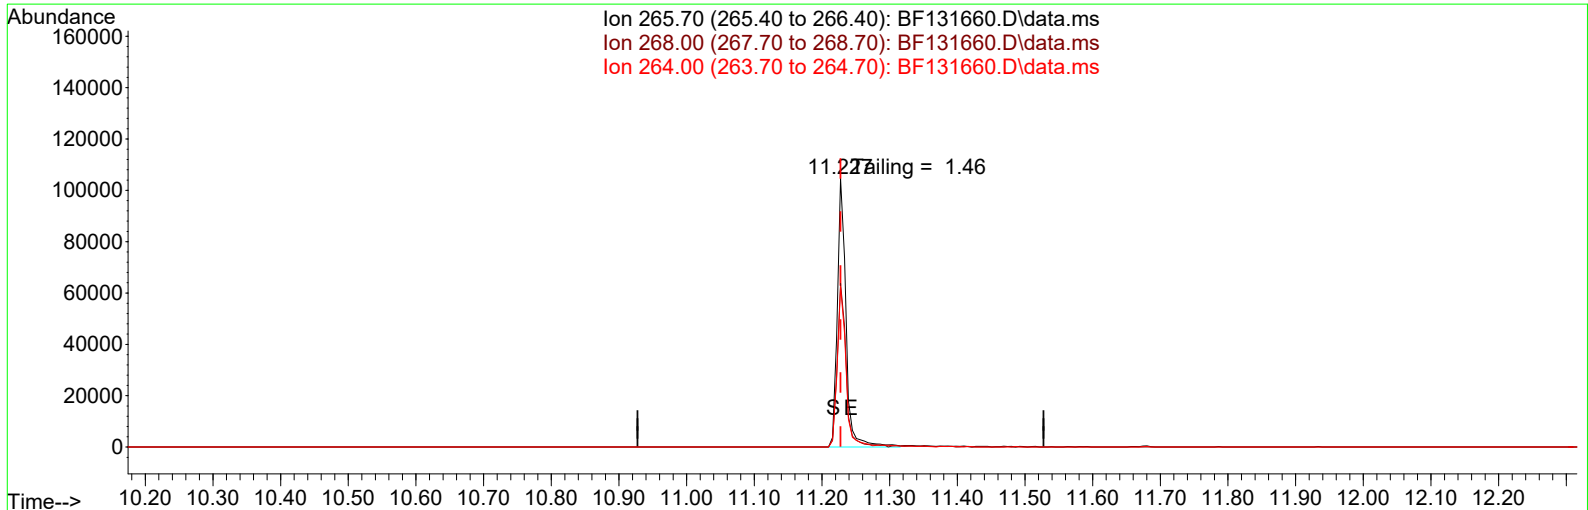

TIC: BF131660.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 184444.87 ng




response 93810

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	60.93
264.00	63.40	59.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121622\
Data File : BF131660.D
Acq On : 16 Dec 2022 11:29
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 17 06:10:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 16 01:44:46 2022
Response via : Initial Calibration

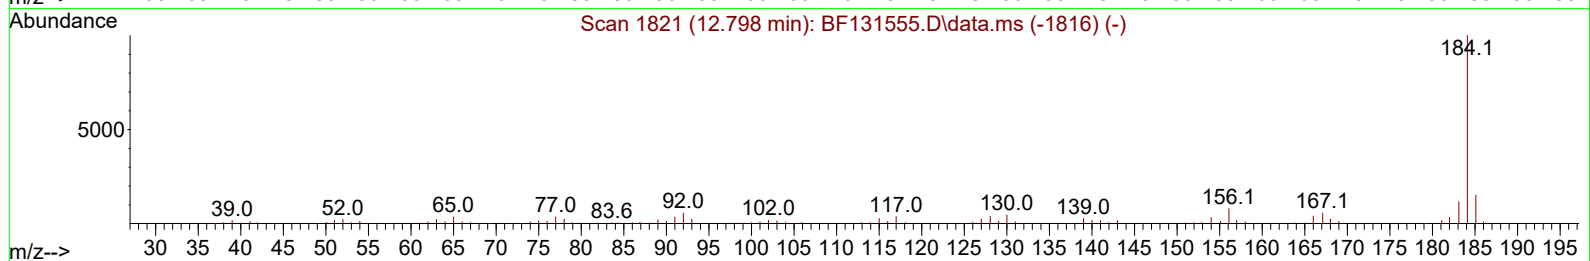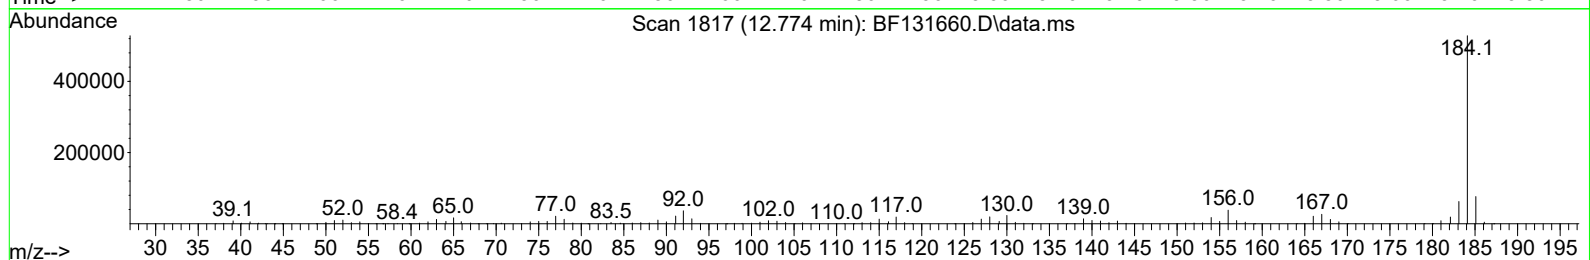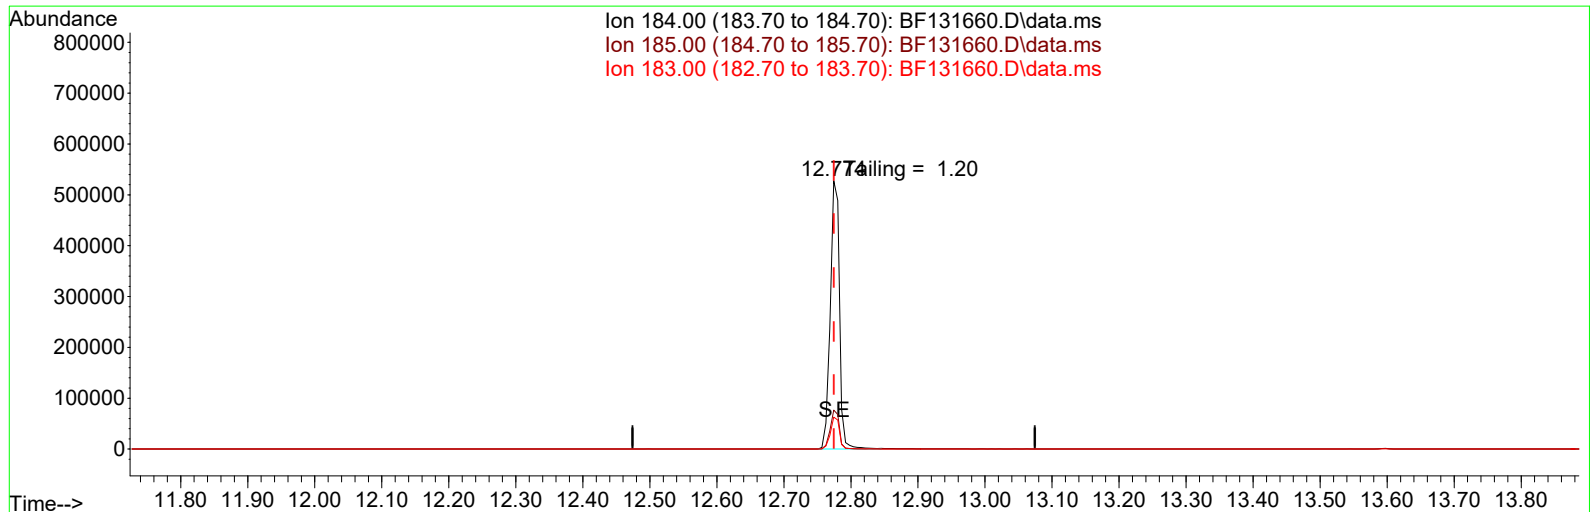

TIC: BF131660.D\data.ms

(77) Benzidine

12.774min (-0.000) 79782.71 ng

response 504494

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.50
183.00	11.60	11.90
0.00	0.00	0.00