


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121718\
 Data File : BF111527.D
 Acq On : 17 Dec 2018 8:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

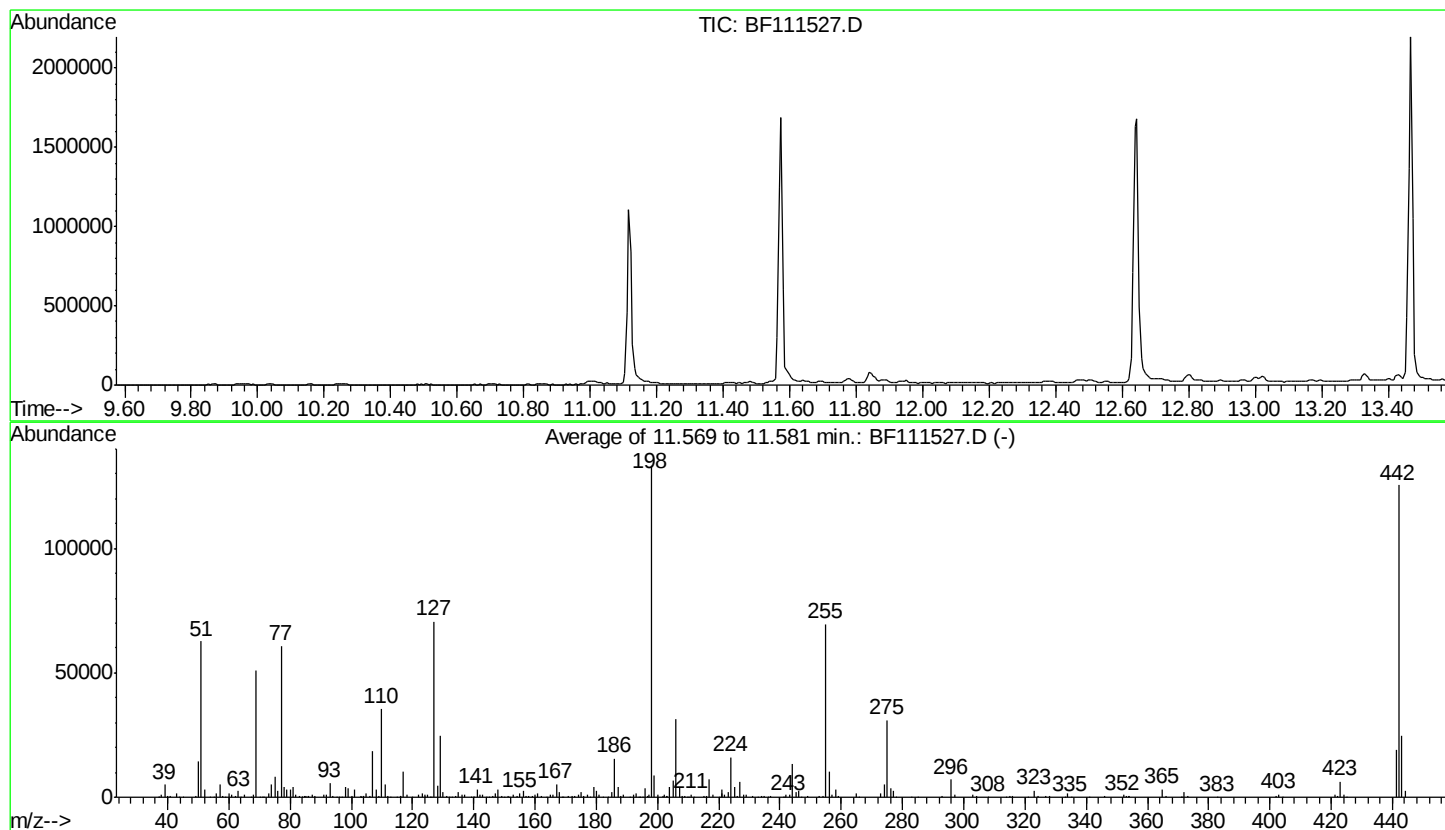

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	62657	PASS
68	69	0.00	2	1.6	817	PASS
69	198	0.00	100	38.4	51183	PASS
70	69	0.00	2	0.4	213	PASS
127	198	10	80	52.9	70570	PASS
197	198	0.00	2	0.7	923	PASS
198	198	100	100	100.0	133354	PASS
199	198	5	9	6.8	9024	PASS
275	198	10	60	23.3	31008	PASS
365	198	1	100	2.5	3279	PASS
441	198	0.01	100	14.4	19213	PASS
442	198	50	100	94.1	125472	PASS
443	442	15	24	19.8	24849	PASS