


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121718\
 Data File : BF111540.D
 Acq On : 17 Dec 2018 15:44
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

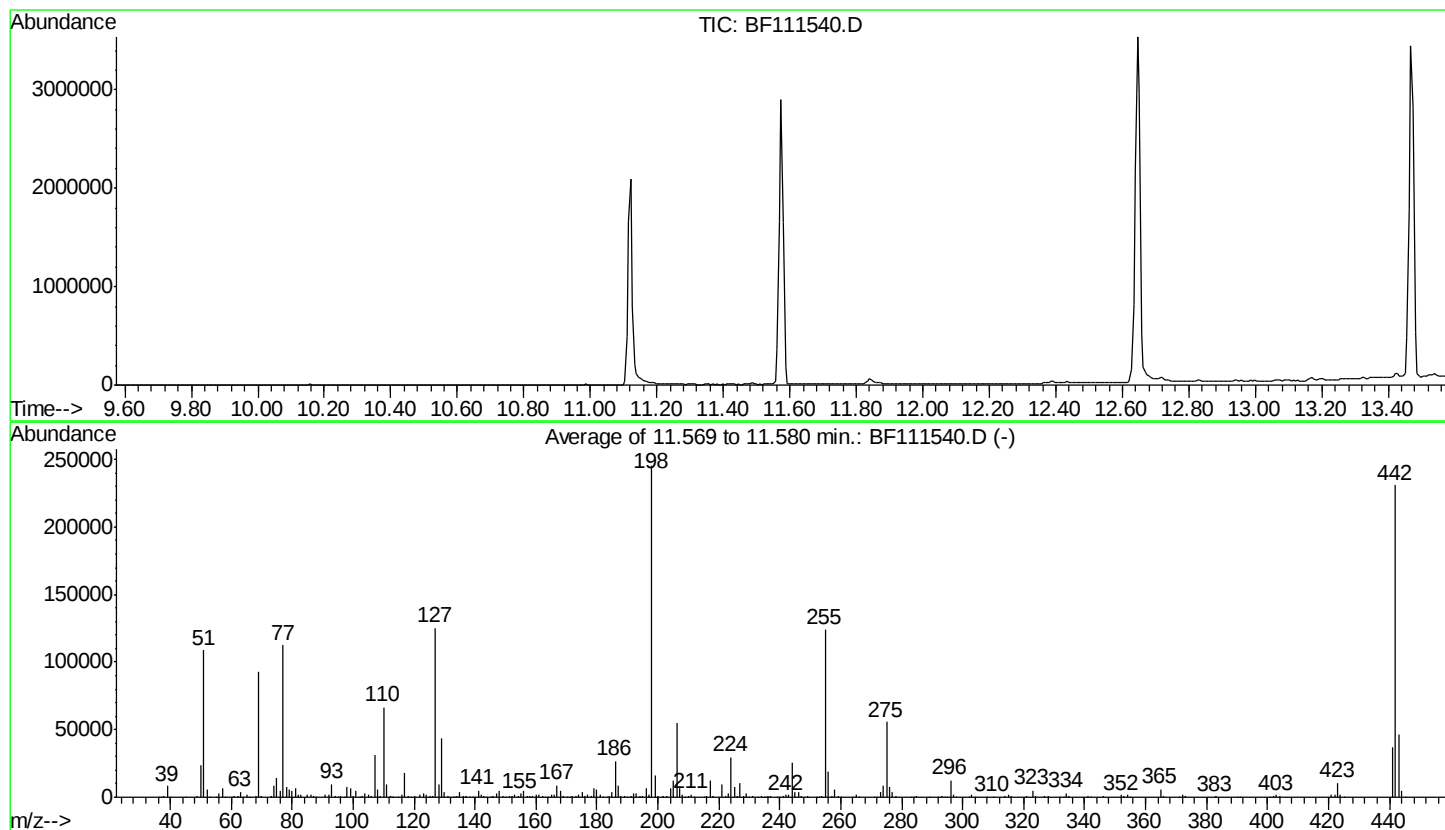

AutoFind: Scans 1612, 1613, 1614; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	108701	PASS
68	69	0.00	2	1.5	1408	PASS
69	198	0.00	100	37.7	92518	PASS
70	69	0.00	2	0.6	555	PASS
127	198	10	80	51.1	125488	PASS
197	198	0.00	2	0.9	2191	PASS
198	198	100	100	100.0	245418	PASS
199	198	5	9	6.4	15825	PASS
275	198	10	60	22.7	55653	PASS
365	198	1	100	2.4	5836	PASS
441	198	0.01	100	15.1	37126	PASS
442	198	50	100	94.0	230720	PASS
443	442	15	24	20.0	46058	PASS