


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121718\
 Data File : BF111567.D
 Acq On : 18 Dec 2018 4:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

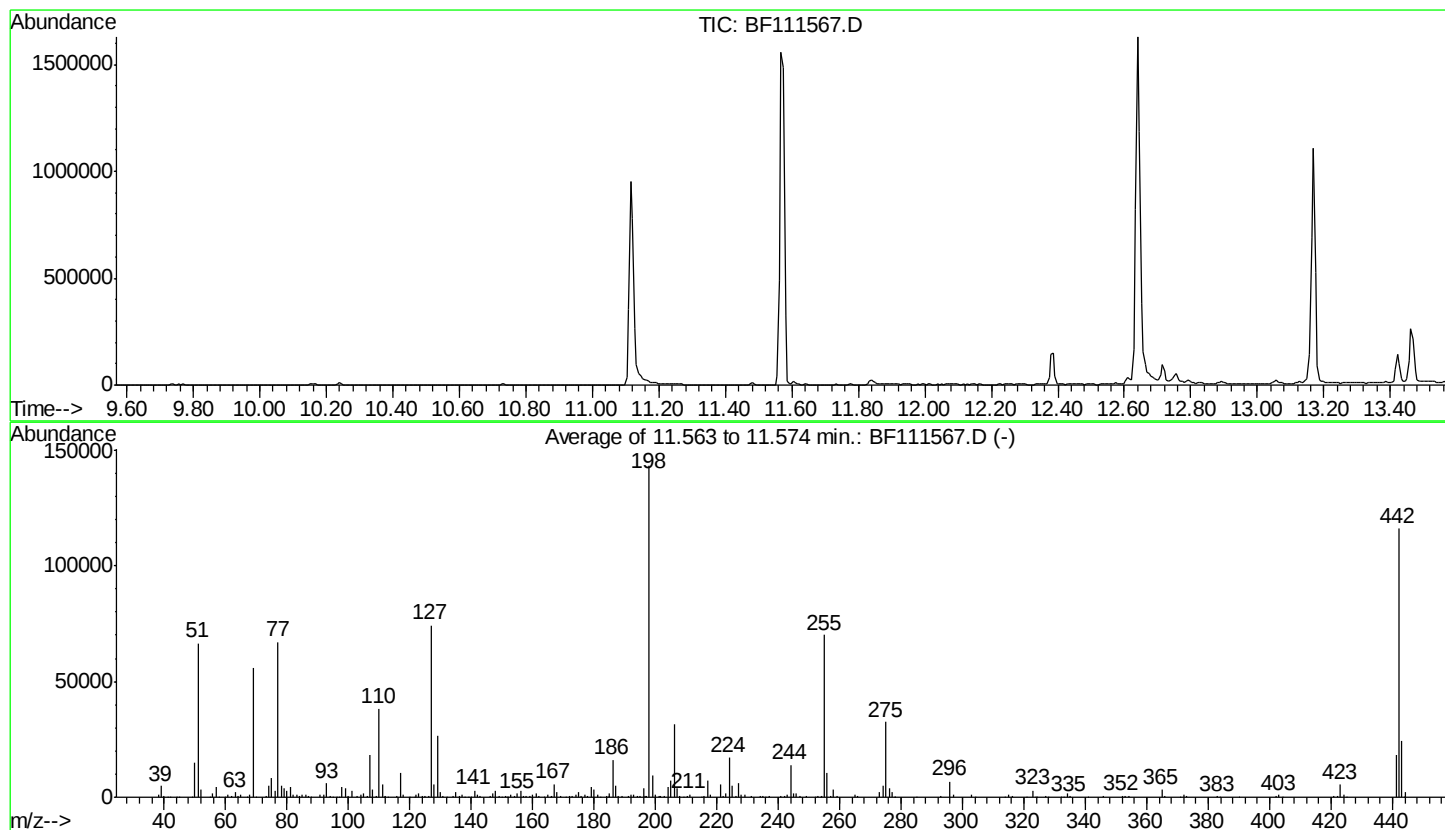

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.5	66661	PASS
68	69	0.00	2	1.6	882	PASS
69	198	0.00	100	38.9	55773	PASS
70	69	0.00	2	0.2	136	PASS
127	198	10	80	51.8	74208	PASS
197	198	0.00	2	0.3	404	PASS
198	198	100	100	100.0	143280	PASS
199	198	5	9	6.5	9260	PASS
275	198	10	60	22.7	32539	PASS
365	198	1	100	2.2	3194	PASS
441	198	0.01	100	12.7	18128	PASS
442	198	50	100	81.1	116149	PASS
443	442	15	24	21.1	24552	PASS