
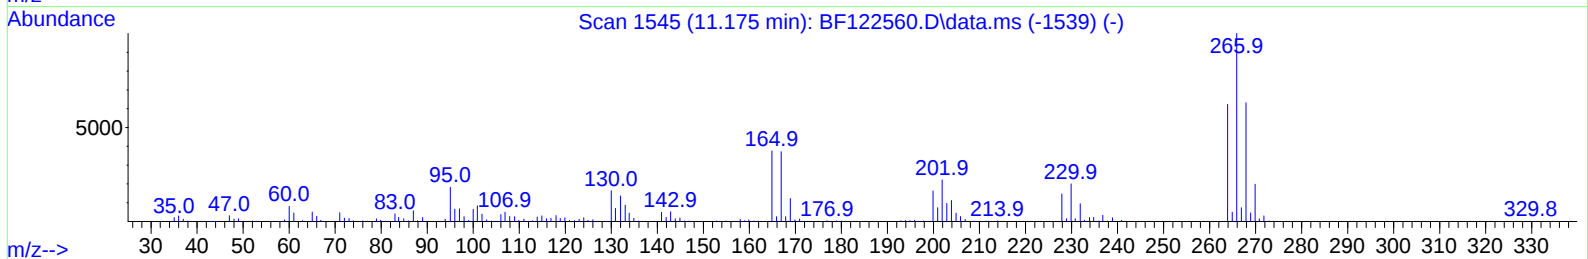
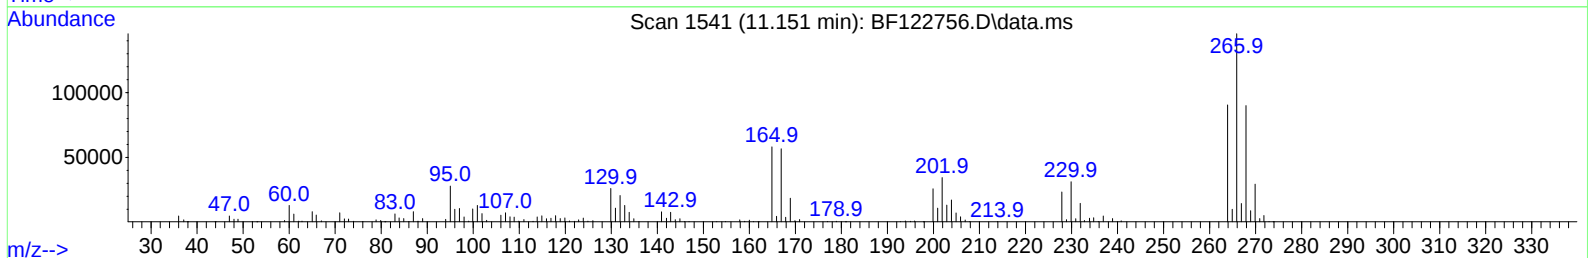


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
Data File : BF122756.D
Acq On : 17 Dec 2020 10:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 05:03:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

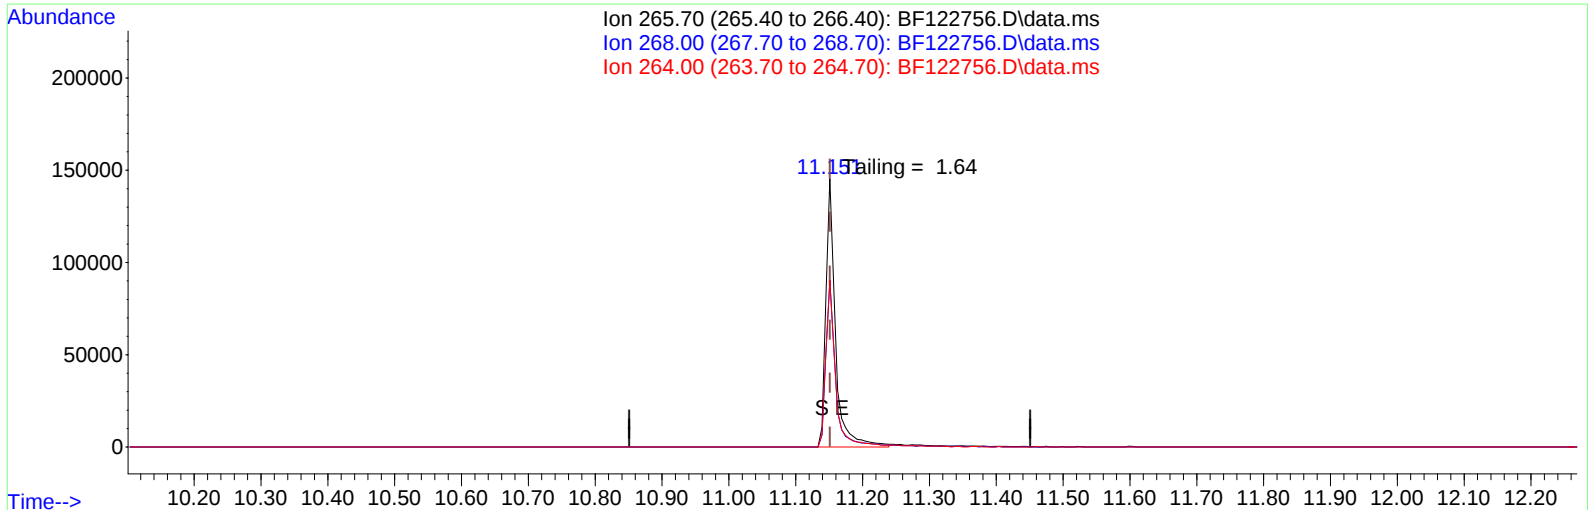

TIC: BF122756.D\data.ms

(70) Pentachlorophenol (C)




11.151min (-0.000) 44406.20 ng

response 148377

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.88
264.00	62.30	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
Data File : BF122756.D
Acq On : 17 Dec 2020 10:49
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 18 05:03:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 15 18:14:23 2020
Response via : Initial Calibration

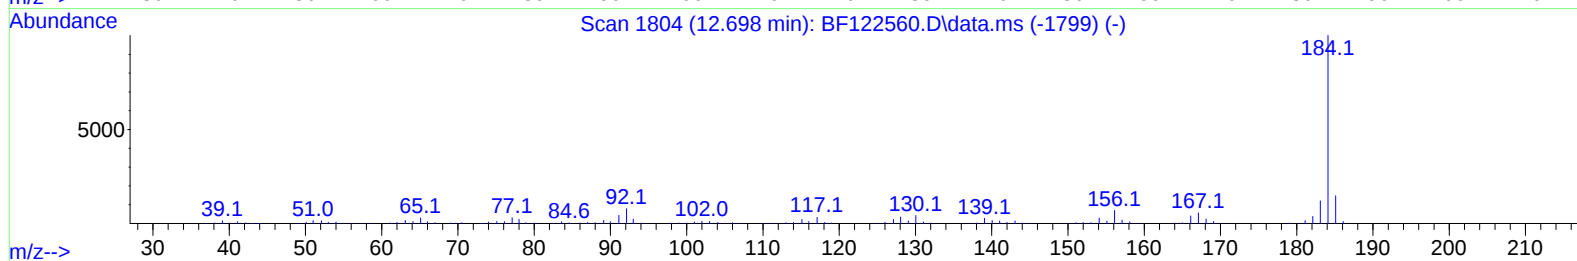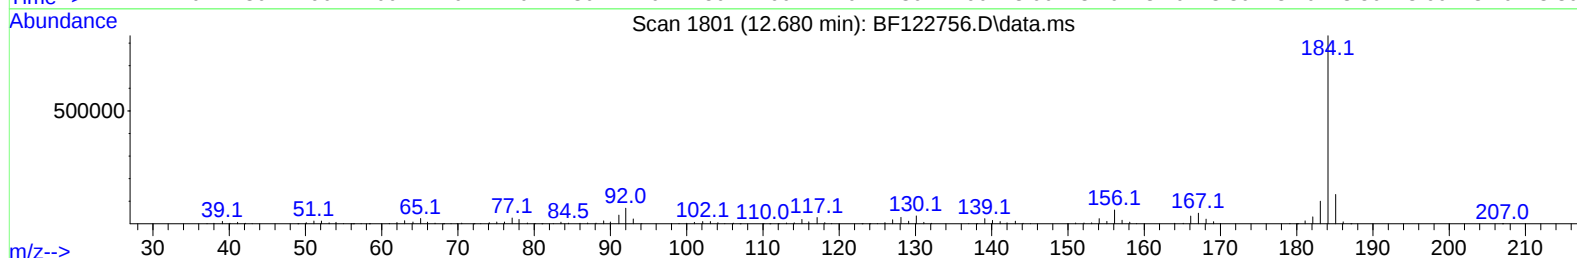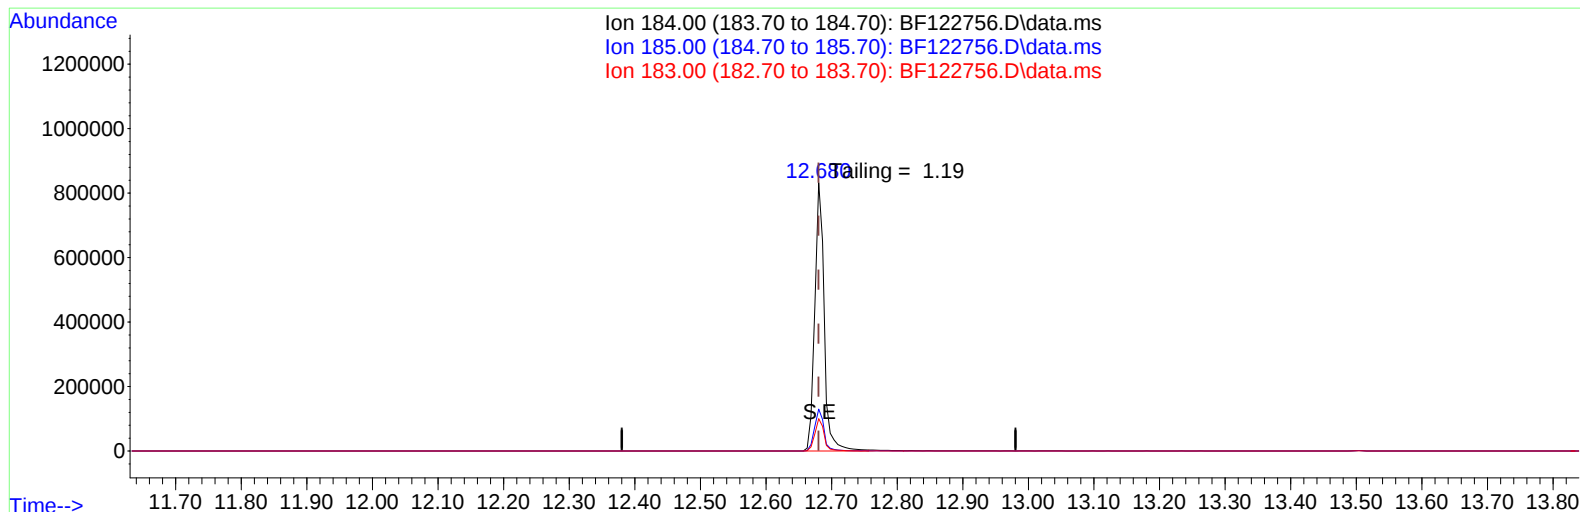

TIC: BF122756.D\data.ms

(77) Benzidine

12.680min (-0.000) 0.00 ng

response 843101

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	15.65
183.00	12.10	12.05
0.00	0.00	0.00