

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
 Data File : BF122768.D
 Acq On : 17 Dec 2020 17:06
 Operator : JU/CG
 Sample : PB133592BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133592BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122768.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.146	8	10	21	rVB2	28625	41608	1.42%	0.208%
2	5.434	566	569	587	rBV	1319637	1372945	47.00%	6.867%
3	6.445	737	741	765	rBV	1313259	1335230	45.71%	6.678%
4	6.816	800	804	813	rBV	1304578	1026143	35.13%	5.132%
5	7.375	895	899	917	rBV	1160429	1197091	40.98%	5.987%
6	8.098	1018	1022	1048	rBV	1323437	1387696	47.50%	6.940%
7	9.175	1200	1205	1217	rBV	2386951	2384147	81.61%	11.924%
8	9.292	1221	1225	1230	rVB	39387	48558	1.66%	0.243%
9	9.569	1269	1272	1281	rBV	61324	59764	2.05%	0.299%
10	9.857	1316	1321	1344	rBV	1739142	1630056	55.80%	8.153%
11	10.645	1451	1455	1473	rBV	1495271	1528627	52.33%	7.645%
12	11.339	1569	1573	1581	rBV	1716406	1691333	57.90%	8.459%
13	12.927	1839	1843	1846	rBV	3329470	2921219	100.00%	14.610%
14	13.980	2018	2022	2035	rVB	1683184	1728048	59.16%	8.643%
15	15.439	2265	2270	2283	rBV2	1119033	1569755	53.74%	7.851%
16	15.886	2342	2346	2351	rVB2	24962	37679	1.29%	0.188%
17	16.380	2425	2430	2436	rBV3	20700	34371	1.18%	0.172%




Sum of corrected areas: 19994270

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
Data File : BF122768.D
Acq On : 17 Dec 2020 17:06
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

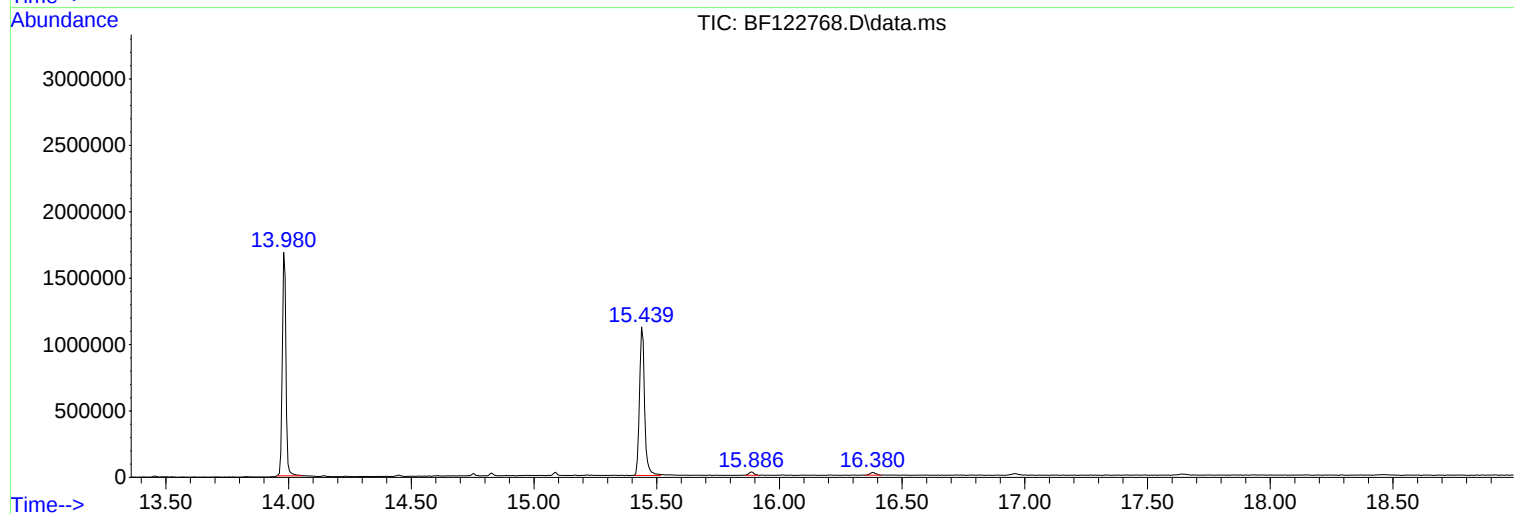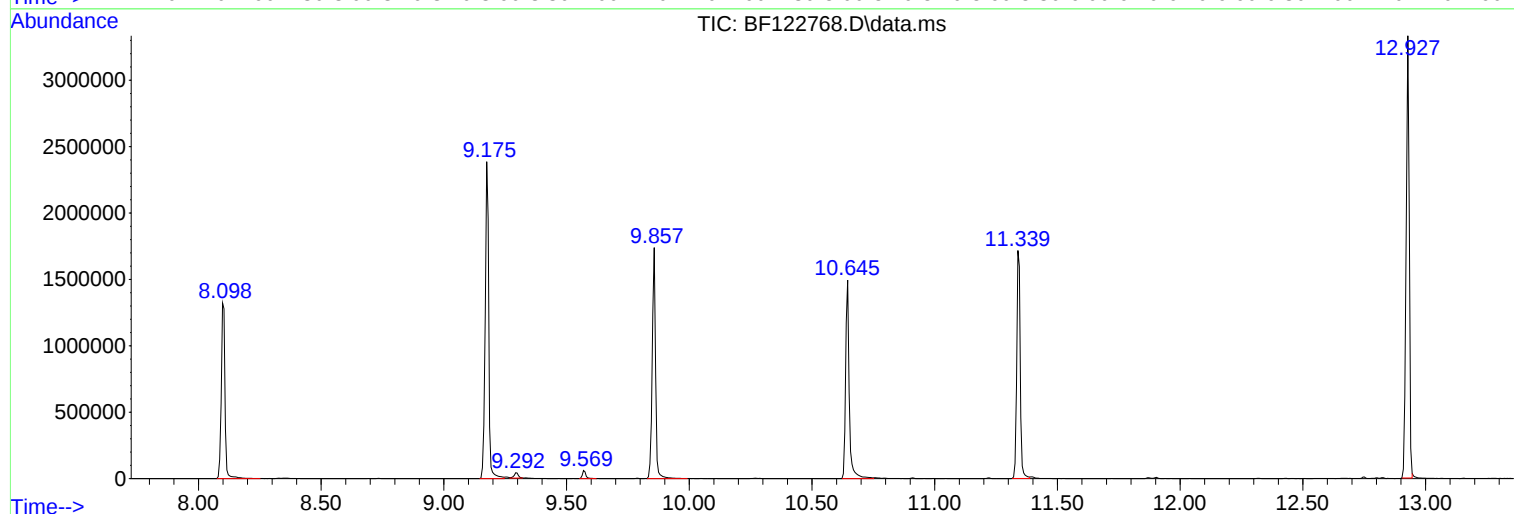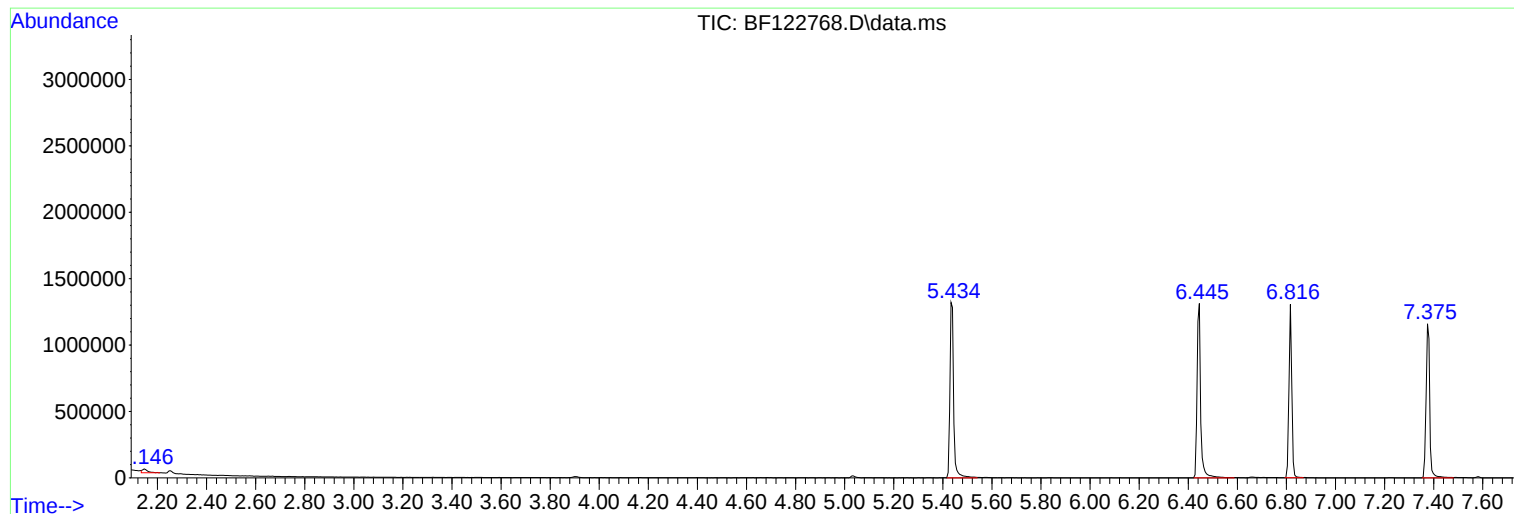

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
Data File : BF122768.D
Acq On : 17 Dec 2020 17:06
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
Data File : BF122768.D
Acq On : 17 Dec 2020 17:06
Operator : JU/CG
Sample : PB133592BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133592BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------