
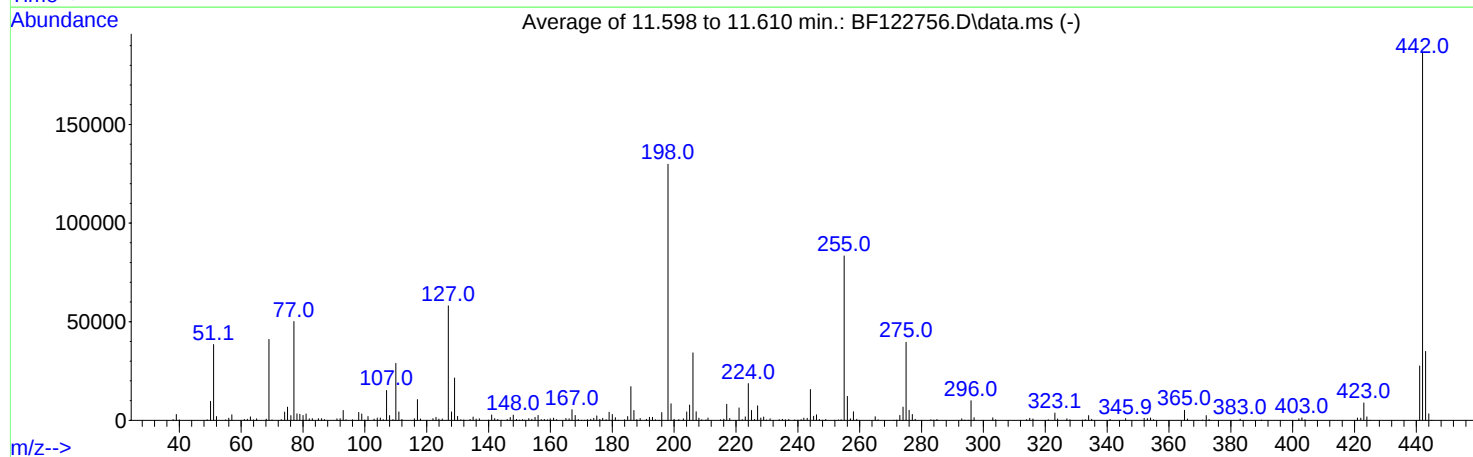


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121720\
 Data File : BF122756.D
 Acq On : 17 Dec 2020 10:49
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

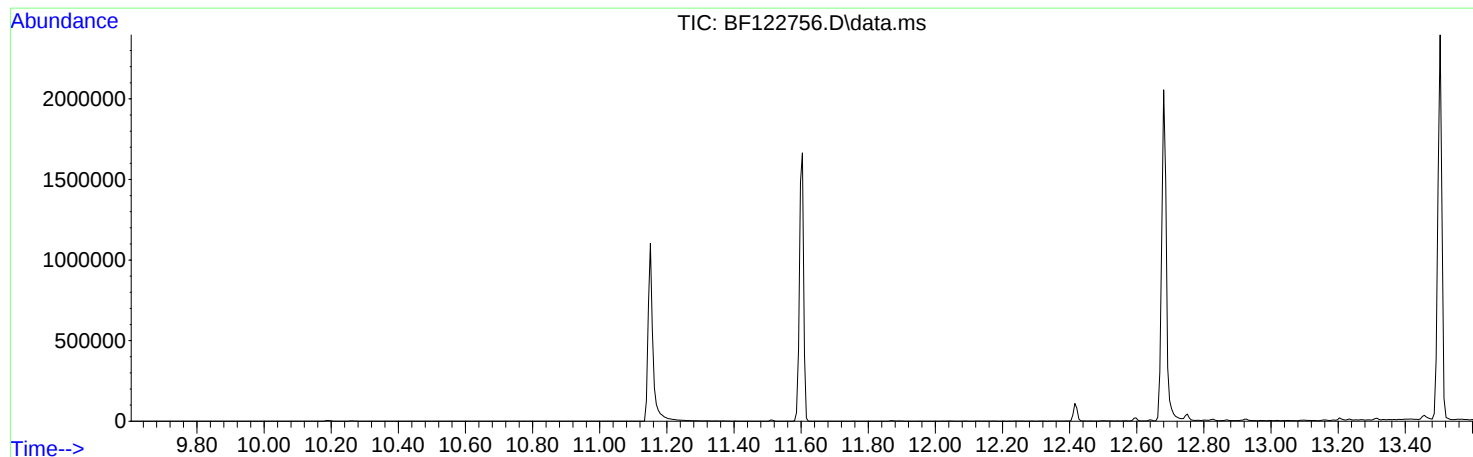

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.6	38492	PASS
68	69	0.00	2	1.6	647	PASS
69	198	0.00	100	31.6	41015	PASS
70	69	0.00	2	0.6	231	PASS
127	198	10	80	44.7	58101	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	129899	PASS
199	198	5	9	6.5	8402	PASS
275	198	10	60	30.5	39562	PASS
365	198	1	100	4.0	5150	PASS
441	198	0.01	100	21.2	27584	PASS
442	442	100	100	100.0	186485	PASS
443	442	15	24	18.7	34947	PASS