


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121818\
 Data File : BF111578.D
 Acq On : 18 Dec 2018 13:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

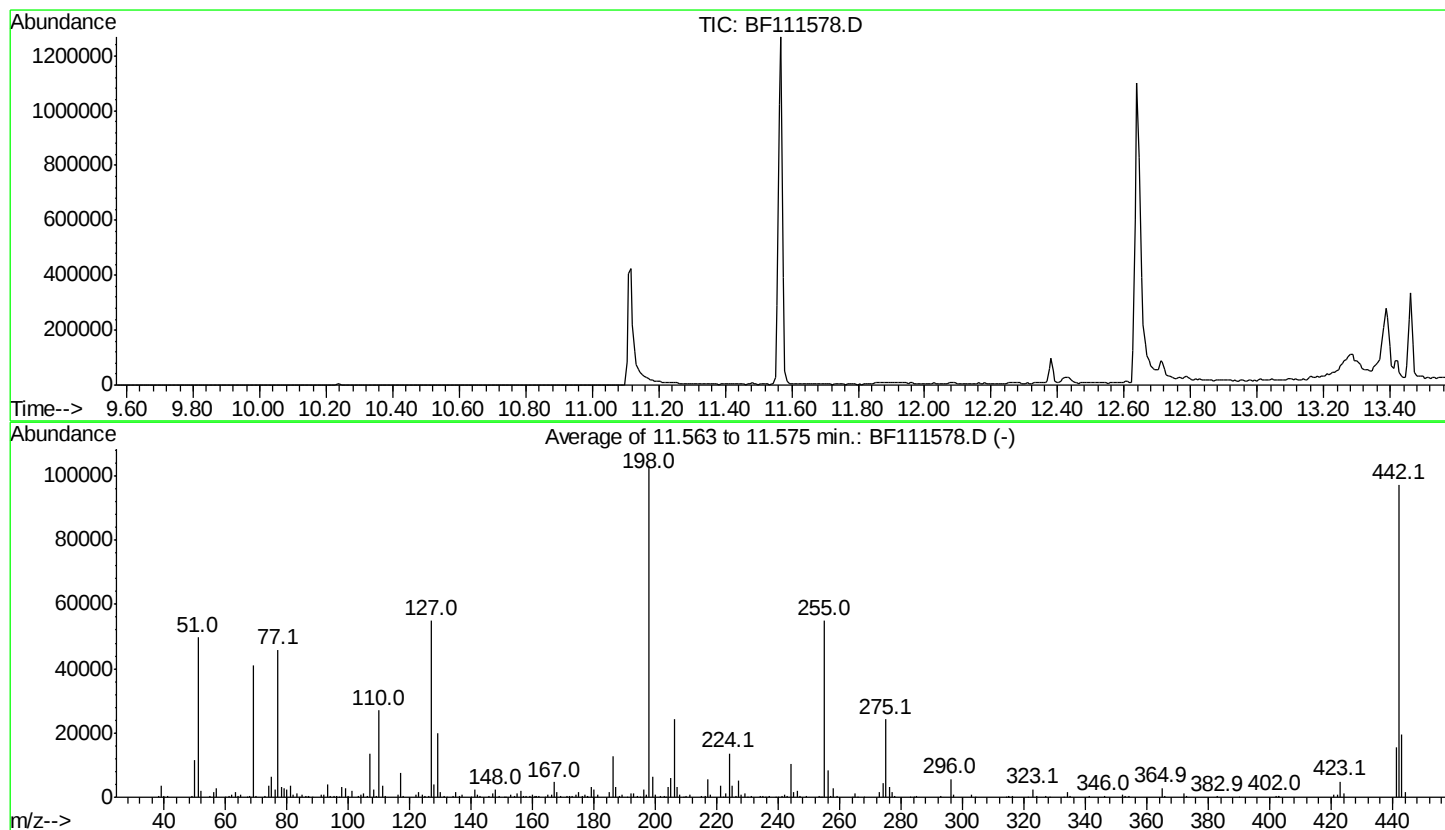

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	49702	PASS
68	69	0.00	2	1.5	609	PASS
69	198	0.00	100	39.6	40875	PASS
70	69	0.00	2	0.6	265	PASS
127	198	10	80	53.2	54930	PASS
197	198	0.00	2	0.7	710	PASS
198	198	100	100	100.0	103197	PASS
199	198	5	9	6.4	6575	PASS
275	198	10	60	23.5	24269	PASS
365	198	1	100	2.9	2988	PASS
441	198	0.01	100	14.9	15378	PASS
442	198	50	100	94.3	97341	PASS
443	442	15	24	20.2	19623	PASS