


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121818\
 Data File : BF111581.D
 Acq On : 18 Dec 2018 17:52
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121418.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 14 13:26:17 2018

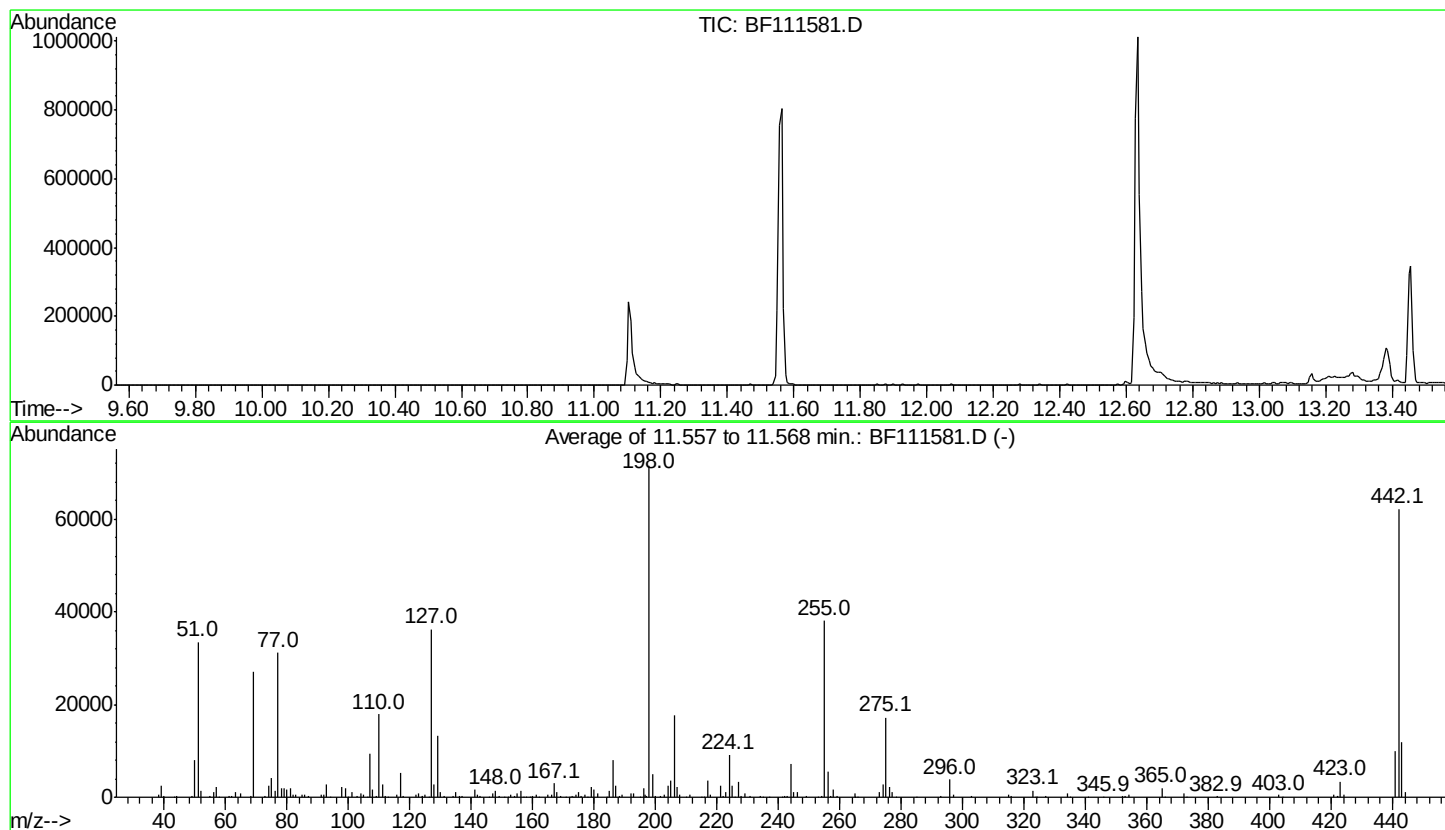

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1604

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	33496	PASS
68	69	0.00	2	1.4	376	PASS
69	198	0.00	100	37.7	27000	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	36327	PASS
197	198	0.00	2	0.7	493	PASS
198	198	100	100	100.0	71552	PASS
199	198	5	9	7.0	5012	PASS
275	198	10	60	24.1	17262	PASS
365	198	1	100	2.8	2002	PASS
441	198	0.01	100	13.8	9888	PASS
442	198	50	100	87.0	62216	PASS
443	442	15	24	19.1	11881	PASS