
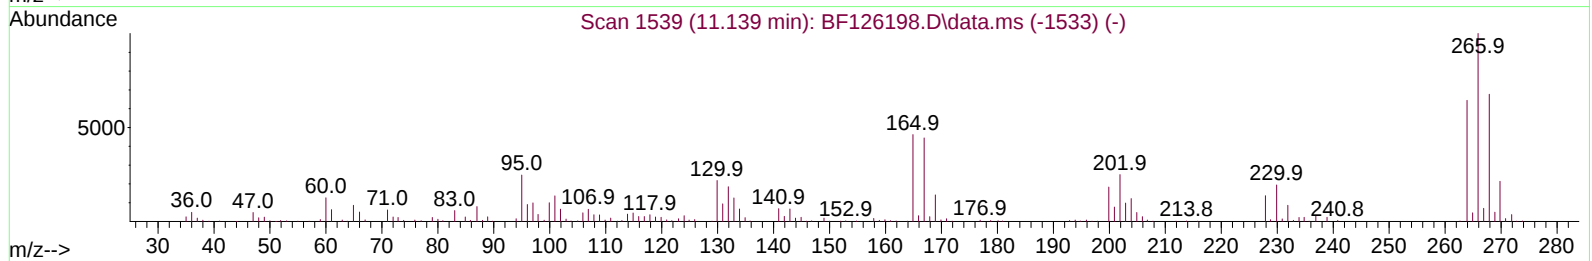
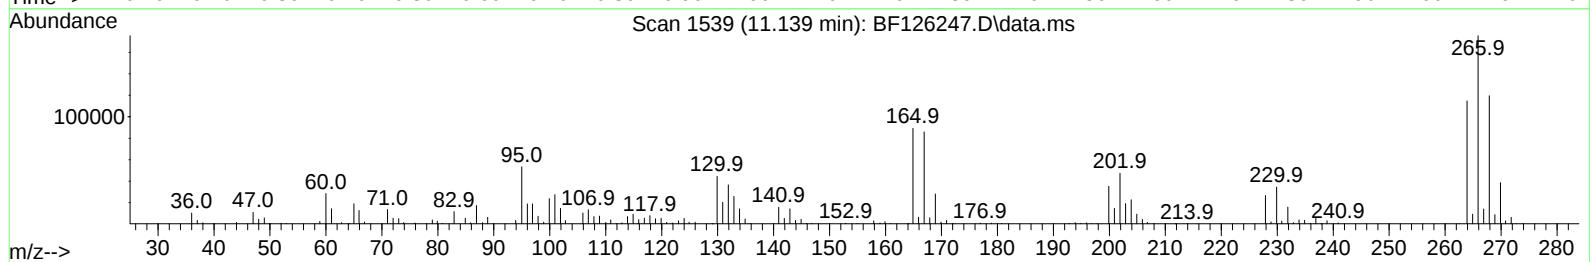


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121821\
Data File : BF126247.D
Acq On : 18 Dec 2021 10:51
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 10:48:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

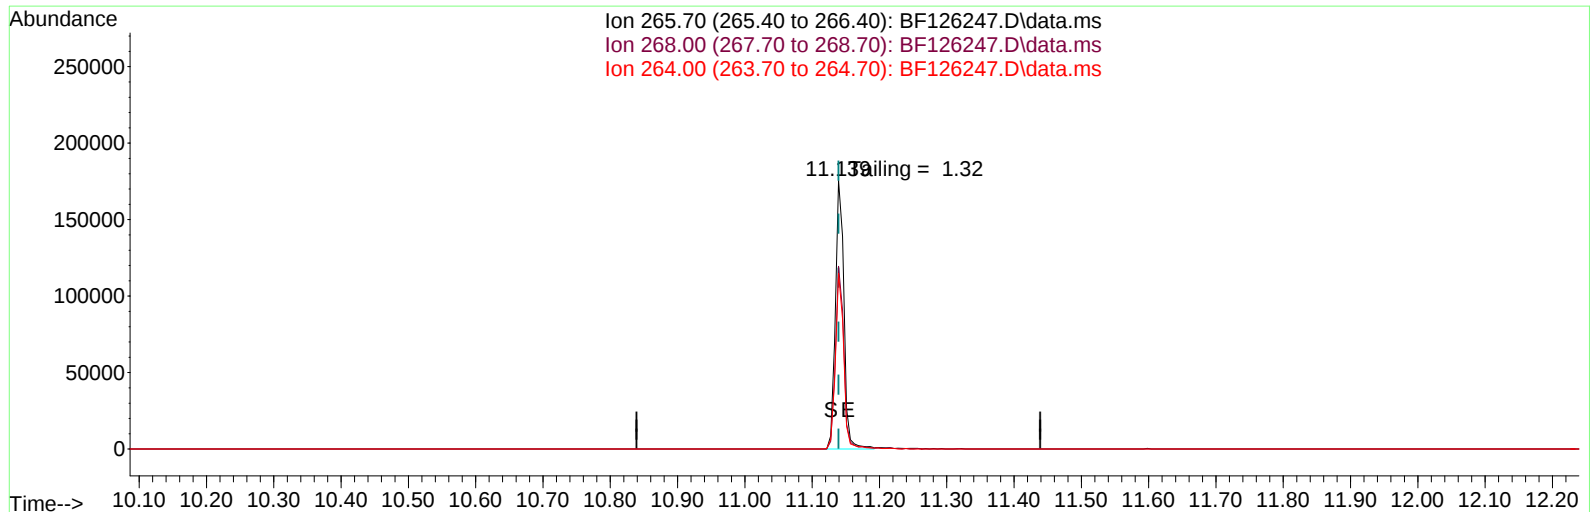

TIC: BF126247.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 35720.27 ng

response 155935

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.11
264.00	69.90	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121821\
Data File : BF126247.D
Acq On : 18 Dec 2021 10:51
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 10:48:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

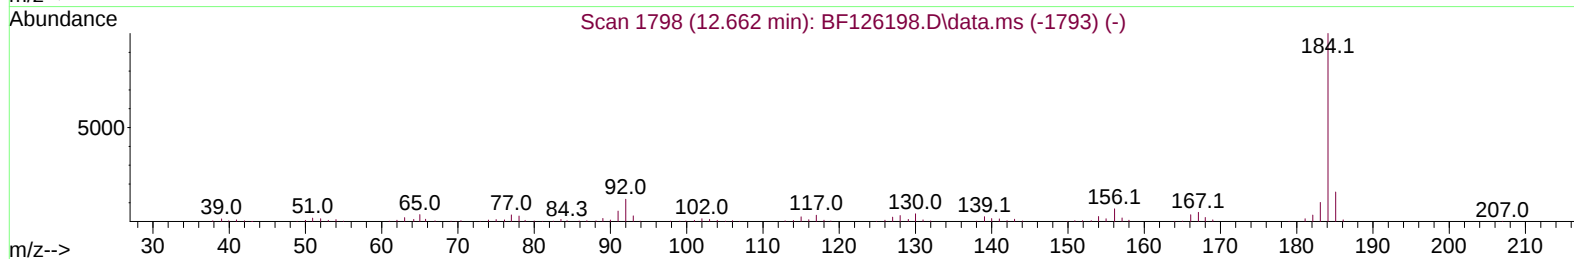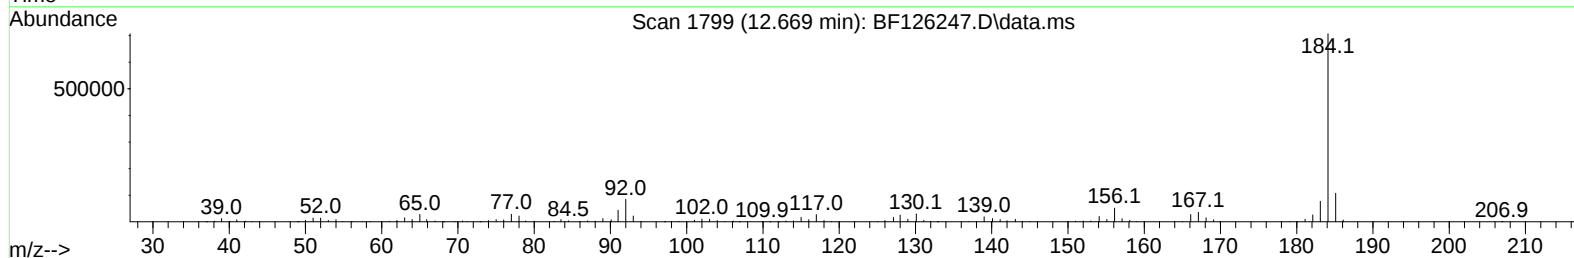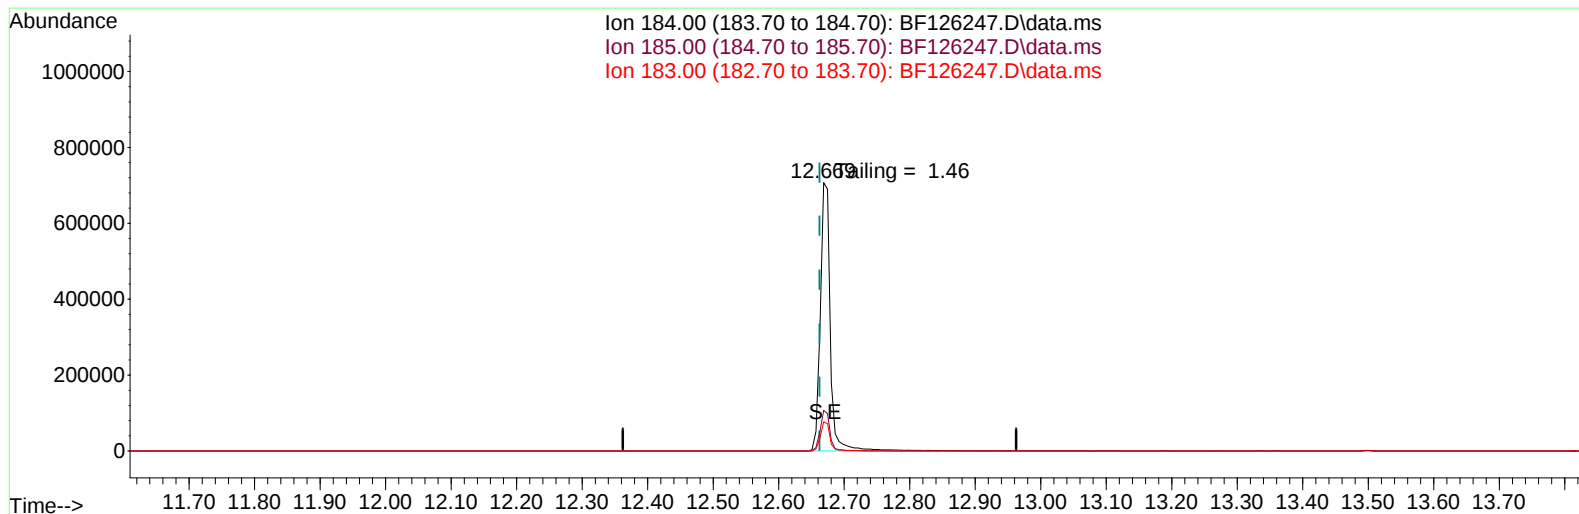

TIC: BF126247.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response 750338

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.16
183.00	10.10	10.92
0.00	0.00	0.00