


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121821\
 Data File : BF126247.D
 Acq On : 18 Dec 2021 10:51
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

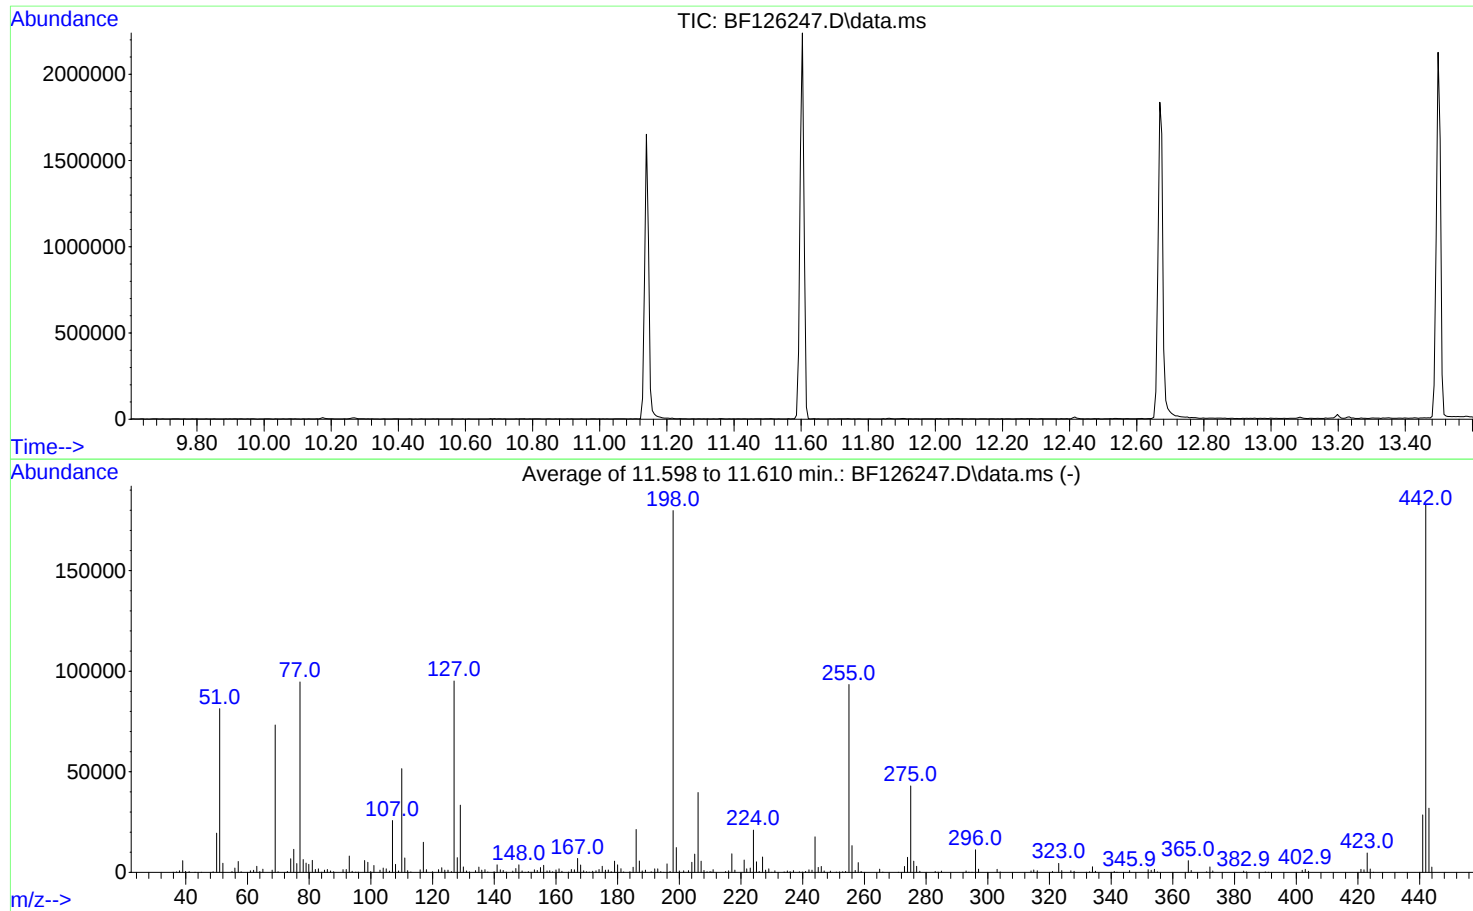




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.2	81392	PASS
68	69	0.00	2	1.5	1114	PASS
69	198	0.00	100	40.7	73283	PASS
70	69	0.00	2	0.5	357	PASS
127	198	10	80	52.9	95109	PASS
197	198	0.00	2	0.3	501	PASS
198	198	100	100	100.0	179880	PASS
199	198	5	9	6.9	12354	PASS
275	198	10	60	23.9	42992	PASS
365	198	1	100	3.2	5845	PASS
441	198	0.01	100	15.9	28552	PASS
442	442	50	100	100.0	182885	PASS
443	442	15	24	17.4	31899	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121821\  
Data File : BF126247.D  
Acq On    : 18 Dec 2021  10:51  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 10:48:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

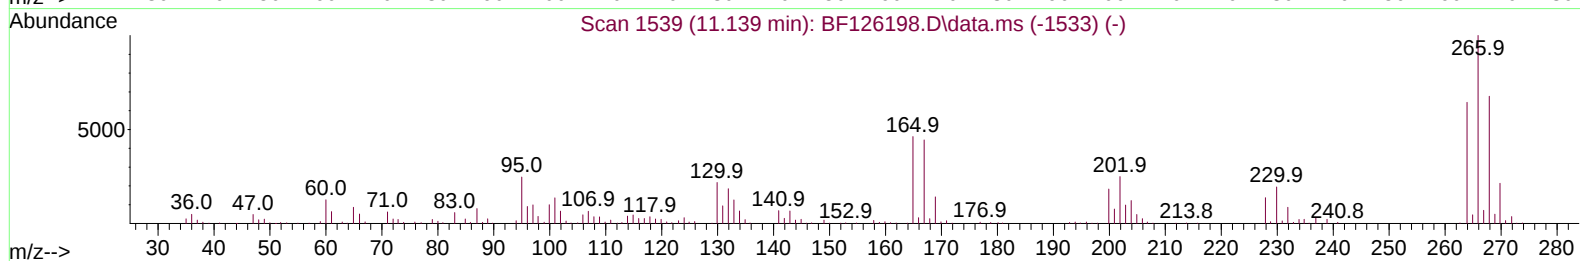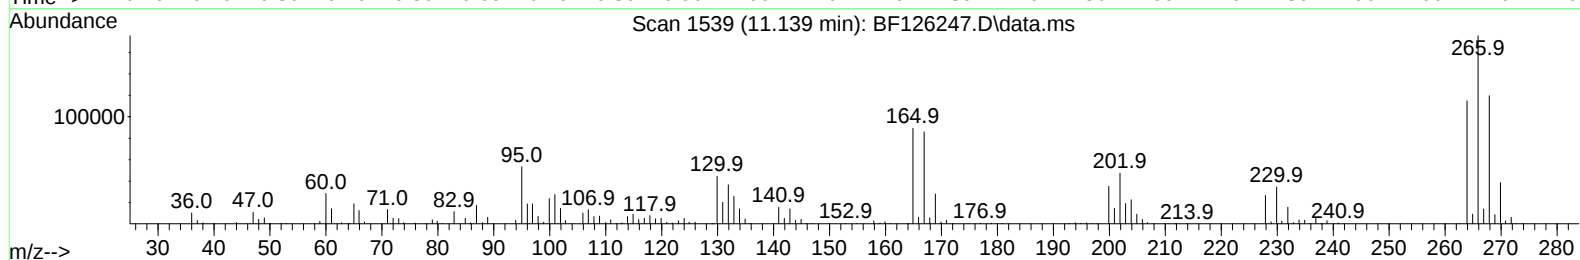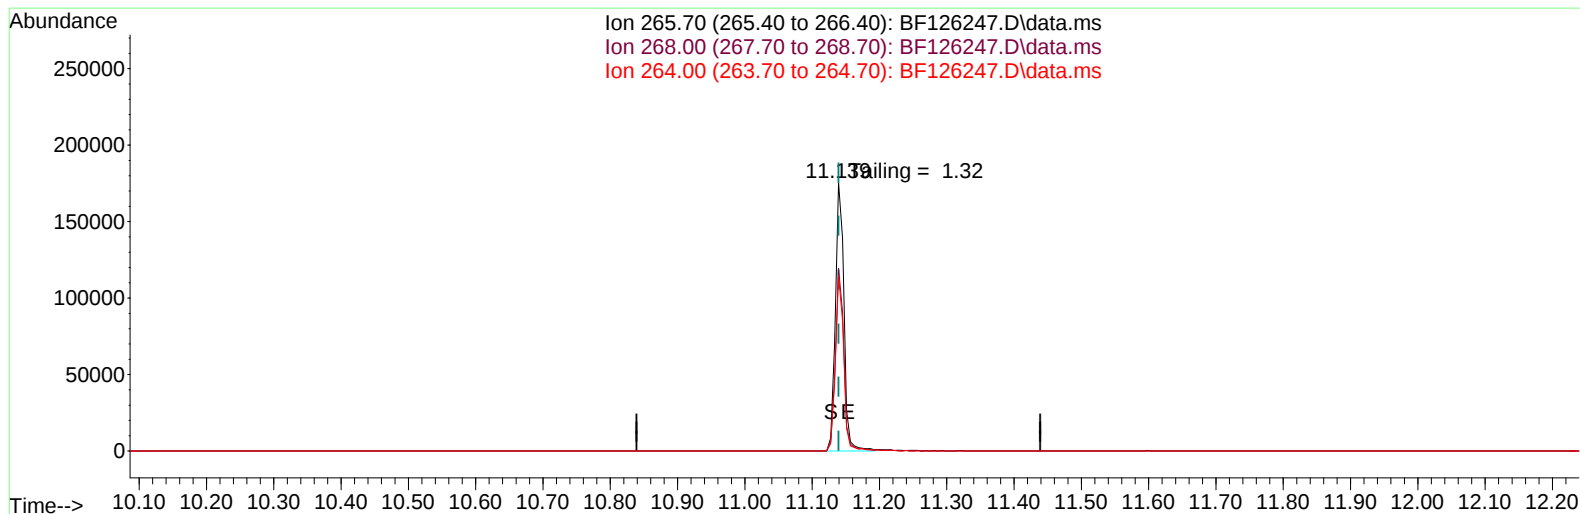

TIC: BF126247.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 35720.27 ng




response **155935**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.11
264.00	69.90	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121821\
Data File : BF126247.D
Acq On : 18 Dec 2021 10:51
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 10:48:16 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

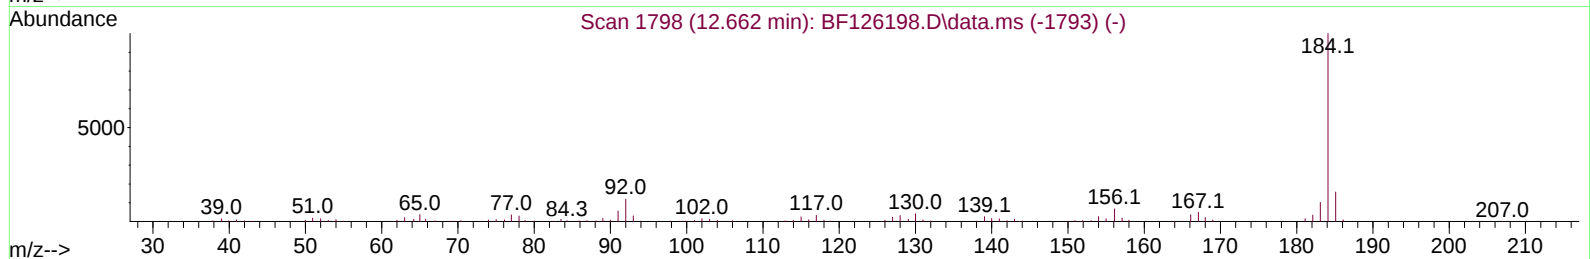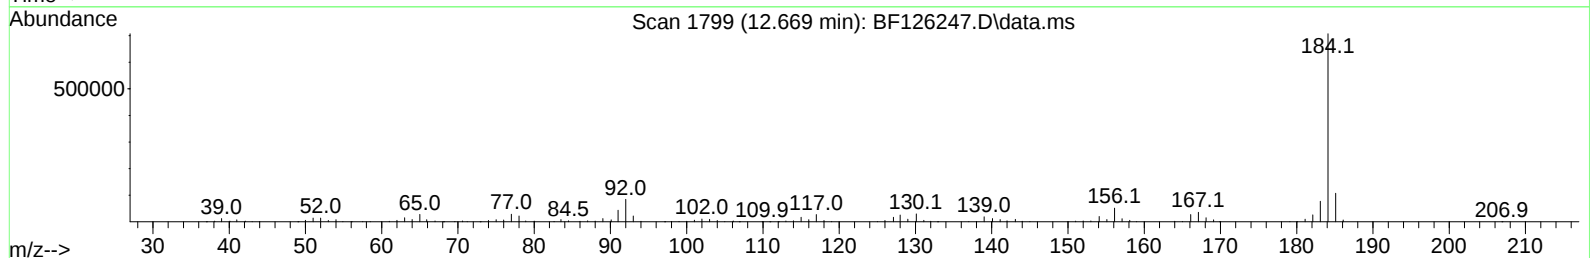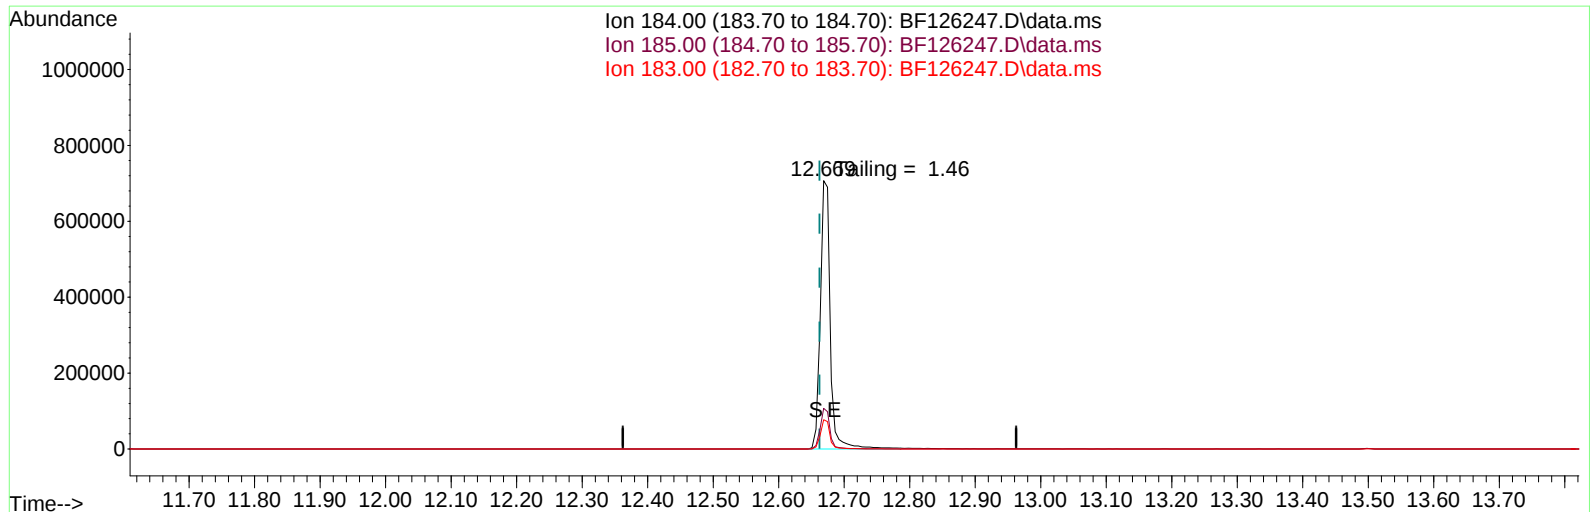

TIC: BF126247.D\data.ms

(77) Benzidine

12.669min (+ 0.006) 0.00 ng

response 750338

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.16
183.00	10.10	10.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/18/2021	BNA_F	<u>BF126247.D</u>
Compound Name	Response	Retention Time
DDT	353045	13.498
DDD	5413	13.198
DDE	280	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5693	358738	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP