
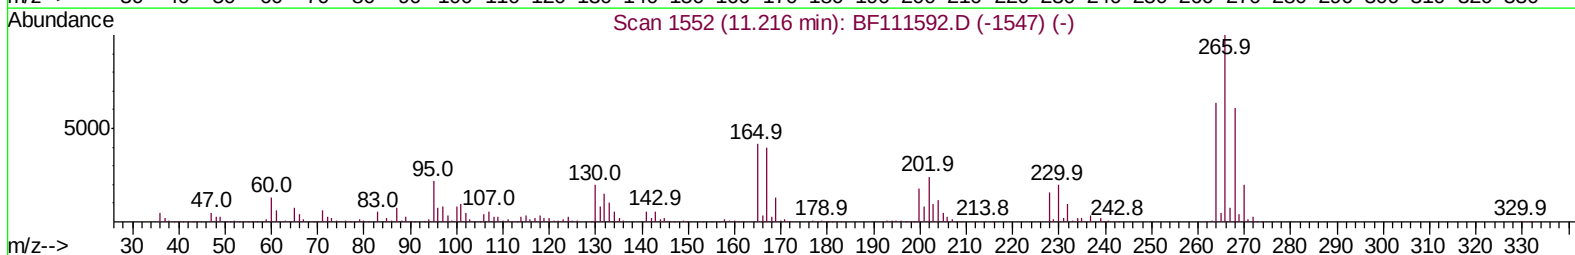
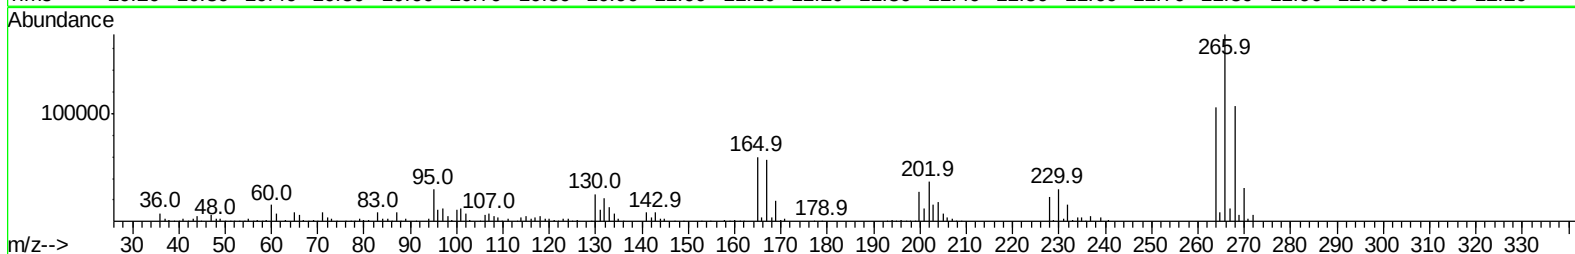


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111588.D
Acq On : 19 Dec 2018 13:43
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 17:25:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 16:16:54 2018
Response via : Initial Calibration

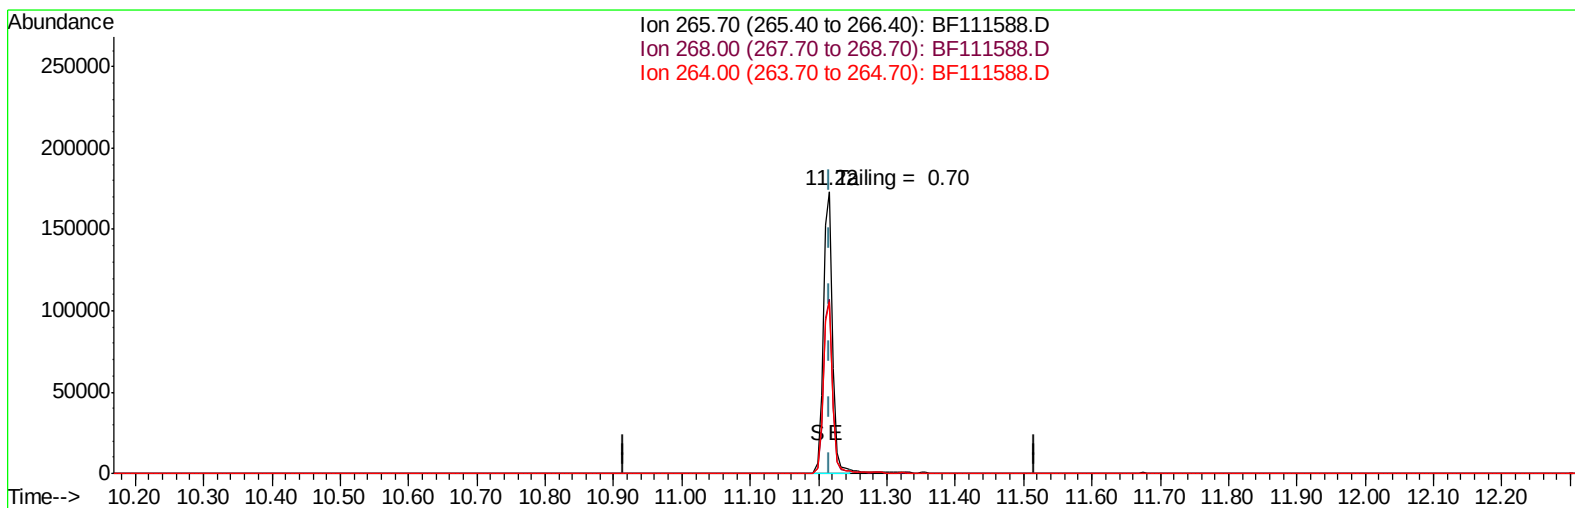

TIC: BF111588.D

(70) Pentachlorophenol (C)




11.216min (-0.000) 47166.18ng

response 168064

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	61.97
264.00	61.40	61.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
 Data File : BF111588.D
 Acq On : 19 Dec 2018 13:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 19 17:25:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 16:16:54 2018
 Response via : Initial Calibration

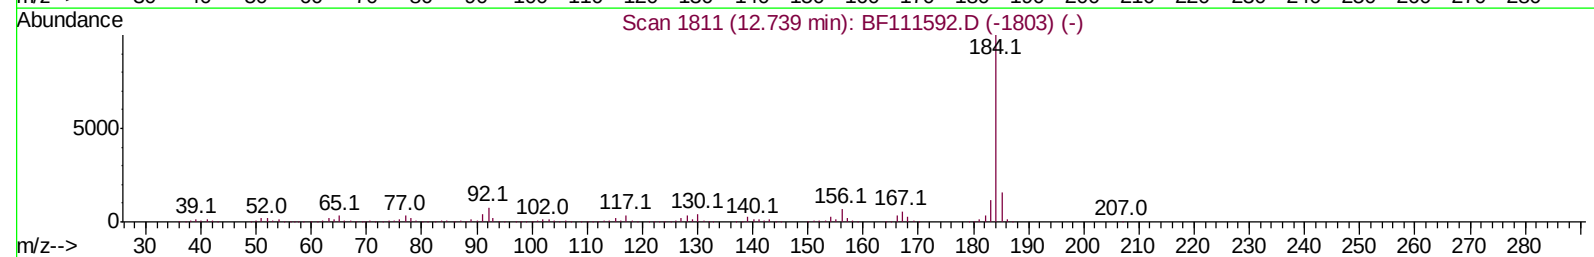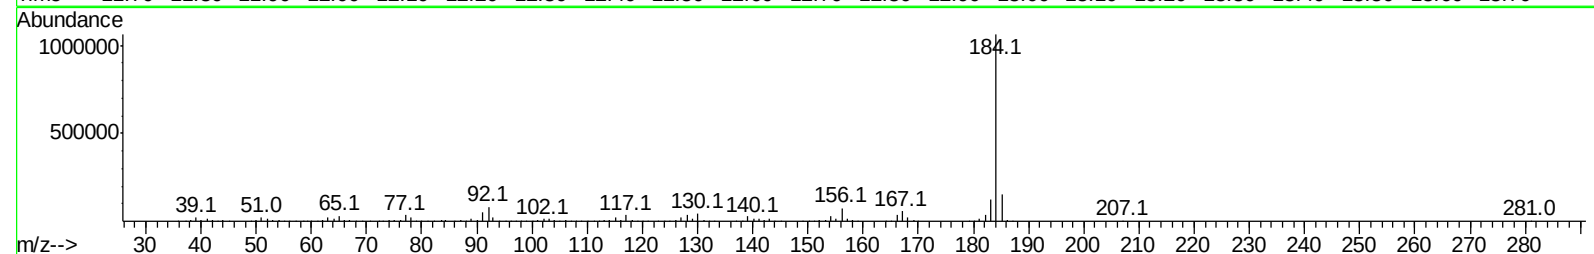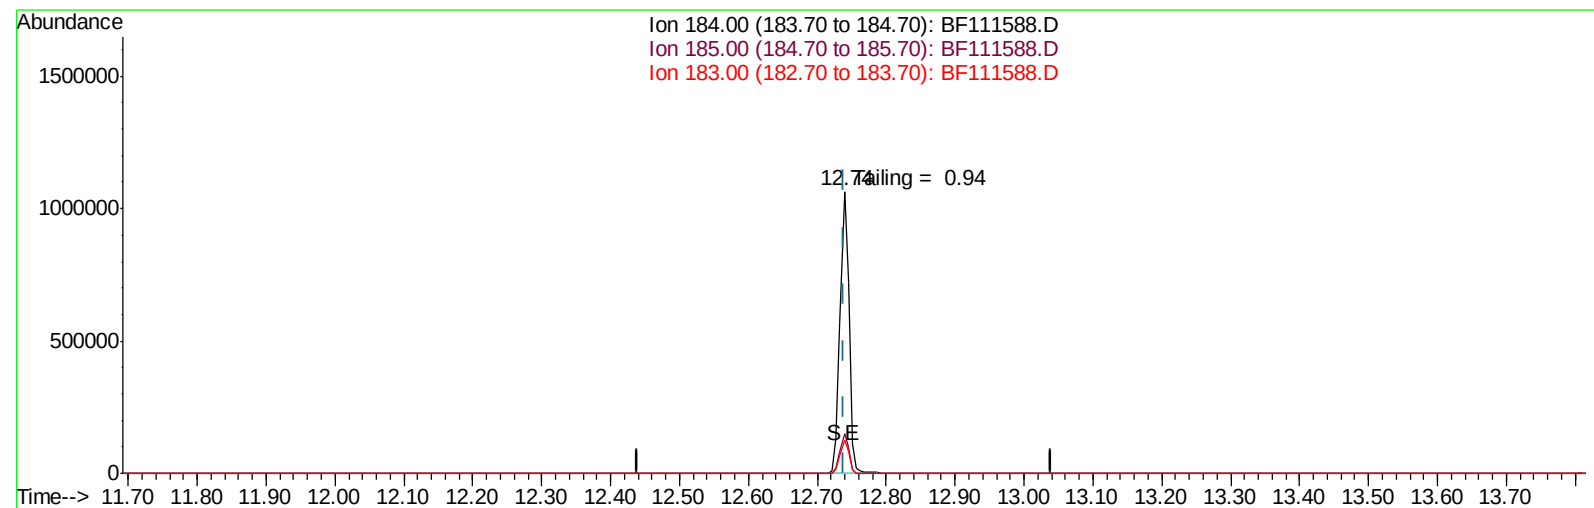

TIC: BF111588.D

(77) Benzidine

12.739min (-0.000) 0.00ng

response 937730

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.30
183.00	11.60	11.77
0.00	0.00	0.00