

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
 Data File : BF111609.D
 Acq On : 20 Dec 2018 00:01
 Operator : JU/SJ
 Sample : J6194-09 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-121818-B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	13	16	24	rVB2	54130	83412	3.32%	0.228%
2	5.104	509	513	517	rBV	109338	114862	4.57%	0.314%
3	5.510	577	582	585	rBV	2181948	2143956	85.22%	5.867%
4	6.510	747	752	757	rBV	2625139	2515872	100.00%	6.885%
5	6.657	773	777	781	rBV	2388015	2288073	90.95%	6.261%
6	6.892	814	817	821	rBV	1633069	1317222	52.36%	3.605%
7	7.051	840	844	847	rBV	2108587	1689097	67.14%	4.622%
8	7.445	905	911	915	rBV	1584990	1378416	54.79%	3.772%
9	8.175	1031	1035	1038	rBV	2167692	1824057	72.50%	4.992%
10	8.198	1038	1039	1042	rVB	233317	107817	4.29%	0.295%
11	8.775	1133	1137	1140	rBV2	31118	30021	1.19%	0.082%
12	8.886	1151	1156	1160	rVB	179369	143479	5.70%	0.393%
13	8.986	1168	1173	1177	rBV	153166	118009	4.69%	0.323%
14	9.251	1214	1218	1221	rVB	2814478	2381343	94.65%	6.517%
15	9.345	1229	1234	1238	rBV2	53728	73669	2.93%	0.202%
16	9.510	1259	1262	1266	rBV2	69452	88443	3.52%	0.242%
17	9.586	1270	1275	1278	rBV	118074	117211	4.66%	0.321%
18	9.616	1278	1280	1281	rVV	74628	56148	2.23%	0.154%
19	9.639	1281	1284	1290	rVB	307690	265841	10.57%	0.727%
20	9.704	1292	1295	1306	rVB	61182	78890	3.14%	0.216%
21	9.786	1306	1309	1312	rBV	168866	141732	5.63%	0.388%
22	9.928	1327	1333	1337	rBV2	2072292	1886238	74.97%	5.162%
23	9.963	1337	1339	1342	rVB2	54707	44029	1.75%	0.120%
24	10.033	1348	1351	1356	rBV3	22955	31829	1.27%	0.087%
25	10.133	1364	1368	1371	rVB	128568	124474	4.95%	0.341%
26	10.169	1371	1374	1377	rBV	49074	42047	1.67%	0.115%
27	10.245	1384	1387	1390	rVB2	35352	32967	1.31%	0.090%
28	10.275	1390	1392	1395	rVB	38544	27381	1.09%	0.075%
29	10.333	1398	1402	1404	rBV4	30791	42615	1.69%	0.117%
30	10.363	1404	1407	1412	rVB3	30495	46576	1.85%	0.127%
31	10.475	1423	1426	1432	rVB	263930	232981	9.26%	0.638%
32	10.539	1432	1437	1439	rBV5	25038	34077	1.35%	0.093%
33	10.633	1450	1453	1458	rVB2	41921	44366	1.76%	0.121%
34	10.710	1462	1466	1470	rBV	1754112	1442379	57.33%	3.947%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121918\
 Data File : BF111609.D
 Acq On : 20 Dec 2018 00:01
 Operator : JU/SJ
 Sample : J6194-09 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-121818-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.839	1485	1488	1494	rVB3	74147	94373	3.75%	0.258%
36	10.916	1498	1501	1506	rBV4	21203	32482	1.29%	0.089%
37	11.022	1515	1519	1521	rBV	62578	68345	2.72%	0.187%
38	11.051	1521	1524	1526	rVV3	52838	46073	1.83%	0.126%
39	11.104	1530	1533	1537	rVB	38559	34724	1.38%	0.095%
40	11.304	1565	1567	1574	rVB2	83320	103533	4.12%	0.283%
41	11.410	1581	1585	1587	rBV	1854391	1580439	62.82%	4.325%
42	11.433	1587	1589	1592	rVV	1051663	801628	31.86%	2.194%
43	11.486	1592	1598	1600	rVV	208569	191541	7.61%	0.524%
44	11.516	1600	1603	1607	rVV2	46863	53887	2.14%	0.147%
45	11.633	1618	1623	1626	rBV2	68919	79140	3.15%	0.217%
46	11.710	1633	1636	1638	rBV	49075	35616	1.42%	0.097%
47	11.739	1639	1641	1644	rVB2	59503	46737	1.86%	0.128%
48	11.804	1650	1652	1654	rBV2	31884	36175	1.44%	0.099%
49	11.863	1659	1662	1665	rBV5	23961	36148	1.44%	0.099%
50	11.910	1667	1670	1672	rVV	193071	179599	7.14%	0.491%
51	11.939	1672	1675	1679	rVV	366283	324662	12.90%	0.888%
52	11.986	1680	1683	1686	rVV	79113	77859	3.09%	0.213%
53	12.022	1686	1689	1692	rVV2	284505	329469	13.10%	0.902%
54	12.045	1692	1693	1697	rVB	152476	89461	3.56%	0.245%
55	12.145	1707	1710	1713	rVB3	32336	29980	1.19%	0.082%
56	12.204	1718	1720	1722	rBV	100162	84767	3.37%	0.232%
57	12.339	1740	1743	1744	rBV2	38686	37146	1.48%	0.102%
58	12.357	1744	1746	1748	rVV	57255	44565	1.77%	0.122%
59	12.386	1748	1751	1753	rVV	82941	74011	2.94%	0.203%
60	12.410	1753	1755	1758	rVB2	61659	50371	2.00%	0.138%
61	12.463	1760	1764	1766	rBV	171064	171732	6.83%	0.470%
62	12.492	1766	1769	1771	rVV3	141943	175444	6.97%	0.480%
63	12.545	1775	1778	1782	rVV4	57946	78209	3.11%	0.214%
64	12.622	1788	1791	1794	rVB	1031524	834557	33.17%	2.284%
65	12.669	1795	1799	1801	rBV2	45337	63578	2.53%	0.174%
66	12.716	1804	1807	1810	rBV	80505	76813	3.05%	0.210%
67	12.774	1814	1817	1820	rVV3	41807	47985	1.91%	0.131%
68	12.851	1824	1830	1832	rBV	911004	937405	37.26%	2.565%
69	12.874	1832	1834	1836	rVV2	79459	71497	2.84%	0.196%
70	12.910	1836	1840	1843	rVB3	65768	82740	3.29%	0.226%
71	12.969	1847	1850	1851	rVV2	50493	55632	2.21%	0.152%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121918\
 Data File : BF111609.D
 Acq On : 20 Dec 2018 00:01
 Operator : JU/SJ
 Sample : J6194-09 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-01-121818-B

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	12.992	1851	1854	1862	rVB	2148969	1836956	73.01%	5.027%
73	13.069	1862	1867	1870	rBV3	103872	170966	6.80%	0.468%
74	13.121	1874	1876	1878	rBV2	37033	32934	1.31%	0.090%
75	13.174	1883	1885	1888	rVB	215526	185625	7.38%	0.508%
76	13.239	1893	1896	1899	rVB2	154288	158063	6.28%	0.433%
77	13.280	1900	1903	1906	rBV2	162645	149847	5.96%	0.410%
78	13.374	1916	1919	1921	rVB	116348	97130	3.86%	0.266%
79	13.404	1921	1924	1927	rBV	126410	113831	4.52%	0.311%
80	13.574	1951	1953	1956	rBV3	61833	67968	2.70%	0.186%
81	13.792	1986	1990	1993	rBV2	100686	155926	6.20%	0.427%
82	13.821	1993	1995	1997	rVV	78046	62463	2.48%	0.171%
83	13.845	1997	1999	2003	rVV3	67269	84500	3.36%	0.231%
84	13.892	2004	2007	2011	rVB4	156961	215360	8.56%	0.589%
85	14.045	2028	2033	2035	rBV2	1799565	1986373	78.95%	5.436%
86	14.068	2035	2037	2043	rVB	499202	401666	15.97%	1.099%
87	14.463	2102	2104	2107	rBV	85814	71464	2.84%	0.196%
88	14.521	2112	2114	2117	rVV2	174856	156439	6.22%	0.428%
89	14.833	2165	2167	2170	rBV	98071	82008	3.26%	0.224%
90	15.086	2206	2210	2221	rVB	343694	775375	30.82%	2.122%
91	15.392	2259	2262	2267	rVB	202330	270063	10.73%	0.739%
92	15.451	2269	2272	2276	rVB	266563	305702	12.15%	0.837%
93	15.515	2279	2283	2287	rVV	801490	1014494	40.32%	2.776%


Sum of corrected areas: 36543005

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

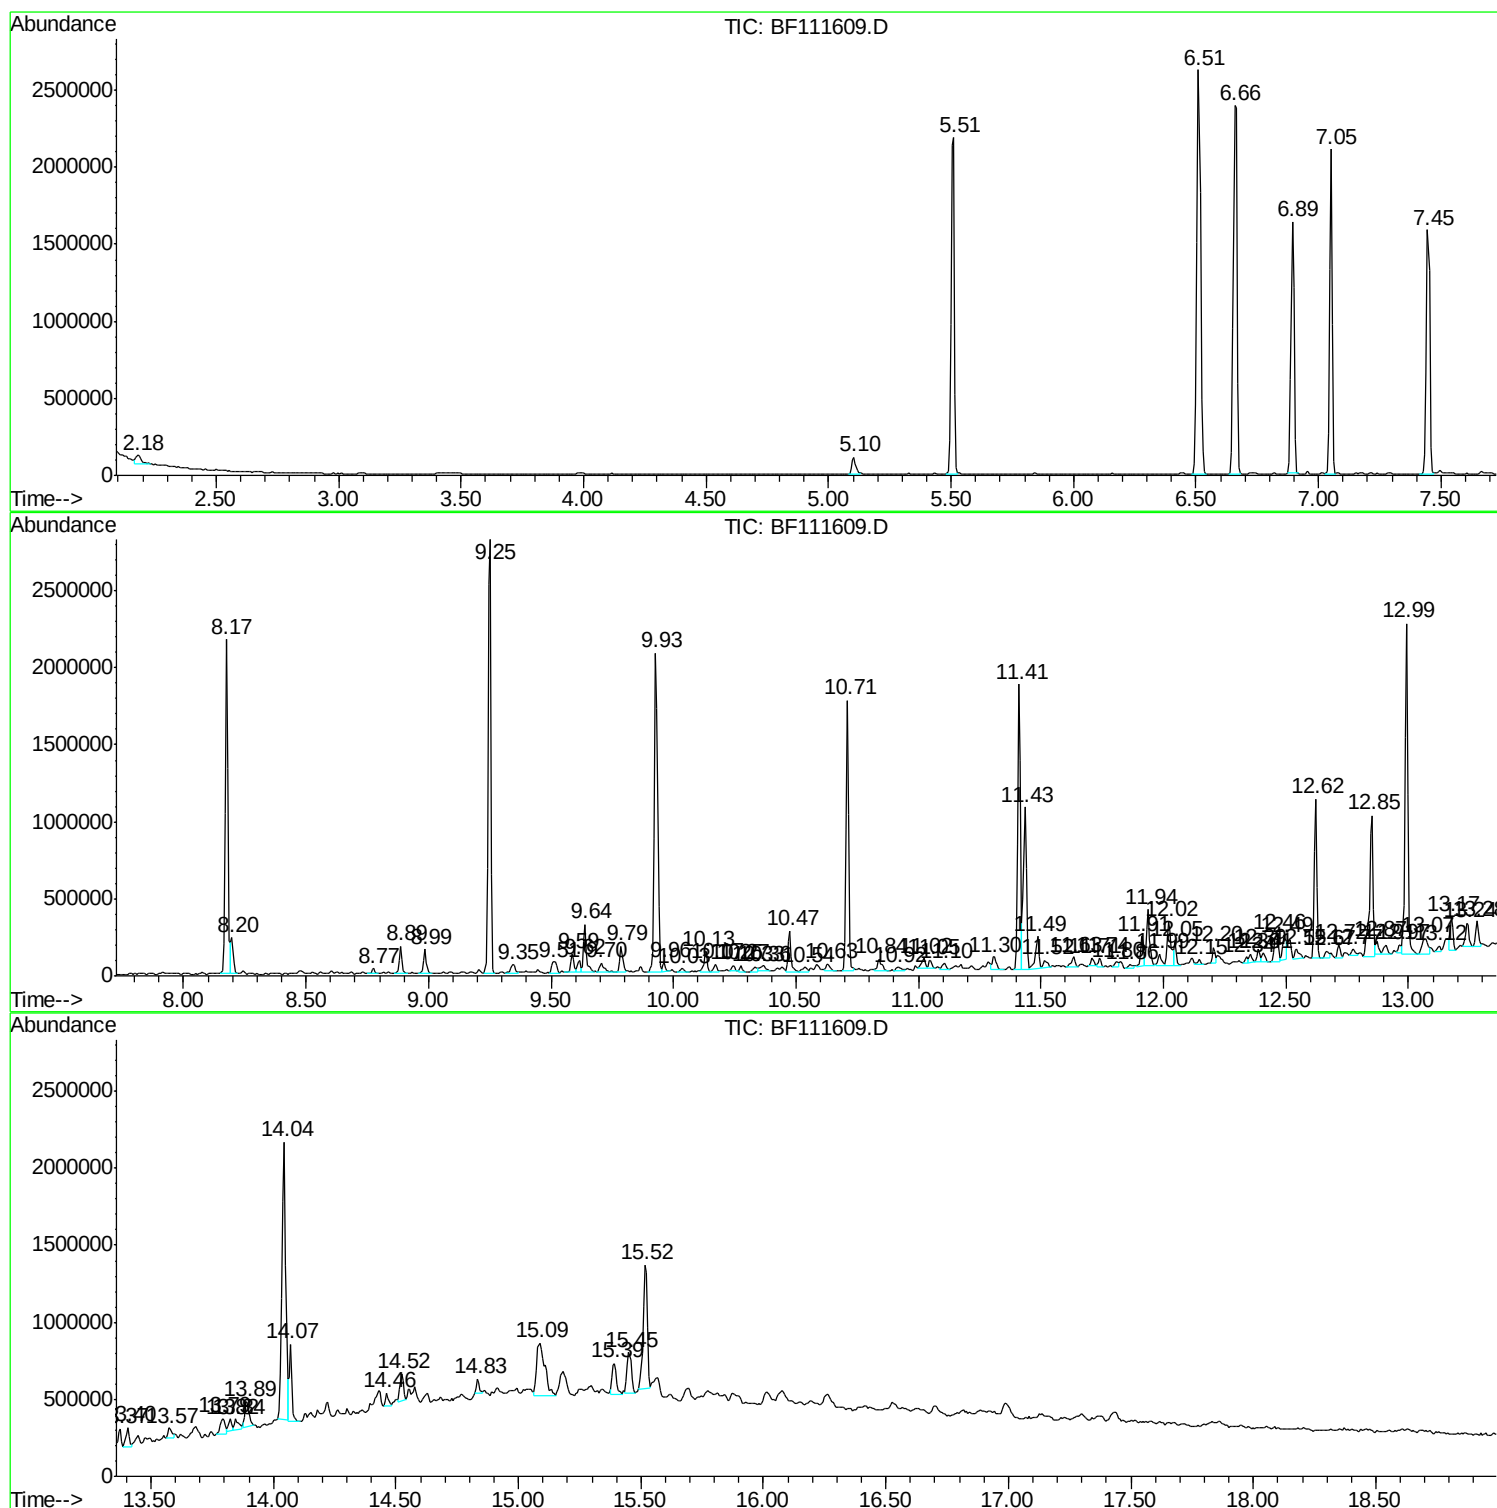

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.66 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.66	34.74 ng	2288070	1,4-Dichlorobenzene-d4	6.89

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

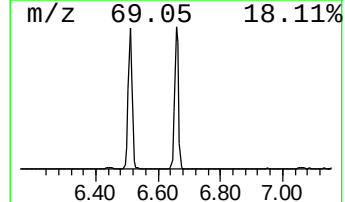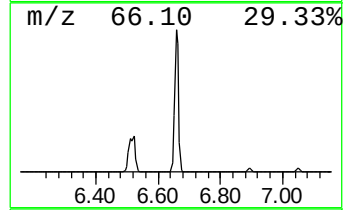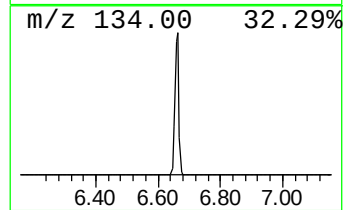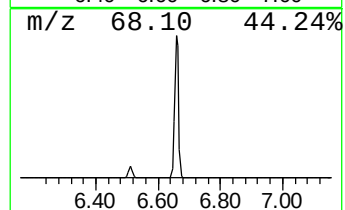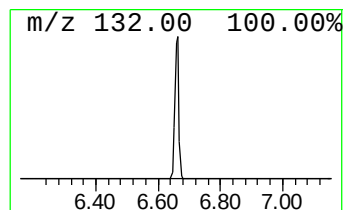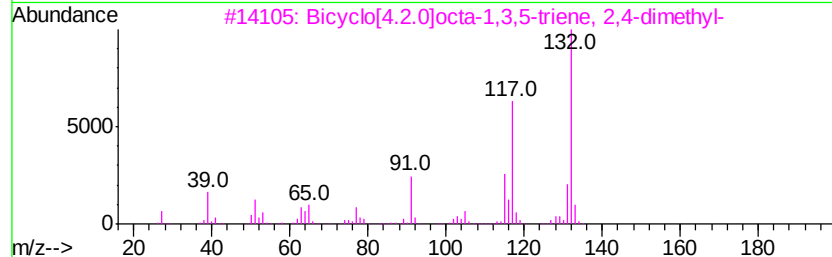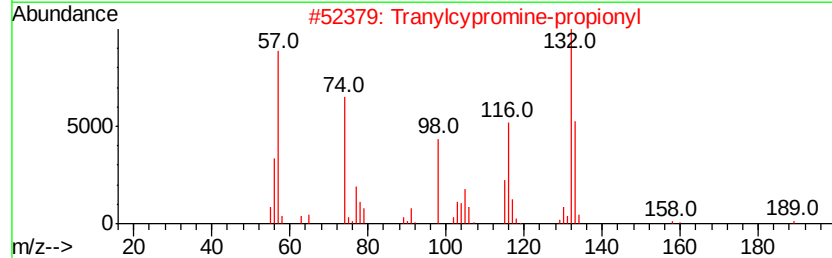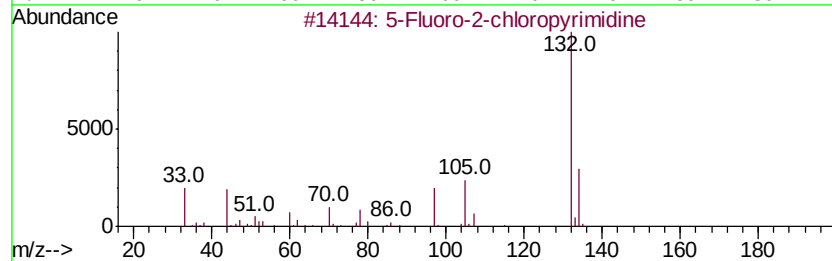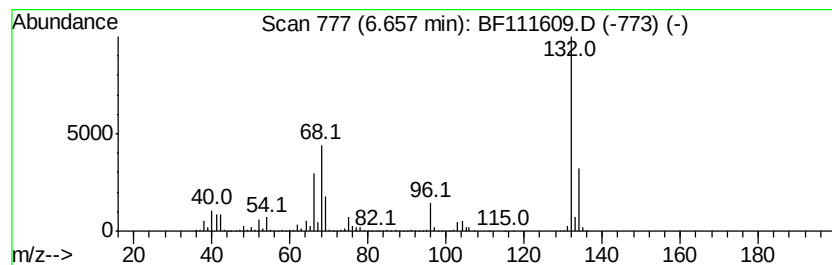

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Anthracene, 2-methyl- Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.91	2.27 ng	179599	Phenanthrene-d10	11.41	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Anthracene, 2-methyl-	192	C15H12	000613-12-7	95
2	Phenanthrene, 2-methyl-	192	C15H12	002531-84-2	94
3	Anthracene, 9-methyl-	192	C15H12	000779-02-2	93
4	Anthracene, 1-methyl-	192	C15H12	000610-48-0	91
5	Phenanthrene, 1-methyl-	192	C15H12	000832-69-9	90

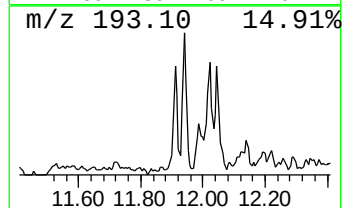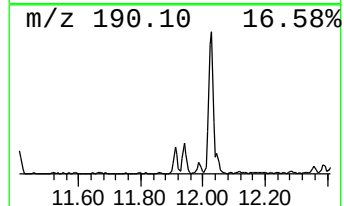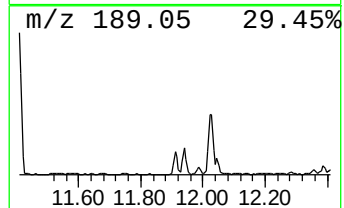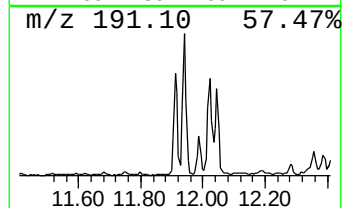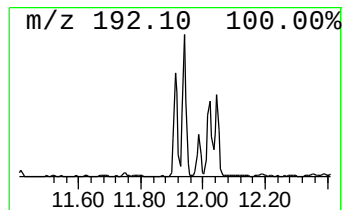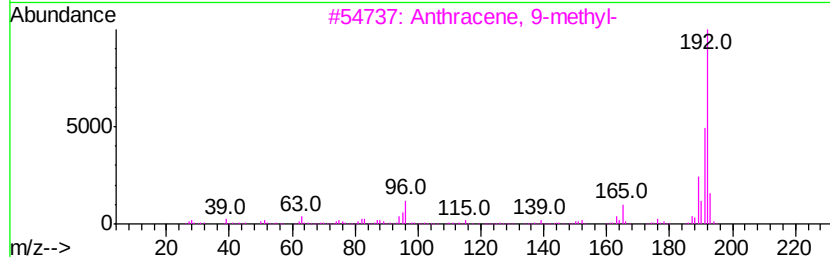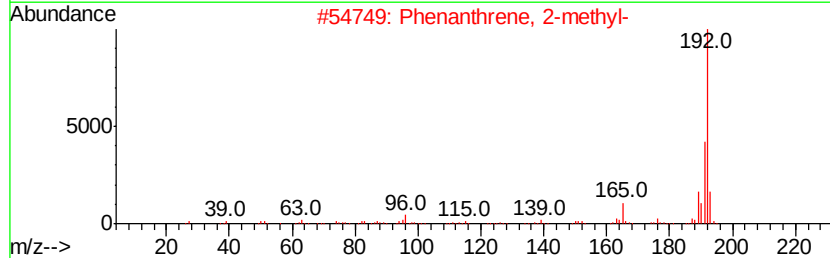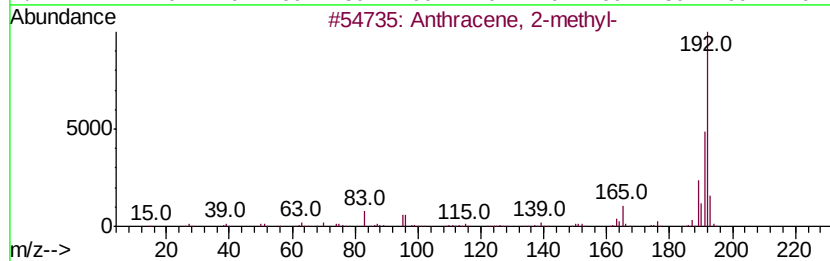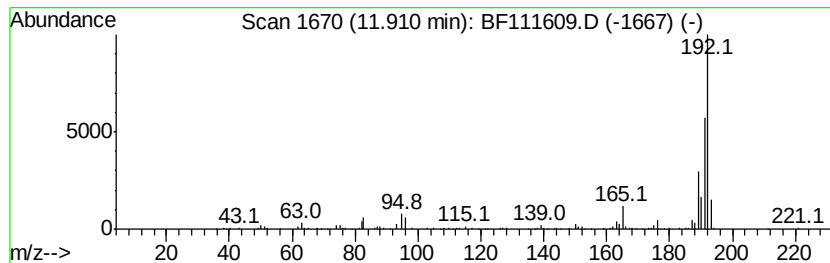

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Anthracene, 9-methyl- Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.	
11.94	4.11 ng	324662	Phenanthrene-d10	11.41	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Anthracene, 2-methyl-	192	C15H12	000613-12-7	97
2	Phenanthrene, 1-methyl-	192	C15H12	000832-69-9	96
3	Anthracene, 9-methyl-	192	C15H12	000779-02-2	96
4	5H-Dibenzo[<i>a,d</i>]cycloheptene	192	C15H12	000256-81-5	96
5	Phenanthrene, 2-methyl-	192	C15H12	002531-84-2	96

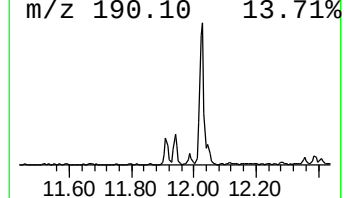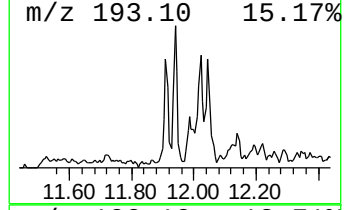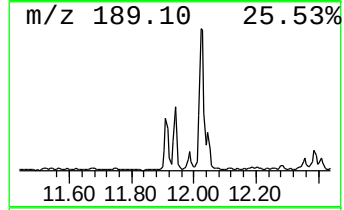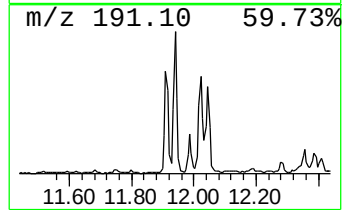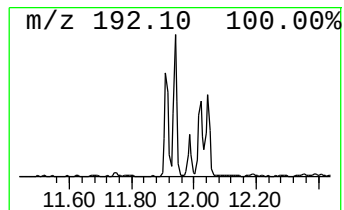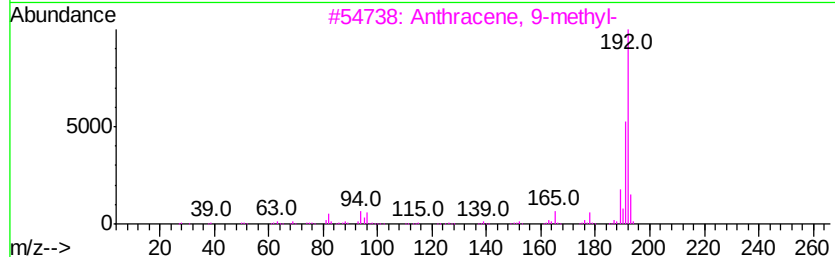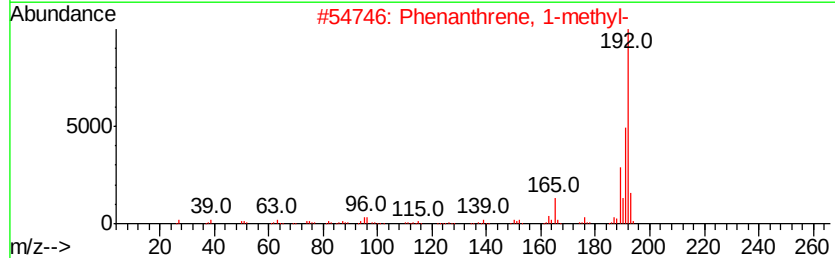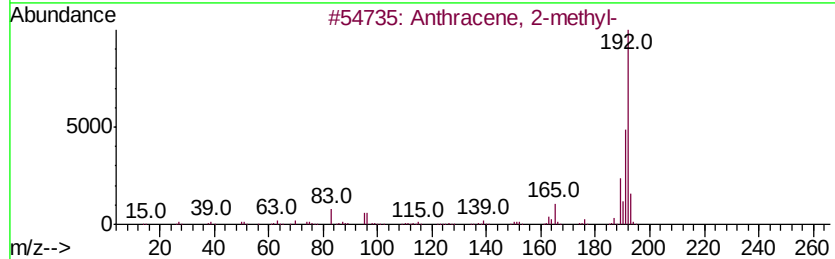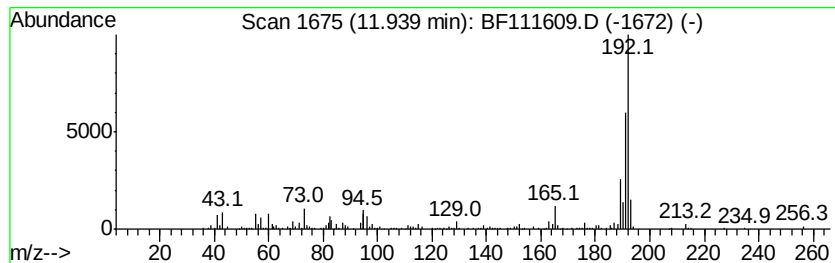

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Benzaldehyde, 3,5-dichloro-... Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.	
12.02	4.17 ng	329469	Phenanthrene-d10	11.41	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Benzaldehyde, 3,5-dichloro-2-hyd...	190	C7H4Cl2O2	000090-60-8	72
2	4H-Cyclopenta[def]phenanthrene	190	C15H10	000203-64-5	60
3	6H-Cyclobuta[f]kphenanthrene	190	C15H10	083469-43-6	49
4	Anthracene, 1-methyl-	192	C15H12	000610-48-0	42
5	Anthracene, 2-methyl-	192	C15H12	000613-12-7	41

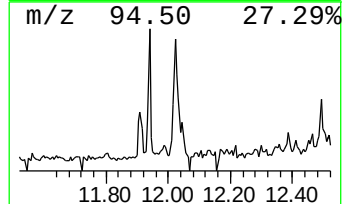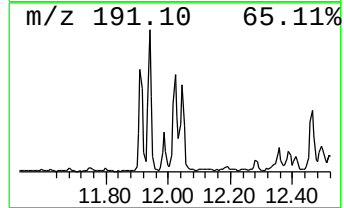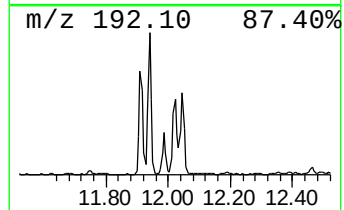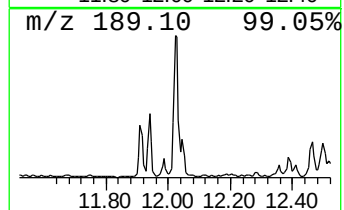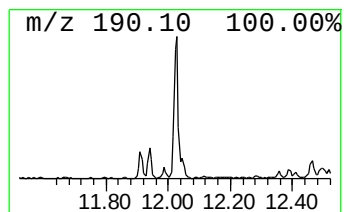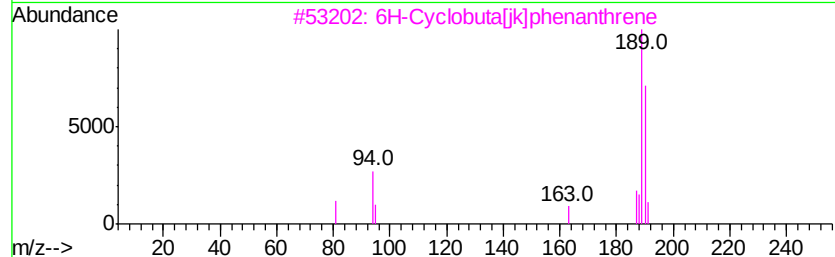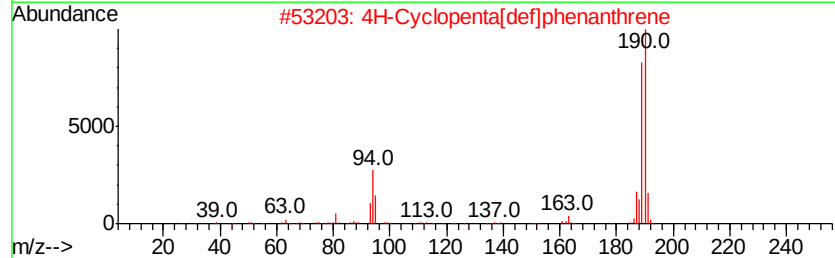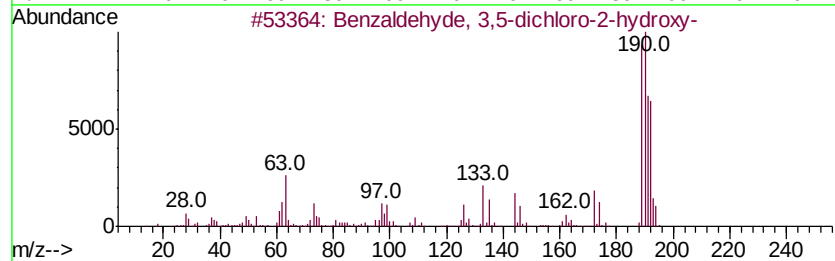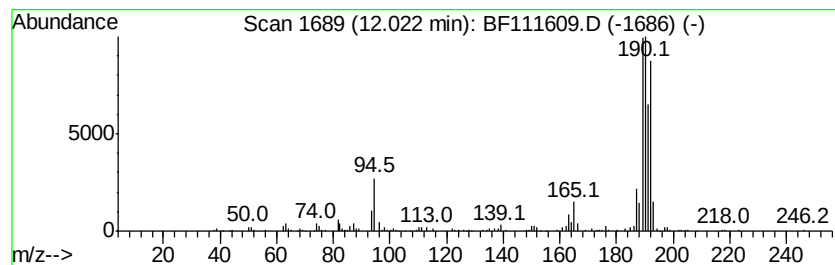

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Phenanthrene, 2,5-dimethyl- Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD		R.T.
12.46	2.17 ng	171732	Phenanthrene-d10		11.41
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Phenanthrene, 2,5-dimethyl-	206	C16H14	003674-66-6	93
2	Phenanthrene, 2,3-dimethyl-	206	C16H14	003674-65-5	87
3	9,10-Dimethylantracene	206	C16H14	000781-43-1	87
4	di-p-Tolylacetylene	206	C16H14	002789-88-0	87
5	Phenanthrene, 3,6-dimethyl-	206	C16H14	001576-67-6	81

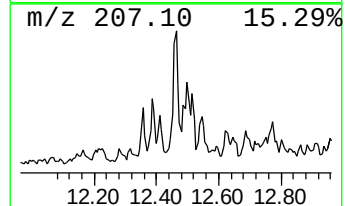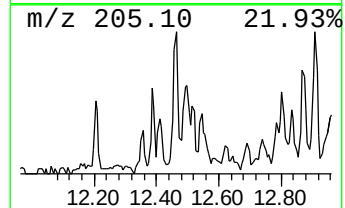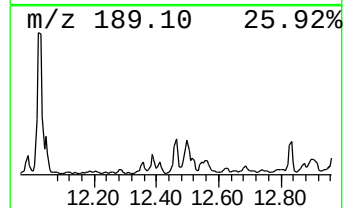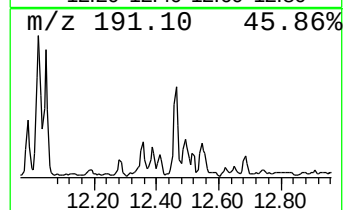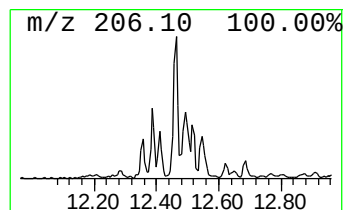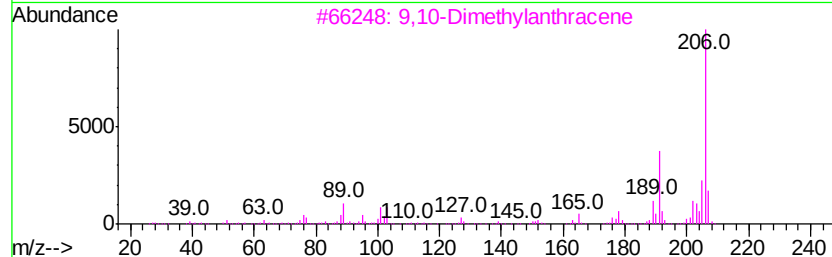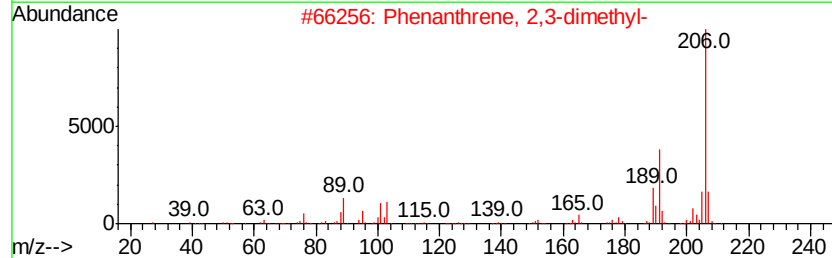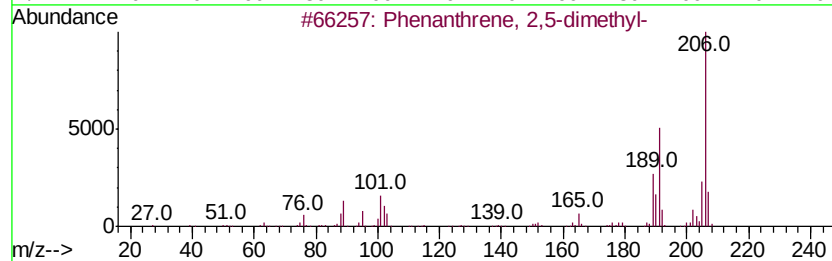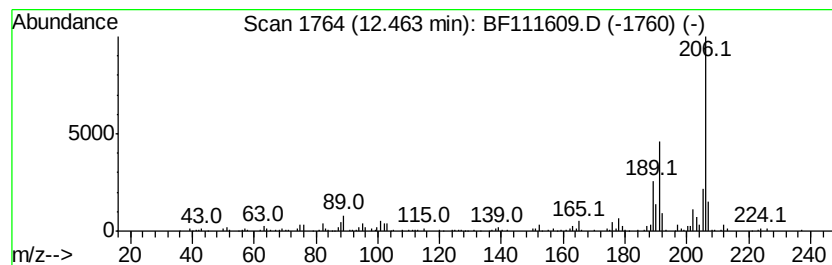

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 di-p-Tolylacetylene Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.49	2.22 ng	175444	Phenanthrene-d10	11.41

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		di-p-Tolylacetylene	206	C16H14	002789-88-0	55
2		Phenanthrene, 3,6-dimethyl-	206	C16H14	001576-67-6	46
3		9,10-Dimethylantracene	206	C16H14	000781-43-1	45
4		Phenanthrene, 2,7-dimethyl-	206	C16H14	001576-69-8	45
5		Phenanthrene, 1,7-dimethyl-	206	C16H14	000483-87-4	43

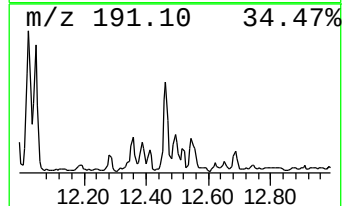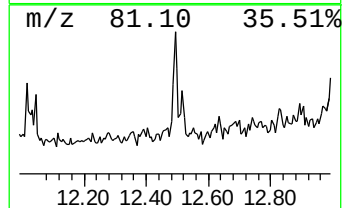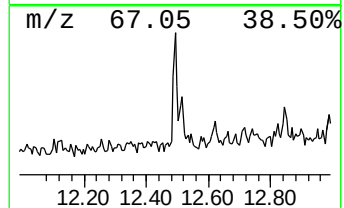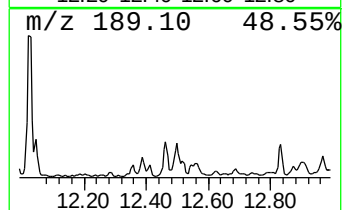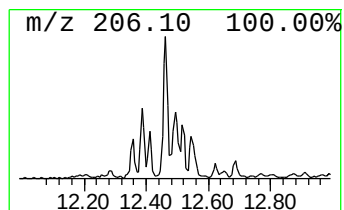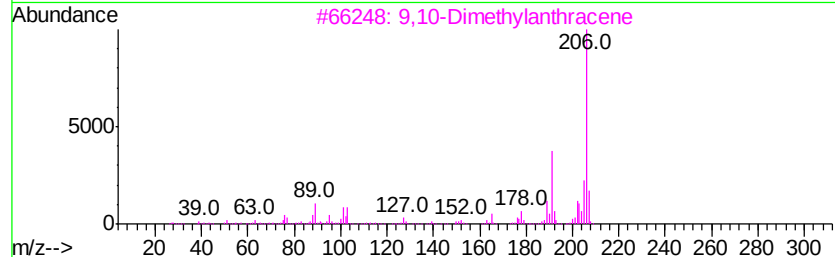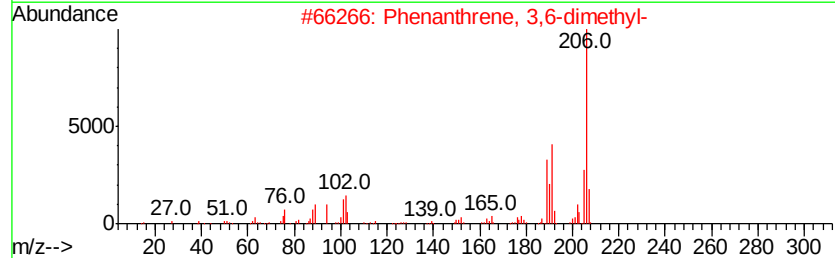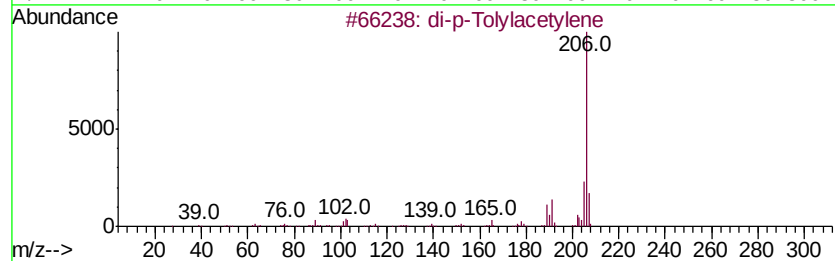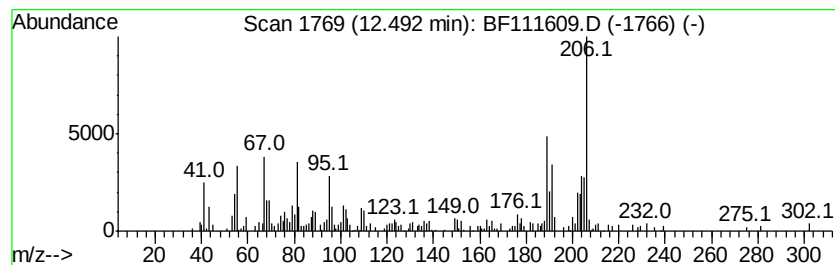

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 1-Docosene Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.89	2.17 ng	215360	Chrysene-d12	14.05	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Docosene	308	C22H44	001599-67-3	97
2	Heptafluorobutyric acid, hexadec...	438	C20H33F7O2	006385-15-5	90
3	Cyclotetracosane	336	C24H48	000297-03-0	87
4	1-Heneicosanol	312	C21H44O	015594-90-8	86
5	9-Nonadecene	266	C19H38	031035-07-1	83

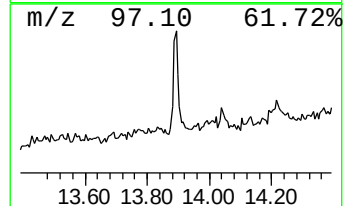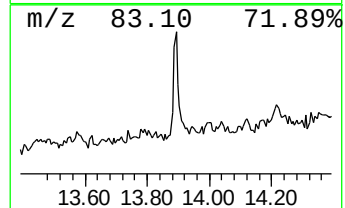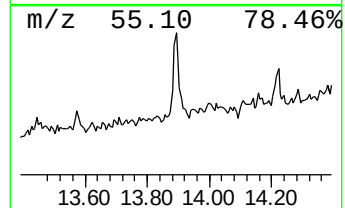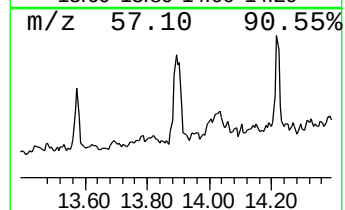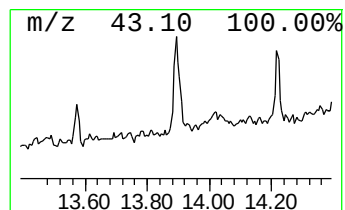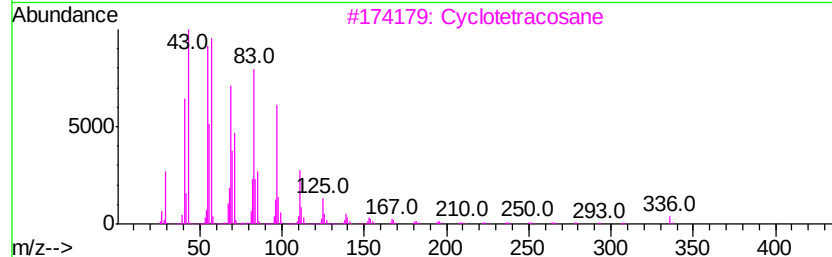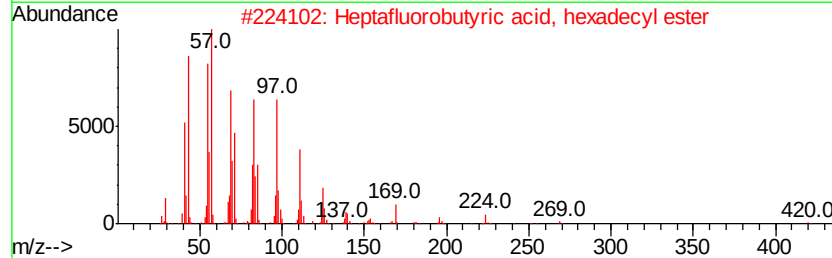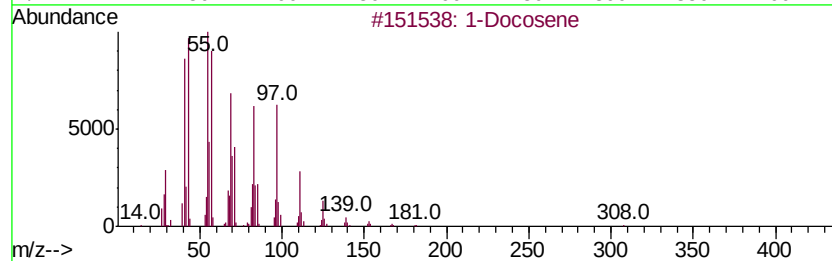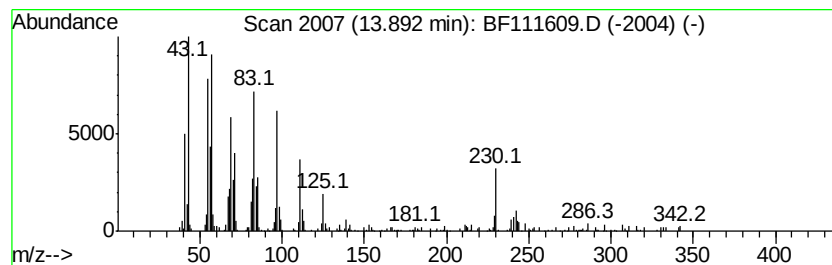

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121918\
Data File : BF111609.D
Acq On : 20 Dec 2018 00:01
Operator : JU/SJ
Sample : J6194-09 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-01-121818-B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.66	6.66	34.7	ng	2288070	1	6.89	1317220	20.0
Anthracene, 2-met...	11.91	2.3	ng	179599	4	11.41	1580440	20.0
Anthracene, 9-met...	11.94	4.1	ng	324662	4	11.41	1580440	20.0
Benzaldehyde, 3,5...	12.02	4.2	ng	329469	4	11.41	1580440	20.0
Phenanthrene, 2,5...	12.46	2.2	ng	171732	4	11.41	1580440	20.0
di-p-Tolylacetylene	12.49	2.2	ng	175444	4	11.41	1580440	20.0
1-Docosene	13.89	2.2	ng	215360	5	14.05	1986370	20.0