


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121918\
 Data File : BF111597.D
 Acq On : 19 Dec 2018 18:26
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

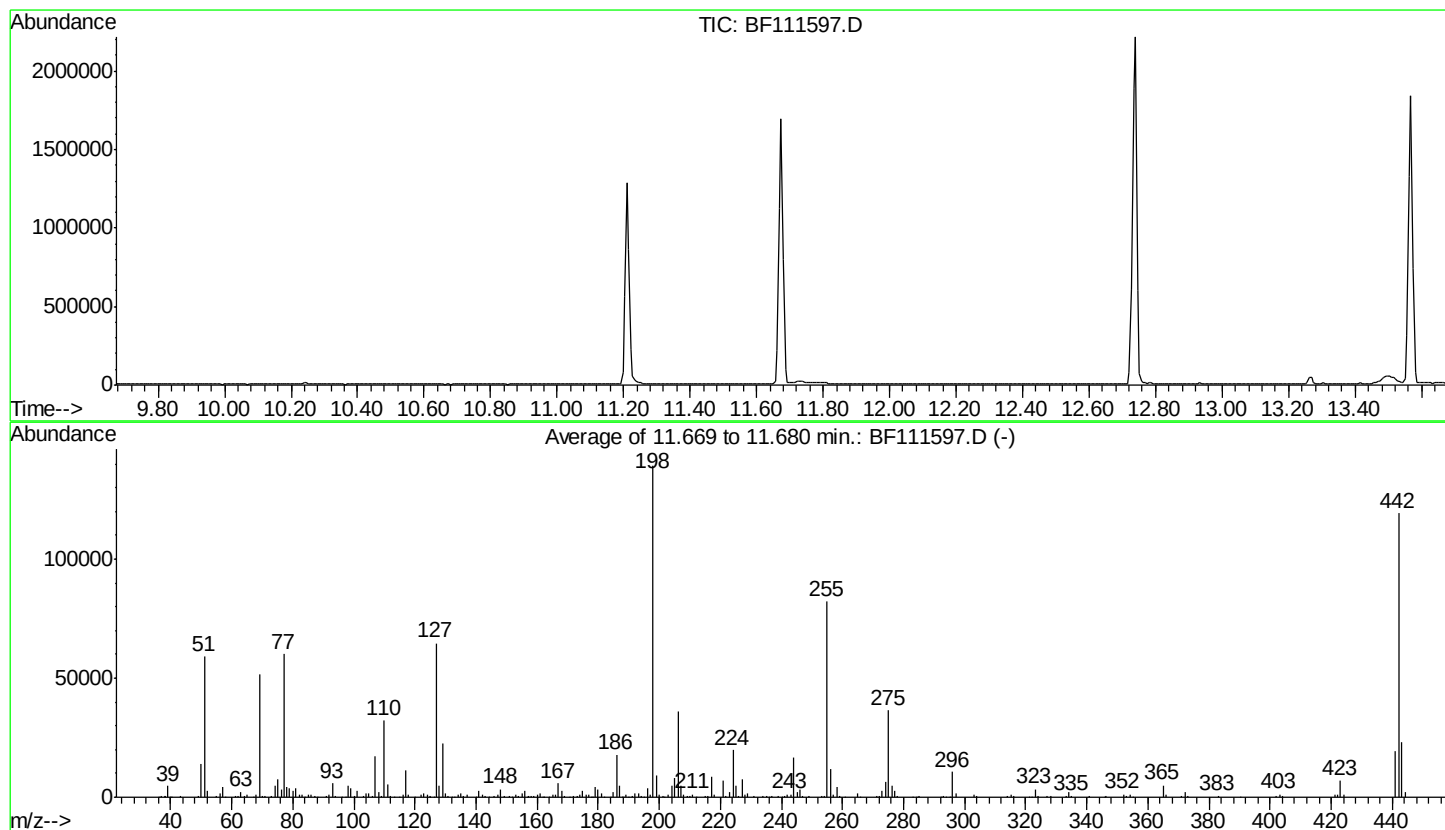

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	59077	PASS
68	69	0.00	2	1.9	963	PASS
69	198	0.00	100	36.9	51378	PASS
70	69	0.00	2	0.8	428	PASS
127	198	10	80	46.4	64637	PASS
197	198	0.00	2	0.7	1025	PASS
198	198	100	100	100.0	139256	PASS
199	198	5	9	6.6	9193	PASS
275	198	10	60	26.1	36325	PASS
365	198	1	100	3.6	5058	PASS
441	198	0.01	100	13.8	19235	PASS
442	198	50	100	85.5	119130	PASS
443	442	15	24	19.4	23135	PASS