

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121919\
 Data File : BF118280.D
 Acq On : 19 Dec 2019 15:34
 Operator : JU
 Sample : PB125583TB
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Dec 20 02:11:47 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 06 17:34:43 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.86	152	124045	20.00	ng	-0.01
21) Naphthalene-d8	8.15	136	479234	20.00	ng	-0.01
39) Acenaphthene-d10	9.90	164	258765	20.00	ng	-0.02
64) Phenanthrene-d10	11.40	188	494874	20.00	ng	-0.01
76) Chrysene-d12	14.05	240	319854	20.00	ng	-0.02
87) Perylene-d12	15.54	264	261790	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	952923	134.55	ng	0.00
7) Phenol-d6	6.49	99	1192866	139.25	ng	0.00
23) Nitrobenzene-d5	7.43	82	715391	83.98	ng	-0.01
42) 2,4,6-Tribromophenol	10.70	330	416177	132.39	ng	-0.01
45) 2-Fluorobiphenyl	9.23	172	1499248	88.16	ng	-0.01
79) Terphenyl-d14	12.99	244	1848941	99.40	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.50	77	1671	Below Cal		Qvalue # 1
19) n-Nitroso-di-n-propylamine	7.43	70	98259	18.876	ng	# 75
25) Isophorone	7.43	82	700514	48.510	ng	# 62
51) 2,6-Dinitrotoluene	9.90	165	33339	8.022	ng	# 28
57) 2,4-Dinitrotoluene	9.90	165	33339	6.010	ng	# 25
67) 4-Bromophenyl-phenylether	10.70	248	25443	4.504	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF121919\
Data File : BF118280.D
Acq On : 19 Dec 2019 15:34
Operator : JU
Sample : PB125583TB
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Dec 20 02:11:47 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF120619.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 06 17:34:43 2019
Response via : Initial Calibration

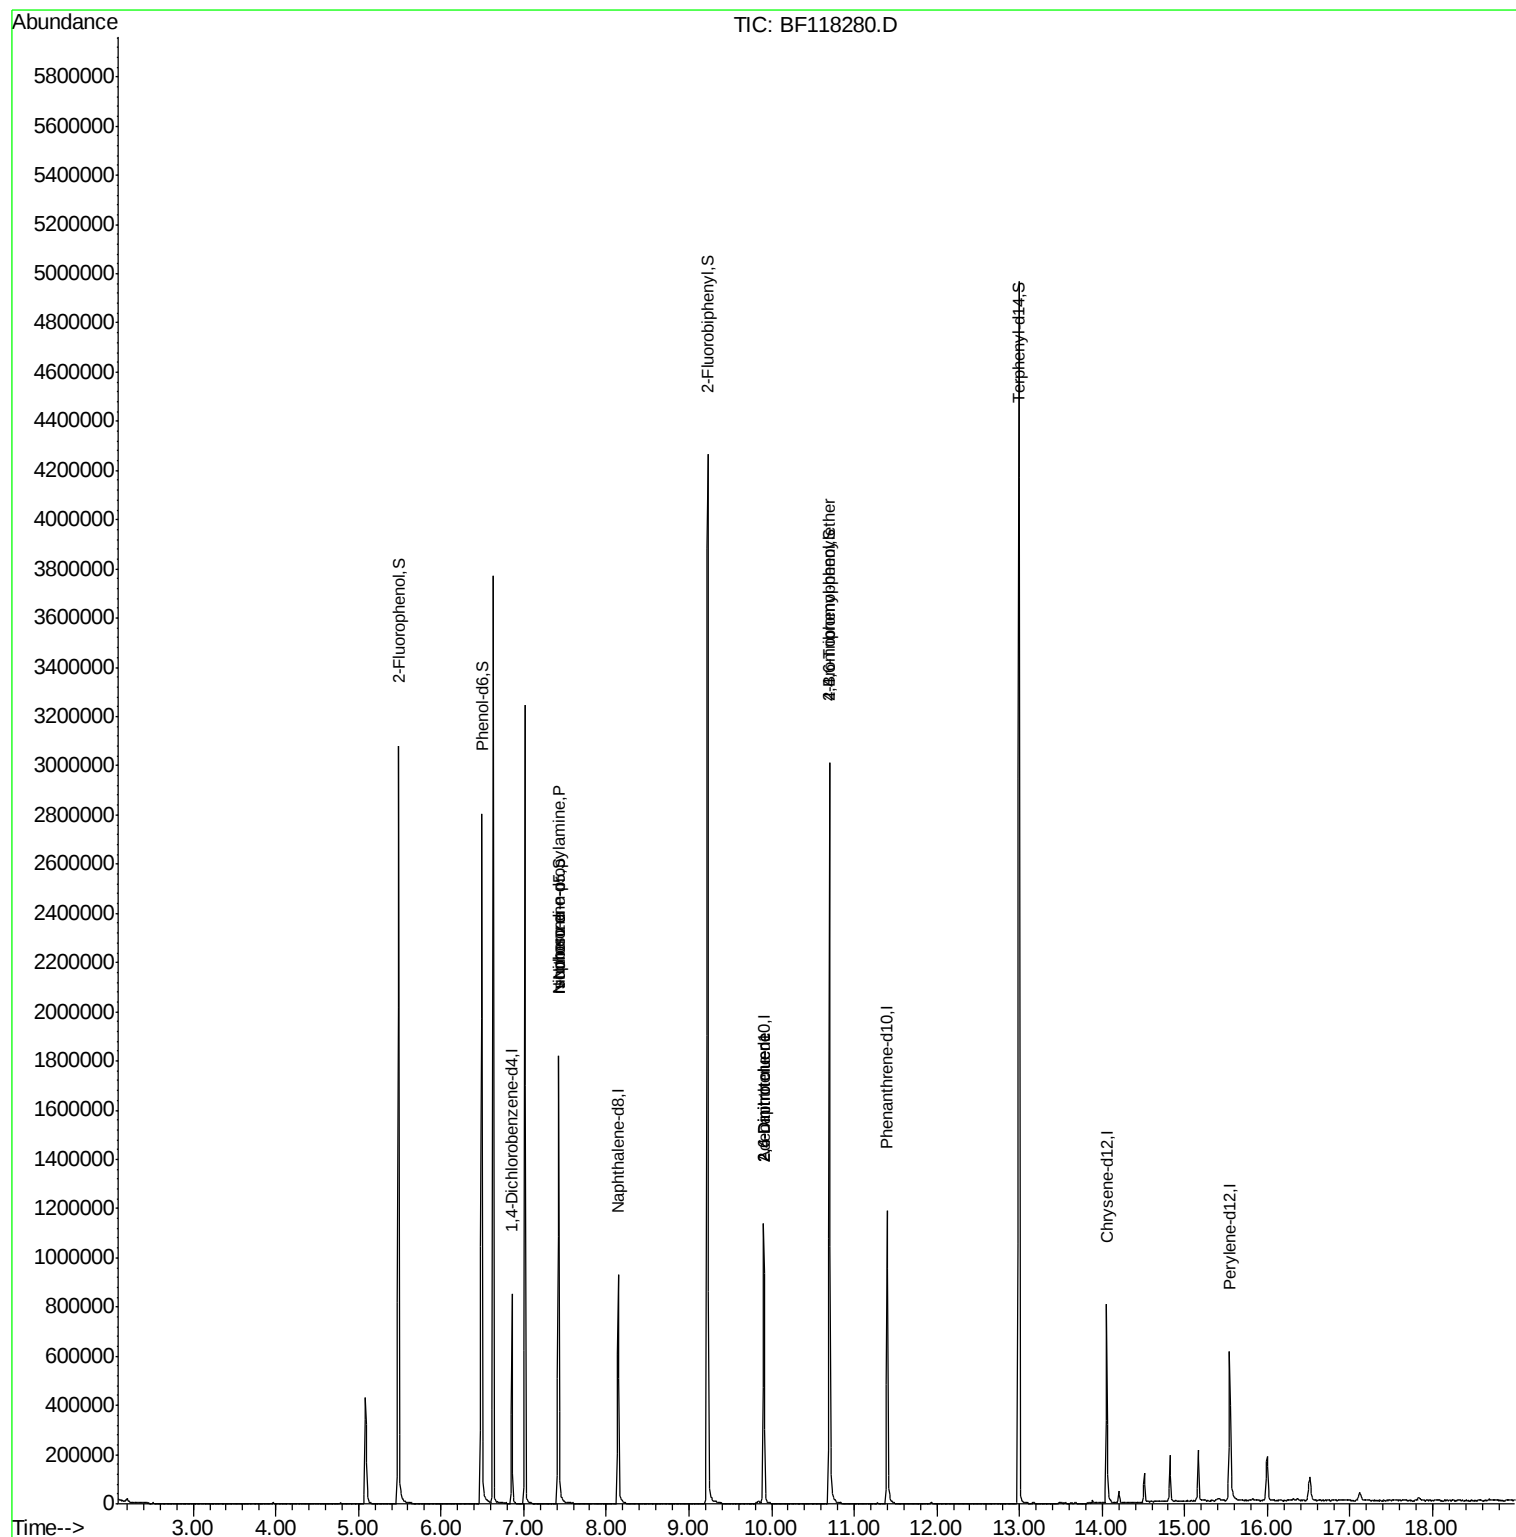




#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.86 min Scan# 811
 Delta R.T. -0.01 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
152	100		
150	152.9	128.3	192.5
115	61.5	51.1	76.7


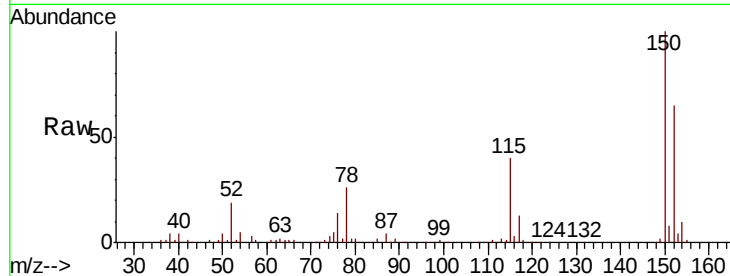


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

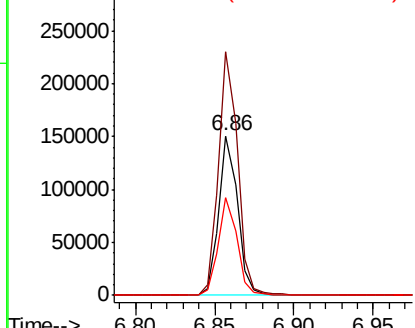

#5

2-Fluorophenol
 Concen: 134.549 ng
 RT: 5.49 min Scan# 578
 Delta R.T. 0.01 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Tgt Ion	Ratio	Lower	Upper
112	100		
64	54.0	41.3	61.9
63	29.2	22.4	33.6






Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

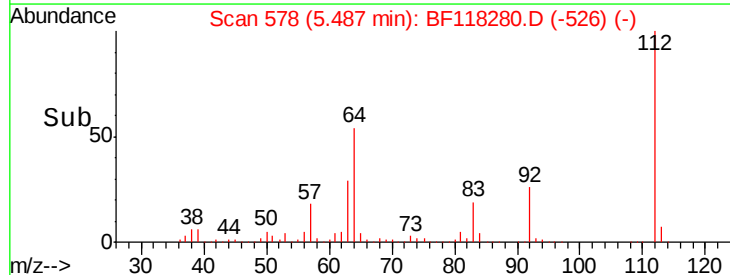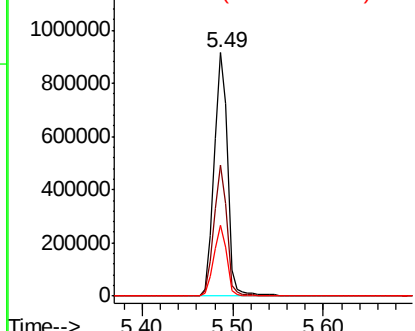

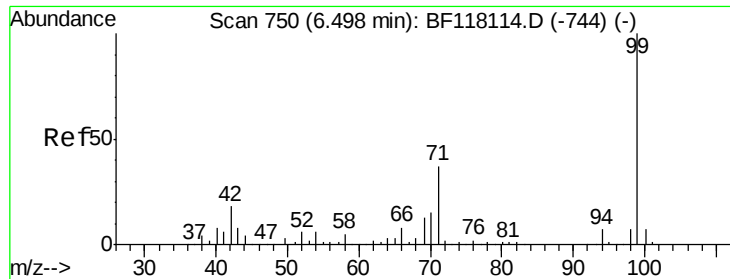

#7

Phenol-d6

Concen: 139.251 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.01 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 1192866

Ion Ratio Lower Upper

99 100

42 18.2 14.1 21.1




71 37.6 29.7 44.5

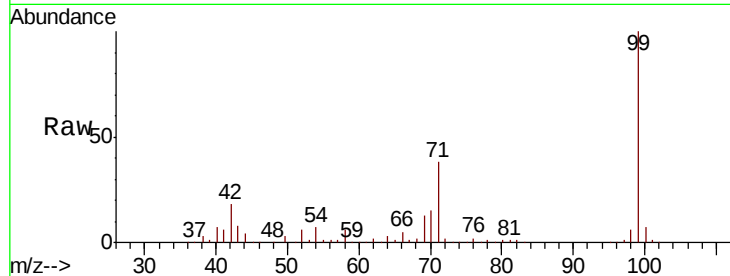

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

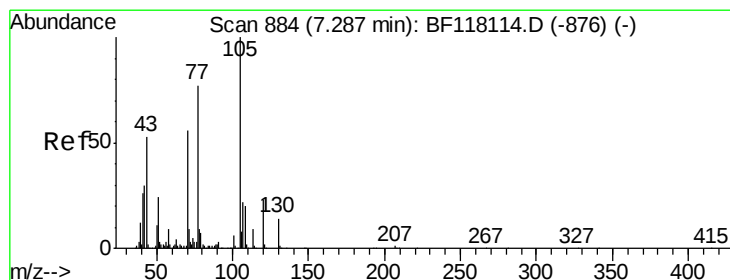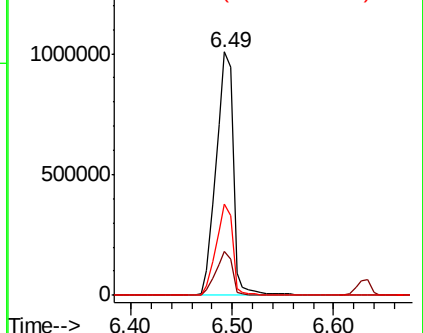

#19

n-Nitroso-di-n-propylamine

Concen: 18.876 ng

RT: 7.43 min Scan# 908

Delta R.T. 0.14 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Tgt Ion: 70 Resp: 98259


Ion Ratio Lower Upper

70 100

42 42.8 43.2 64.8#

101 0.0 8.1 12.1#

130 2.5 19.8 29.8#





Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

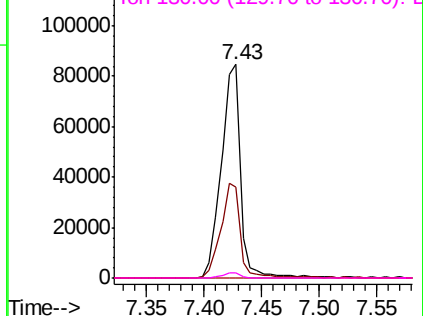



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.15 min Scan# 1030

Delta R.T. -0.01 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 479234


Ion Ratio Lower Upper

136 100

137 11.2 9.0 13.6

54 6.1 5.0 7.6

68 4.6 3.8 5.8



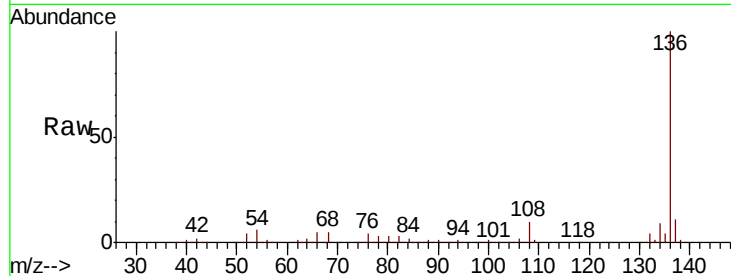


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

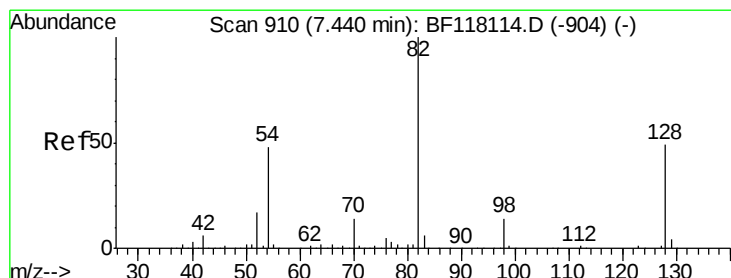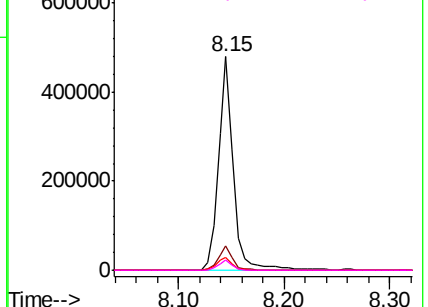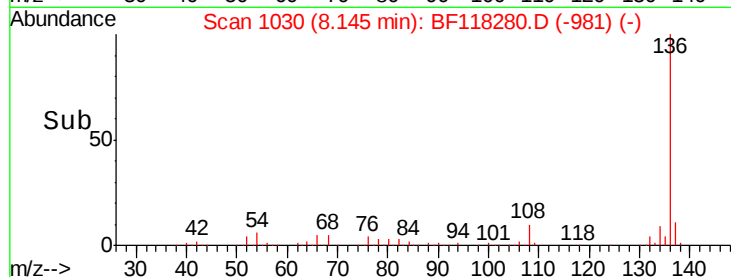

#23

Nitrobenzene-d5

Concen: 83.981 ng

RT: 7.43 min Scan# 908

Delta R.T. -0.01 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34


Tgt Ion: 82 Resp: 715391

Ion Ratio Lower Upper

82 100

128 50.0 39.1 58.7



54 46.1 38.2 57.2

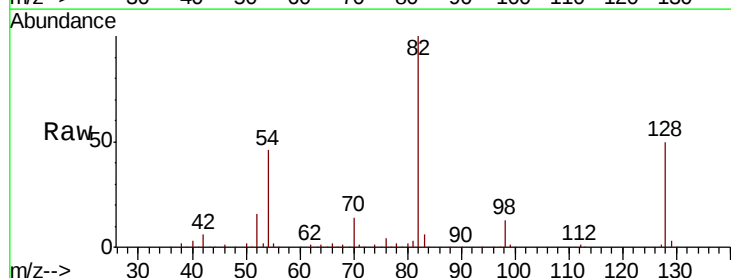


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

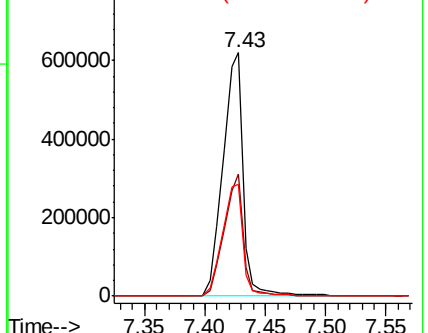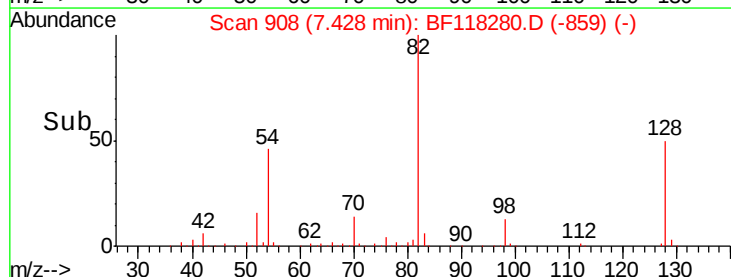

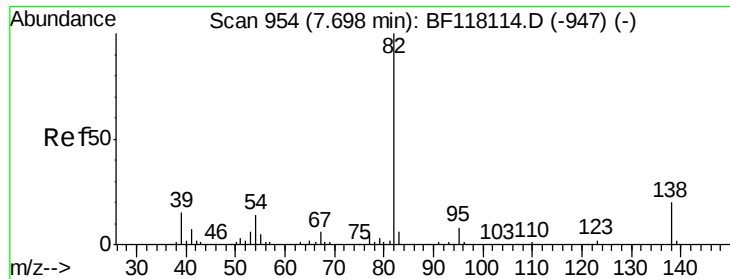

#25

Isophorone

Concen: 48.510 ng

RT: 7.43 min Scan# 908

Delta R.T. -0.27 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 700514

Ion Ratio Lower Upper




82 100

95 0.0 6.3 9.5#

138 0.0 16.3 24.5#

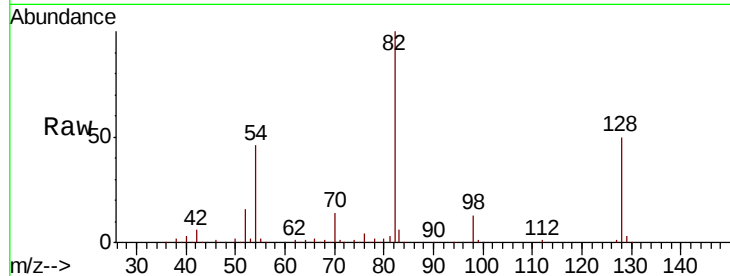

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 95.00 (94.70 to 95.70): BF1
Ion 138.00 (137.70 to 138.70): BF1

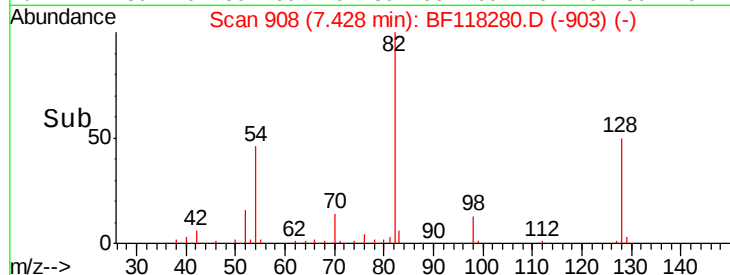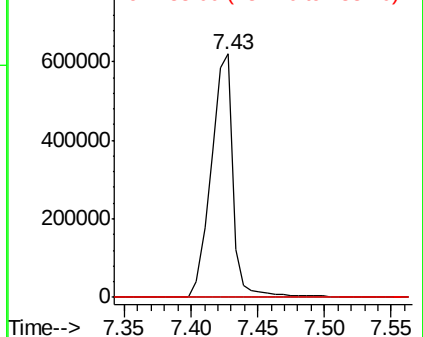

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.90 min Scan# 1329

Delta R.T. -0.02 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34


Tgt Ion: 164 Resp: 258765

Ion Ratio Lower Upper



164 100


162 105.1 83.4 125.0

160 46.3 36.6 54.8



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

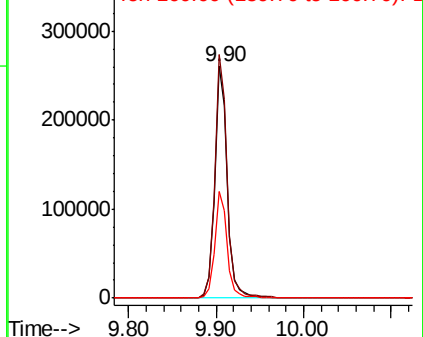







#42
 2,4,6-Tribromophenol
 Concen: 132.392 ng
 RT: 10.70 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 416177
 Ion Ratio Lower Upper
 330 100
 332 97.6 78.1 117.1
 141 32.3 26.9 40.3

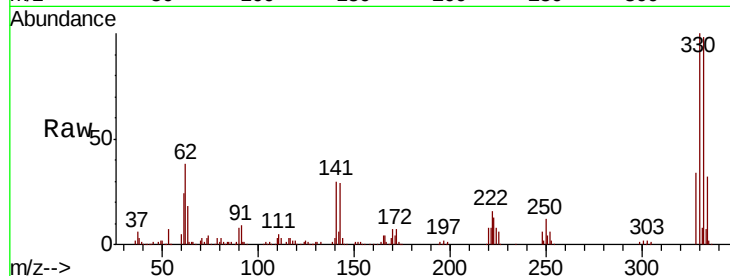


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


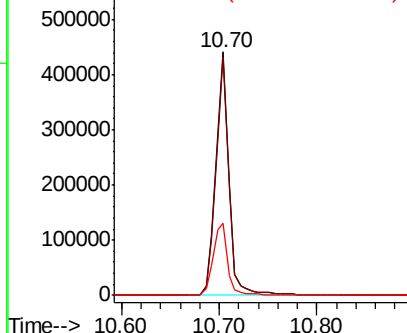



#45
 2-Fluorobiphenyl
 Concen: 88.162 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. -0.01 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Tgt Ion:172 Resp: 1499248
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.2 43.8
 170 24.0 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

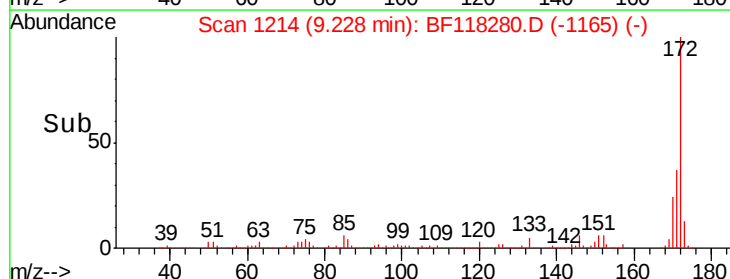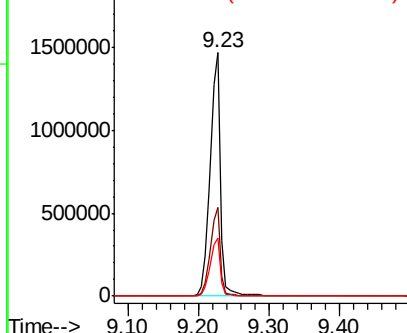







#51
 2,6-Dinitrotoluene
 Concen: 8.022 ng
 RT: 9.90 min Scan# 1329
 Delta R.T. 0.20 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
165	100		
63	1.5	41.4	62.0#
89	1.4	42.9	64.3#

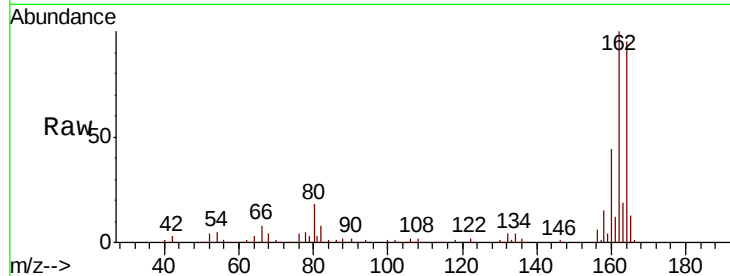


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1


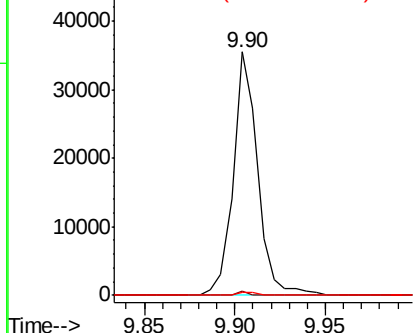



#57
 2,4-Dinitrotoluene
 Concen: 6.010 ng
 RT: 9.90 min Scan# 1329
 Delta R.T. -0.21 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.5	32.6	49.0#
89	1.4	56.1	84.1#
182	0.0	2.1	3.1#

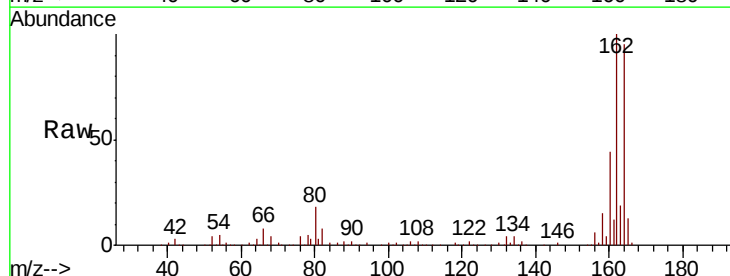

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF1
 Ion 89.00 (88.70 to 89.70): BF1
 Ion 182.00 (181.70 to 182.70): E

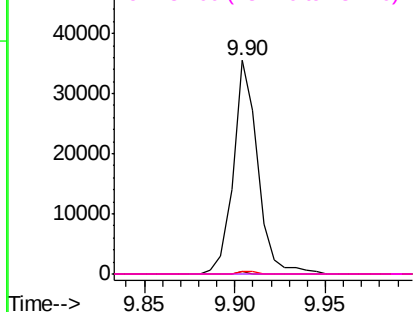



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.40 min Scan# 1583

Delta R.T. -0.01 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Instrument :

BNA_F

ClientSampleId :


Tot Ion:188 Resp: 494874

Ion Ratio Lower Upper

188 100

94 9.3 7.1 10.7




80 9.6 7.9 11.9

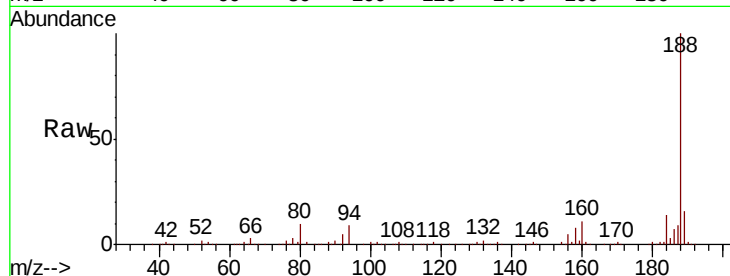

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

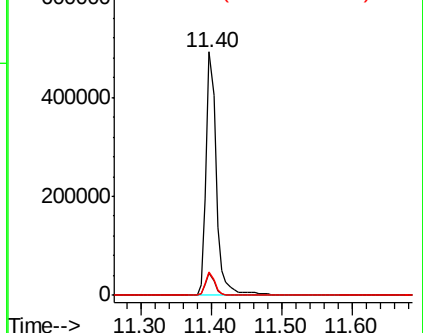

#67

4-Bromophenyl-phenylether

Concen: 4.504 ng

RT: 10.70 min Scan# 1465

Delta R.T. -0.25 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34


Tgt Ion:248 Resp: 25443

Ion Ratio Lower Upper

248 100

250 196.1 78.3 117.5#



141 478.3 52.2 78.4#




Abundance Ion 248.00 (247.70 to 248.70): E

Ion 250.00 (249.70 to 250.70): E

Ion 141.00 (140.70 to 141.70): E

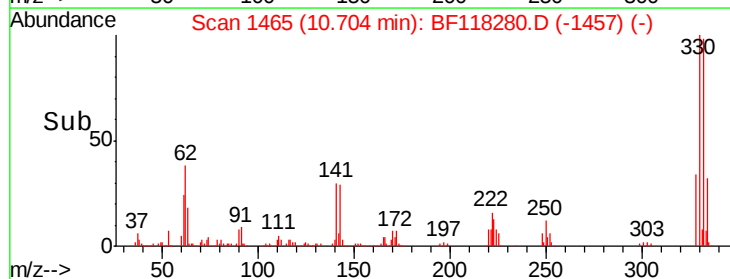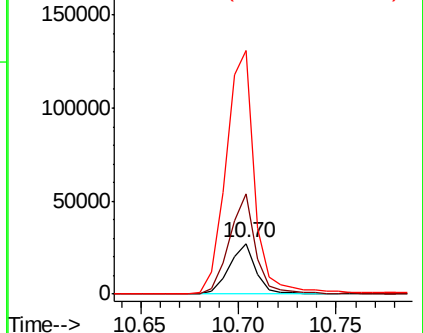



#76

Chrvsene-d12

Concen: 20.000 ng

RT: 14.05 min Scan# 2034

Delta R.T. -0.02 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34

Instrument :

BNA_F

ClientSampleId :

Tot Ion:240 Resp: 319854

Ion Ratio Lower Upper

240 100

120 12.1 7.1 10.7#




236 26.5 21.0 31.6



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

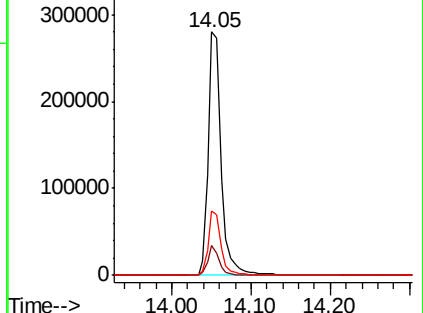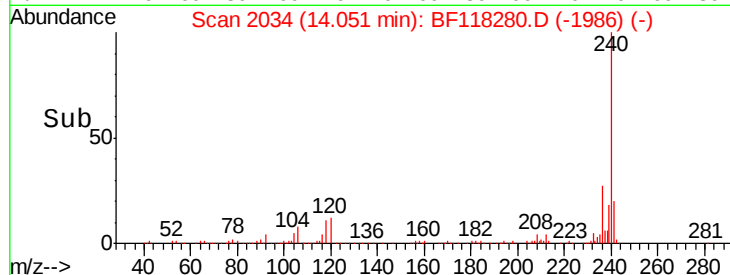

#79

Terphenyl-d14

Concen: 99.404 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BF118280.D

Acq: 19 Dec 2019 15:34


Tgt Ion:244 Resp: 1848941

Ion Ratio Lower Upper

244 100

212 7.2 5.9 8.9



122 12.3 9.0 13.6




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

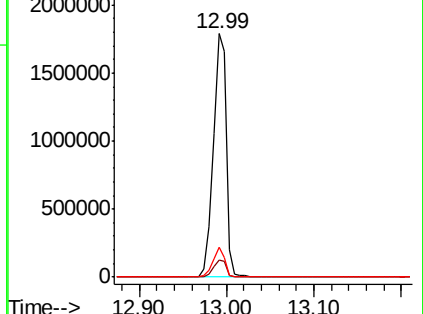

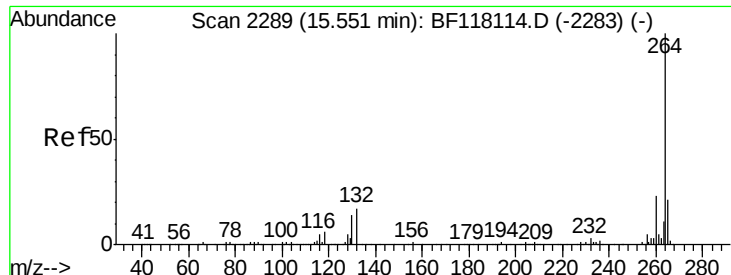

#87
 Pervlene-d12
 Concen: 20.000 ng
 RT: 15.54 min Scan# 2288
 Delta R.T. -0.01 min
 Lab File: BF118280.D
 Acq: 19 Dec 2019 15:34

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.6	18.6	28.0
265	22.1	16.8	25.2

