


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF121919\
 Data File : BF118274.D
 Acq On : 19 Dec 2019 12:37
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120619.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 06 17:34:43 2019

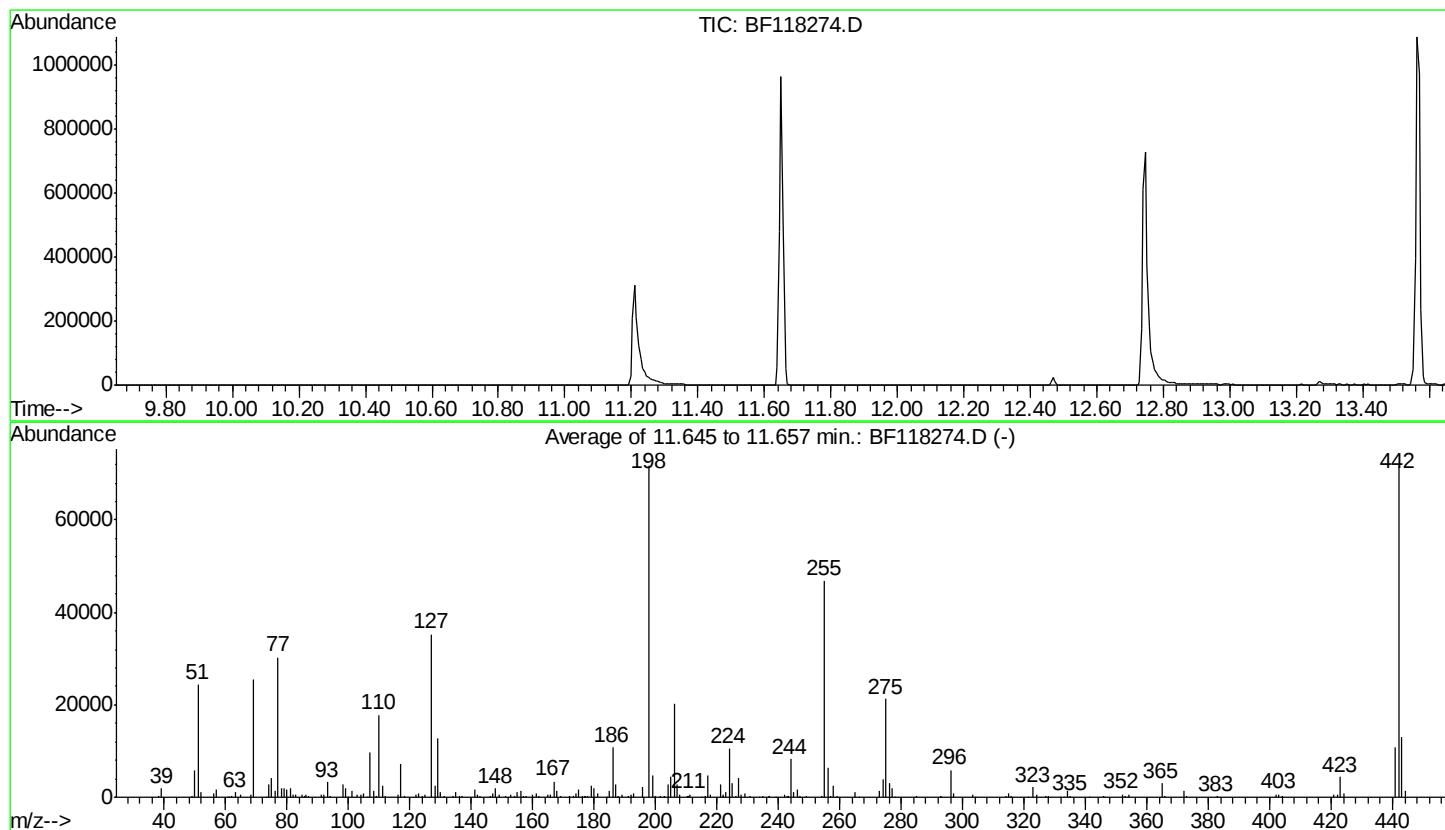

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	24288	PASS
68	69	0.00	2	1.7	434	PASS
69	198	0.00	100	35.5	25451	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.1	35269	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71760	PASS
199	198	5	9	6.7	4795	PASS
275	198	10	60	29.6	21243	PASS
365	198	1	100	4.2	3021	PASS
441	198	0.01	100	15.1	10854	PASS
442	198	50	100	100.0	71744	PASS
443	442	15	24	18.1	12966	PASS