

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122018\
 Data File : BF111662.D
 Acq On : 21 Dec 2018 2:04
 Operator : JU/SJ
 Sample : J6447-08 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS025-1218-01

Quant Time: Dec 21 06:24:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.90	152	206695	20.00	ng	0.00
21) Naphthalene-d8	8.17	136	753580	20.00	ng	0.00
39) Acenaphthene-d10	9.93	164	330975	20.00	ng	0.00
64) Phenanthrene-d10	11.42	188	496426	20.00	ng	0.00
76) Chrysene-d12	14.04	240	489744	20.00	ng	0.00
87) Perylene-d12	15.52	264	355550	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	130070	10.73	ng	0.00
7) Phenol-d6	6.51	99	167444	10.85	ng	-0.01
23) Nitrobenzene-d5	7.45	82	95091	7.34	ng	-0.01
42) 2,4,6-Tribromophenol	10.71	330	33033	8.45	ng	-0.01
45) 2-Fluorobiphenyl	9.25	172	191595	8.44	ng	0.00
79) Terphenyl-d14	12.99	244	150929	5.84	ng	0.00
Target Compounds						
25) Isophorone	7.45	82	95088	4.137	ng	# 64
57) 2,4-Dinitrotoluene	9.93	165	42220	7.279	ng	# 24


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122018\
Data File : BF111662.D
Acq On : 21 Dec 2018 2:04
Operator : JU/SJ
Sample : J6447-08 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
P001-SS025-1218-01

Quant Time: Dec 21 06:24:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

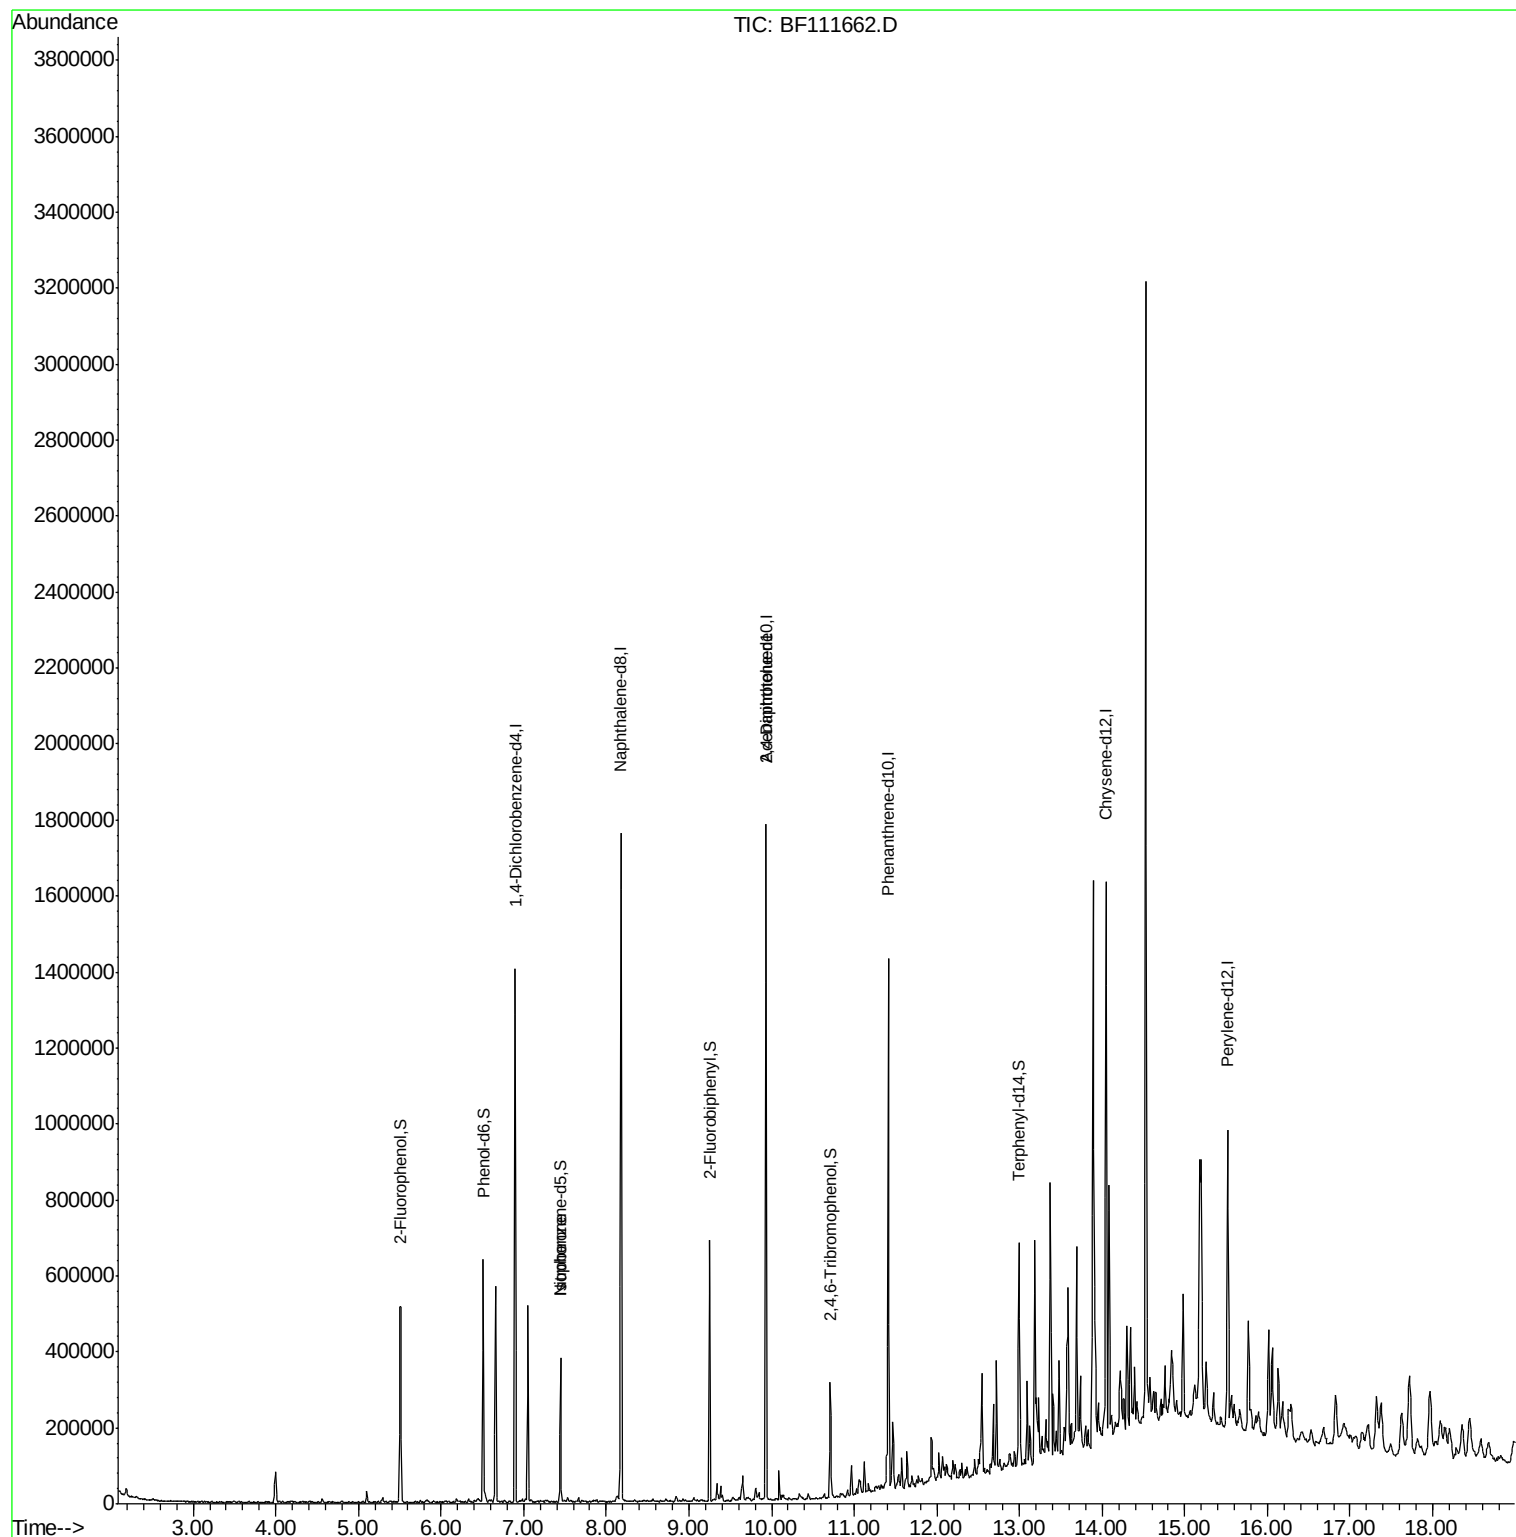




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.90 min Scan# 818
Delta R.T. -0.00 min
Lab File: BF111662.D
Acq: 21 Dec 2018 2:04

Instrument :
BNA_F
ClientSampleId :
P001-SS025-1218-01

Tgt Ion:152 Resp: 206695
Ion Ratio Lower Upper
152 100
150 154.6 126.6 189.8
115 55.4 50.7 76.1

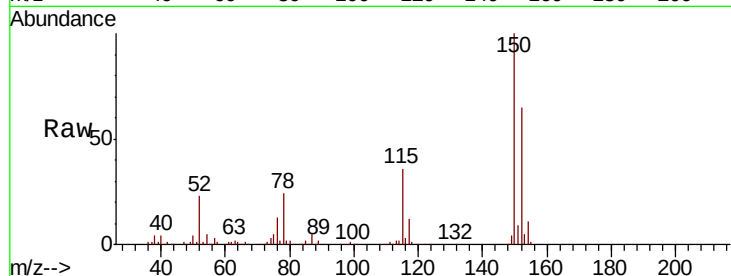


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

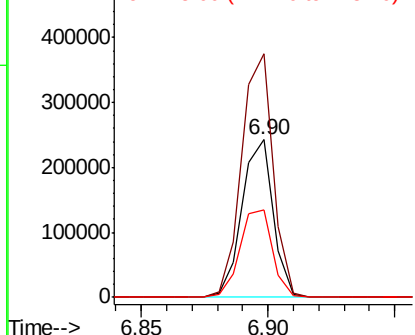



#5


2-Fluorophenol
Concen: 10.726 ng
RT: 5.51 min Scan# 582
Delta R.T. -0.01 min
Lab File: BF111662.D
Acq: 21 Dec 2018 2:04

Tgt Ion:112 Resp: 130070
Ion Ratio Lower Upper
112 100
64 55.8 51.8 77.6
63 29.5 26.8 40.2



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

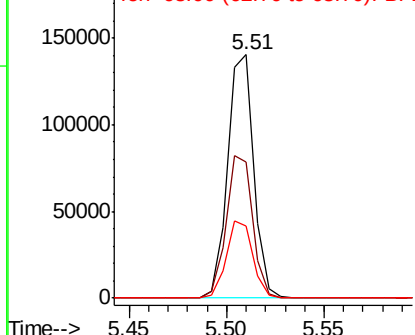

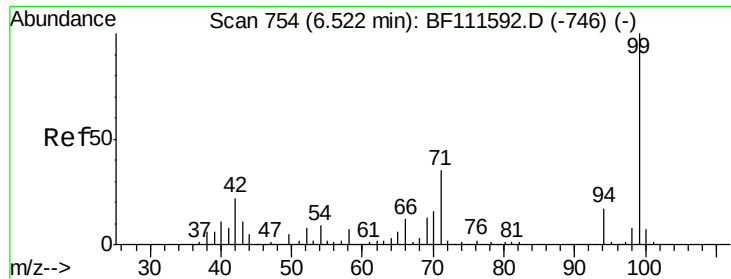

#7

Phenol-d6

Concen: 10.850 ng

RT: 6.51 min Scan# 752

Delta R.T. -0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04

Instrument :

BNA_F

ClientSampleId :

P001-SS025-1218-01


Tgt Ion: 99 Resp: 167444

Ion Ratio Lower Upper




99 100

42 19.9 17.4 26.0

71 33.4 26.1 39.1



Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

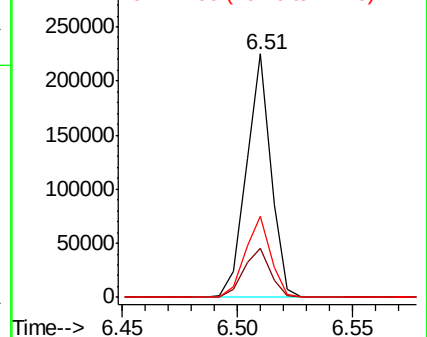

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.17 min Scan# 1035

Delta R.T. -0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04

Tgt Ion: 136 Resp: 753580


Ion Ratio Lower Upper

136 100



137 11.4 9.1 13.7


54 9.6 7.7 11.5

68 6.0 4.9 7.3



Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

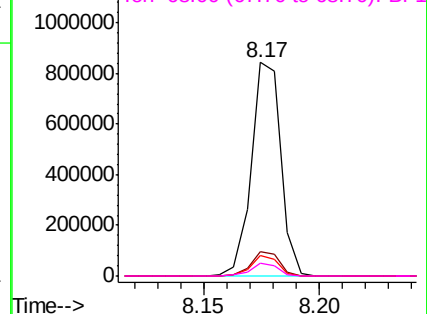







#23
 Nitrobenzene-d5
 Concen: 7.345 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.01 min
 Lab File: BF111662.D
 Acq: 21 Dec 2018 2:04

Instrument :
 BNA_F
 ClientSampleId :
 P001-SS025-1218-01

Tgt Ion: 82 Resp: 95091
 Ion Ratio Lower Upper
 82 100
 128 44.3 37.4 56.2
 54 58.5 47.6 71.4

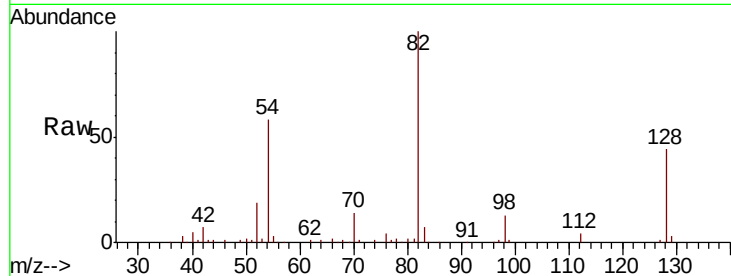


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1


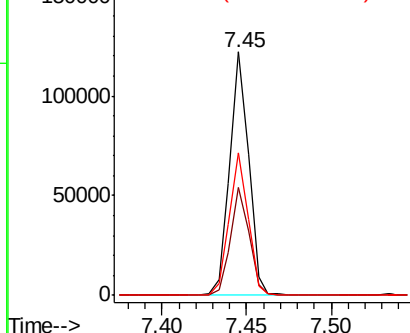



#25
 Isophorone
 Concen: 4.137 ng
 RT: 7.45 min Scan# 911
 Delta R.T. -0.27 min
 Lab File: BF111662.D
 Acq: 21 Dec 2018 2:04

Tgt Ion: 82 Resp: 95088
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.4 8.2#
 138 0.0 15.1 22.7#



Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 95.00 (94.70 to 95.70): BF1
 Ion 138.00 (137.70 to 138.70): BF1

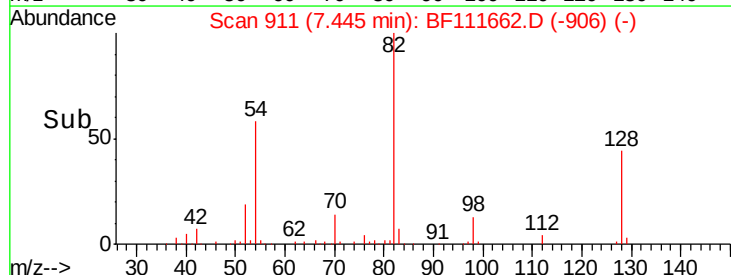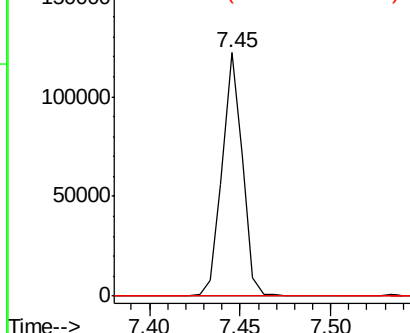

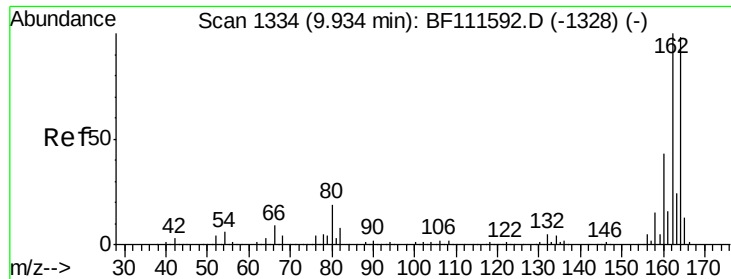

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.93 min Scan# 1334

Delta R.T. -0.00 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04

Instrument :

BNA_F

ClientSampleId :

P001-SS025-1218-01


Tgt Ion:164 Resp: 330975

Ion Ratio Lower Upper

164 100

162 100.0 81.4 122.0




160 43.9 35.7 53.5



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

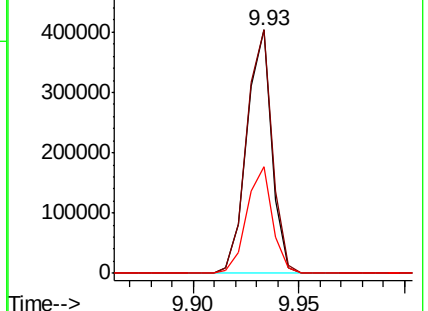

#42

2,4,6-Tribromophenol

Concen: 8.447 ng

RT: 10.71 min Scan# 1466

Delta R.T. -0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04


Tgt Ion:330 Resp: 33033

Ion Ratio Lower Upper

330 100

332 94.5 76.0 114.0



141 30.2 31.0 46.6#




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



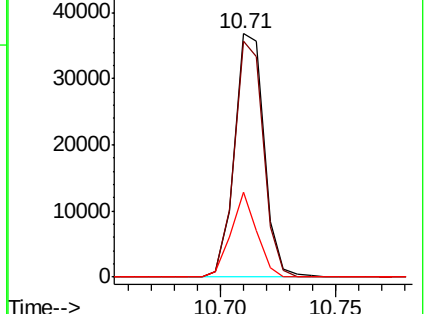



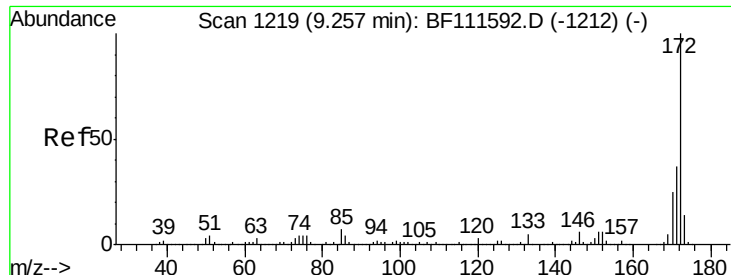

#45
 2-Fluorobiphenyl
 Concen: 8.438 ng
 RT: 9.25 min Scan# 1218
 Delta R.T. -0.01 min
 Lab File: BF111662.D
 Acq: 21 Dec 2018 2:04




Instrument :
 BNA_F
 ClientSampleId :
 P001-SS025-1218-01


Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.5	33.0	49.4
170	23.0	22.3	33.5

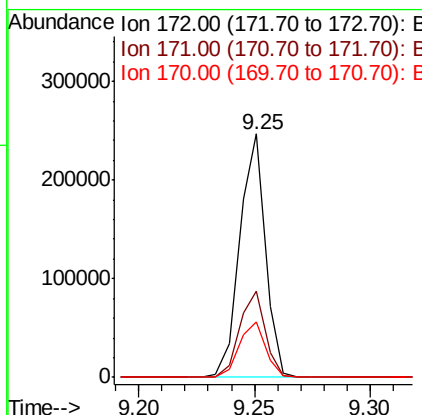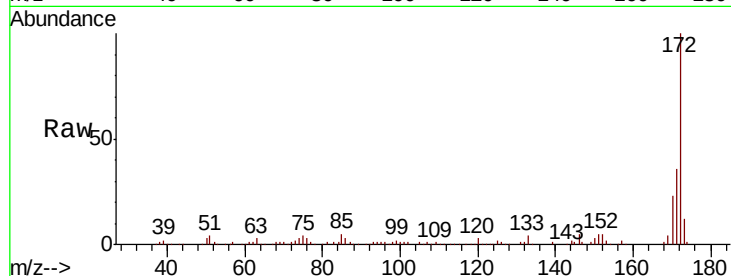

#57
 2,4-Dinitrotoluene
 Concen: 7.279 ng
 RT: 9.93 min Scan# 1334
 Delta R.T. -0.18 min
 Lab File: BF111662.D
 Acq: 21 Dec 2018 2:04

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.2	34.6	52.0#
89	1.3	56.2	84.4#
182	0.0	1.8	2.6#

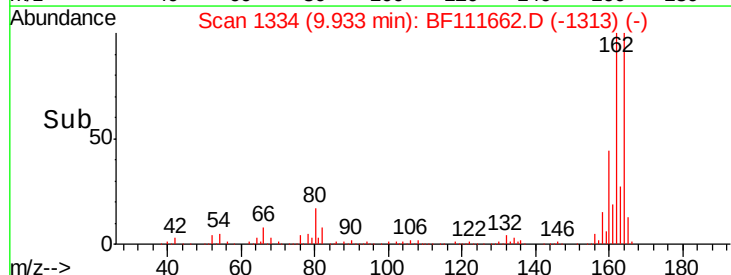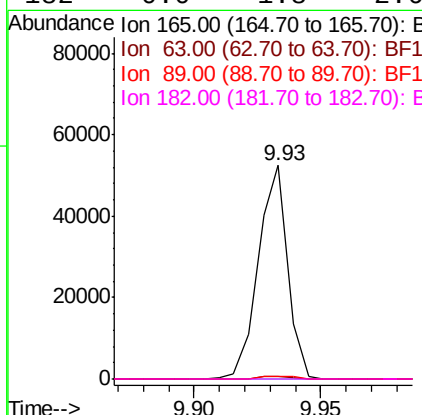

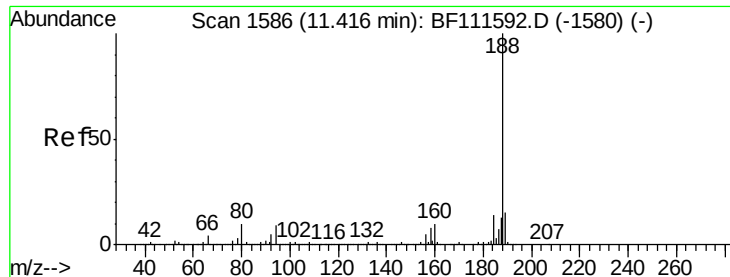

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.42 min Scan# 1586

Delta R.T. -0.00 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04

Instrument :

BNA_F

ClientSampleId :

P001-SS025-1218-01


Tgt Ion:188 Resp: 496426

Ion Ratio Lower Upper

188 100

94 7.9 9.6 14.4#




80 8.0 9.8 14.6#

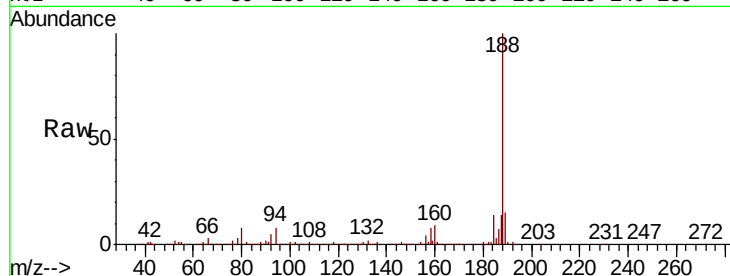

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

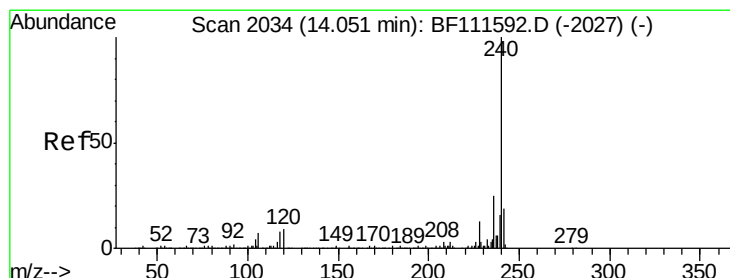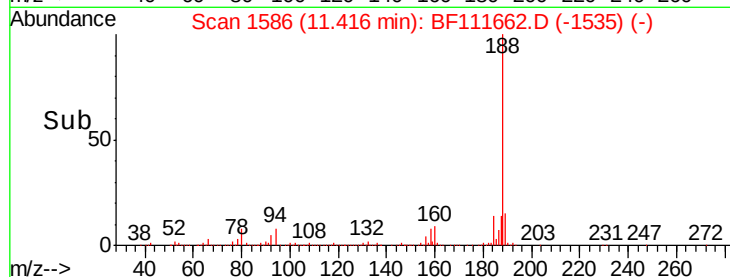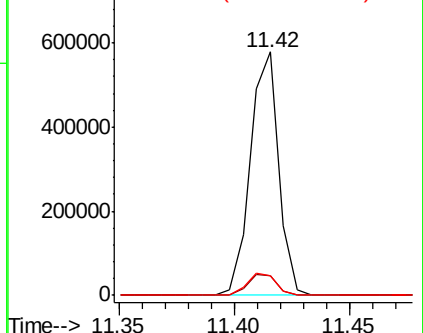

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.04 min Scan# 2033

Delta R.T. -0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04


Tgt Ion:240 Resp: 489744

Ion Ratio Lower Upper

240 100

120 10.5 12.2 18.2#



236 25.7 20.2 30.2

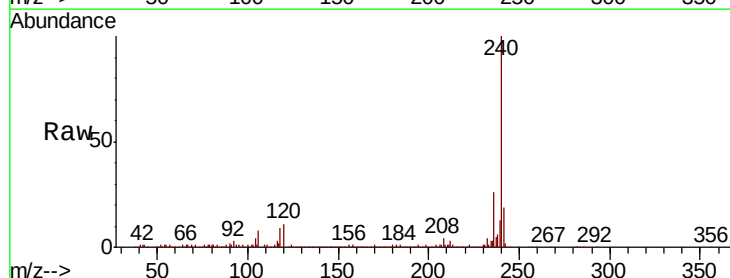


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

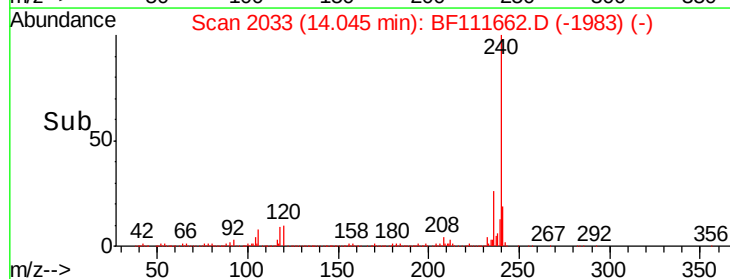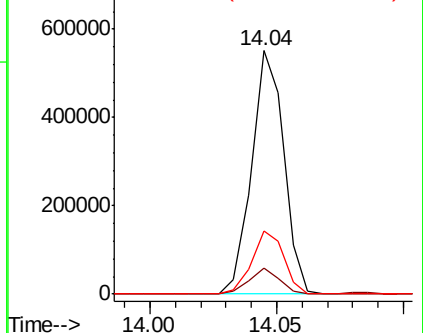

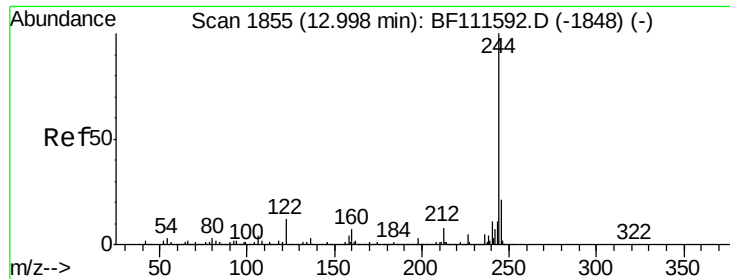

#79

Terphenyl-d14

Concen: 5.844 ng

RT: 12.99 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04

Instrument :

BNA_F

ClientSampleId :

P001-SS025-1218-01


Tgt Ion:244 Resp: 150929

Ion Ratio Lower Upper

244 100

212 5.8 5.7 8.5




122 11.0 13.1 19.7#

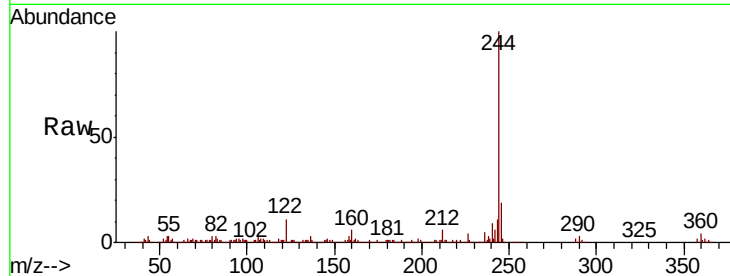

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

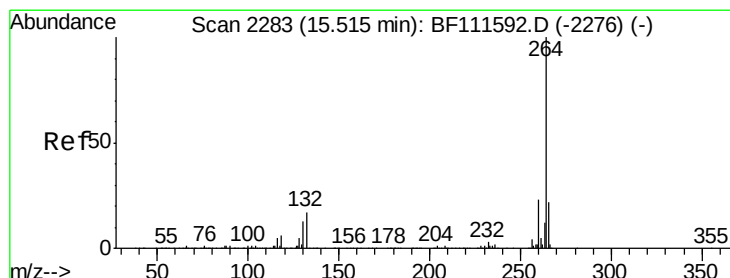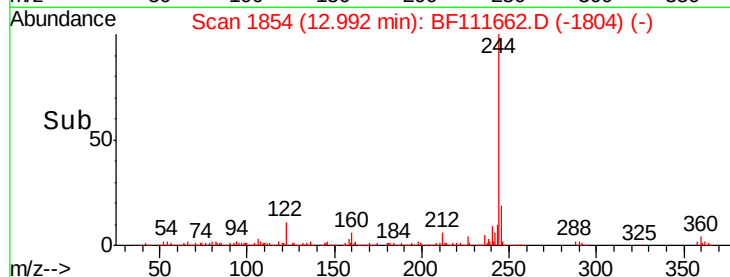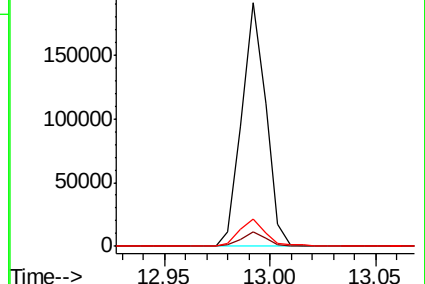

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.52 min Scan# 2284

Delta R.T. 0.01 min

Lab File: BF111662.D

Acq: 21 Dec 2018 2:04


Tgt Ion:264 Resp: 355550

Ion Ratio Lower Upper

264 100

260 24.0 18.3 27.5

265 20.8 17.7 26.5

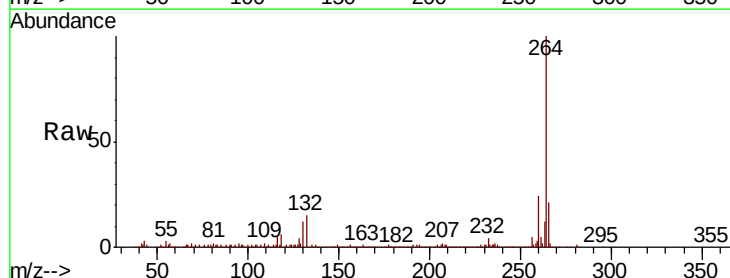

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

