
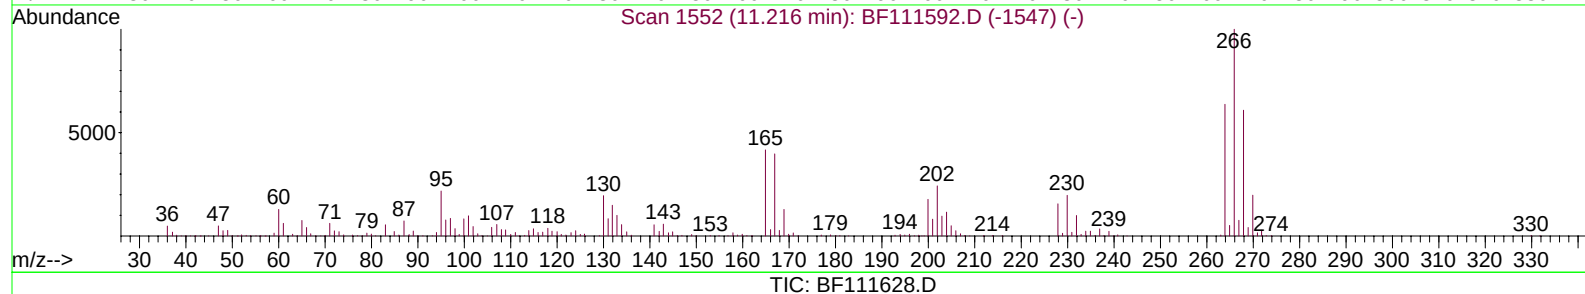
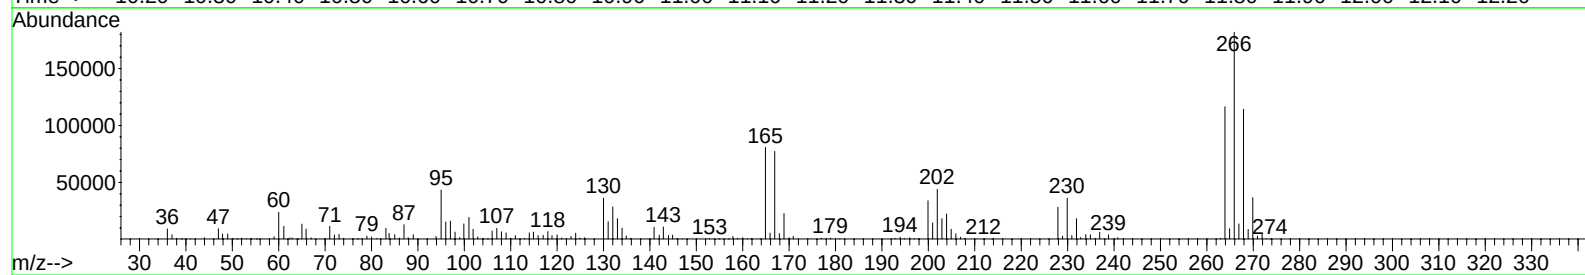


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122018\
Data File : BF111628.D
Acq On : 20 Dec 2018 9:58
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 18:00:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

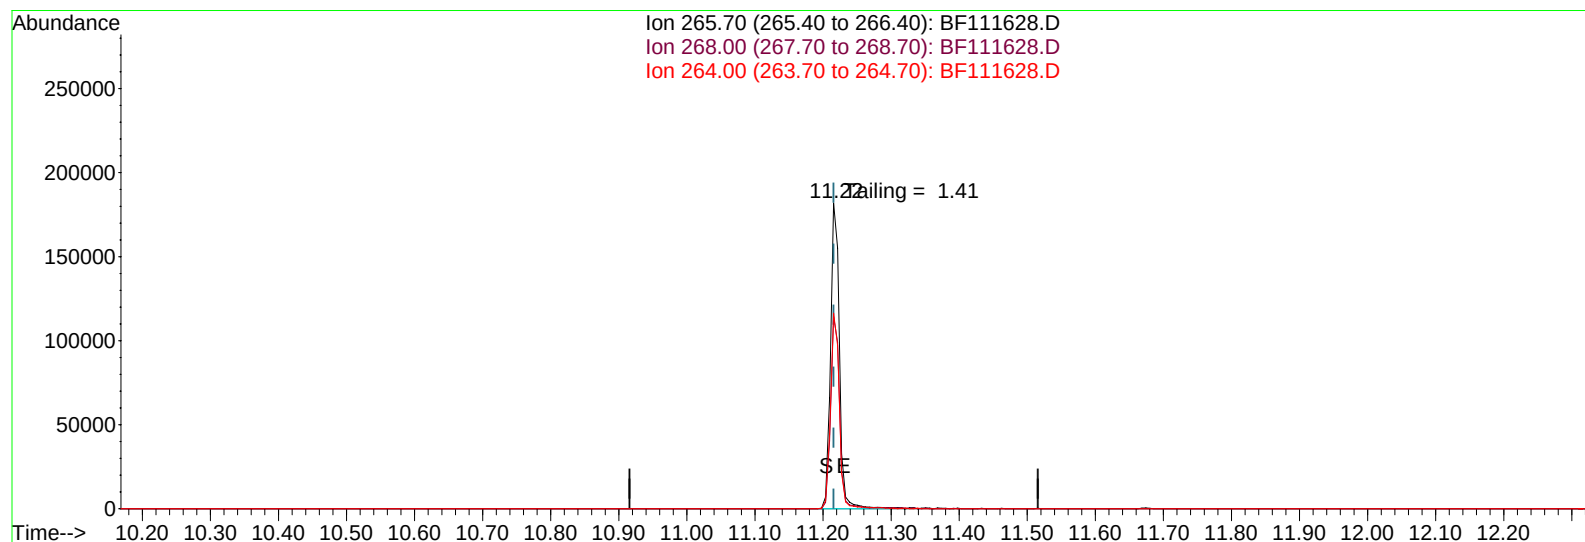

(70) Pentachlorophenol (C)




11.216min (-0.000) 168005.19ng

response 165181

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	62.85
264.00	61.40	63.97
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122018\
 Data File : BF111628.D
 Acq On : 20 Dec 2018 9:58
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 18:00:31 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration

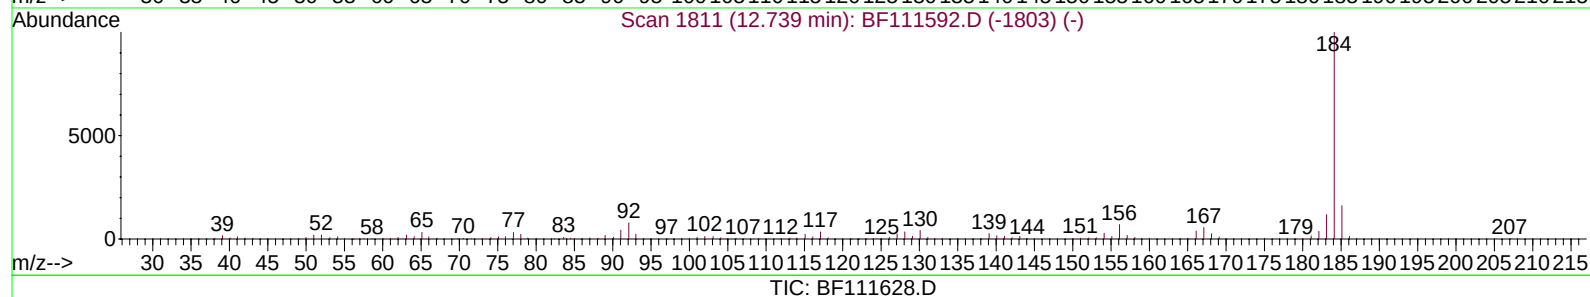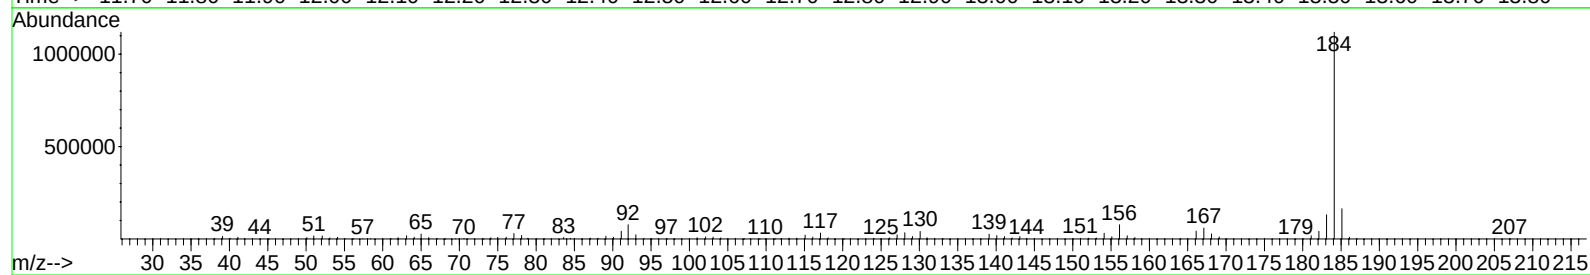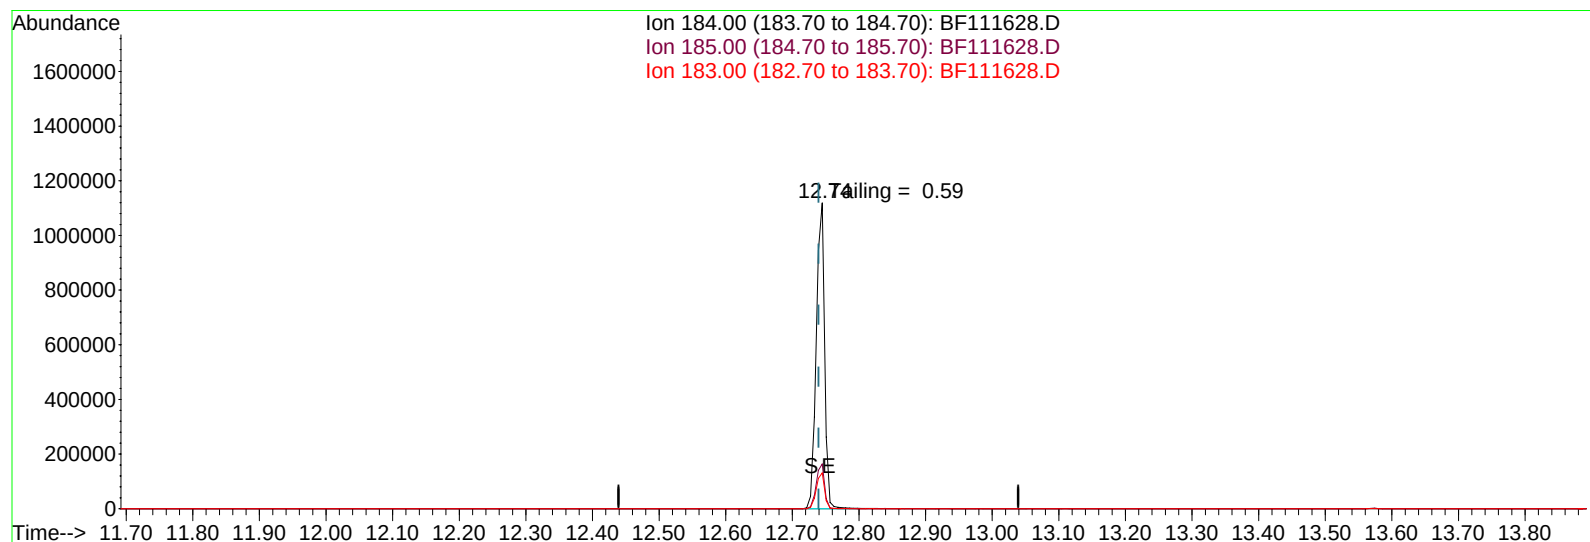

(77) Benzidine

12.745min (+0.006) 49655.06ng

response 979093

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	14.66
183.00	11.60	11.72
0.00	0.00	0.00