

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122018\
 Data File : BF111633.D
 Acq On : 20 Dec 2018 12:21
 Operator : JU/SJ
 Sample : J6490-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 72-11929

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	18	24	30	rVB	99148	130284	2.37%	0.269%
2	5.122	508	516	522	rBV	366904	462806	8.41%	0.954%
3	5.522	579	584	587	rBV	4498177	4353252	79.07%	8.976%
4	6.522	748	754	759	rBV	4439292	4902248	89.04%	10.107%
5	6.669	774	779	782	rBV	4933847	4624713	84.00%	9.535%
6	6.898	814	818	821	rBV	1428702	1190355	21.62%	2.454%
7	7.057	840	845	848	rBV	4150481	3689701	67.02%	7.607%
8	7.451	907	912	915	rBV	2969971	2986814	54.25%	6.158%
9	8.175	1031	1035	1039	rBV	1729025	1531422	27.81%	3.157%
10	9.251	1213	1218	1222	rBV	5763883	5505745	100.00%	11.352%
11	9.639	1281	1284	1287	rBV	420912	301345	5.47%	0.621%
12	9.933	1330	1334	1337	rVB	1947453	1706007	30.99%	3.517%
13	10.716	1462	1467	1470	rBV	3656336	3195531	58.04%	6.589%
14	11.416	1582	1586	1588	rBV	1960500	1625945	29.53%	3.352%
15	11.439	1588	1590	1593	rVV	335316	265101	4.81%	0.547%
16	11.486	1596	1598	1601	rVB	102451	77496	1.41%	0.160%
17	11.633	1620	1623	1627	rBV2	67282	64361	1.17%	0.133%
18	11.939	1672	1675	1679	rVB2	187979	176086	3.20%	0.363%
19	12.027	1687	1690	1693	rBV2	57760	60437	1.10%	0.125%
20	12.621	1788	1791	1795	rBV	440791	392202	7.12%	0.809%
21	12.851	1825	1830	1836	rBV	340949	364902	6.63%	0.752%
22	12.998	1851	1855	1858	rVB	5014005	4311164	78.30%	8.889%
23	13.245	1893	1897	1899	rBV2	63548	66621	1.21%	0.137%
24	13.892	2003	2007	2013	rBV	676893	702662	12.76%	1.449%
25	14.045	2028	2033	2036	rBV2	1508021	1614152	29.32%	3.328%
26	14.068	2036	2037	2042	rVB	148210	99650	1.81%	0.205%
27	14.221	2060	2063	2068	rVB2	125479	138804	2.52%	0.286%
28	14.521	2111	2114	2118	rBV	222328	219961	4.00%	0.454%
29	14.833	2164	2167	2172	rVB	272060	285245	5.18%	0.588%
30	14.915	2178	2181	2185	rVB	92094	95986	1.74%	0.198%
31	15.086	2207	2210	2213	rBV	126862	150906	2.74%	0.311%
32	15.180	2222	2226	2233	rBV2	331859	435198	7.90%	0.897%
33	15.392	2259	2262	2268	rVB	62196	93393	1.70%	0.193%
34	15.456	2269	2273	2276	rVV	116523	164633	2.99%	0.339%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122018\
Data File : BF111633.D
Acq On : 20 Dec 2018 12:21
Operator : JU/SJ
Sample : J6490-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11929

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	15.521	2279	2284	2288	rVV	1071809	1354718	24.61%	2.793%
36	15.568	2288	2292	2297	rVB2	298302	417045	7.57%	0.860%
37	16.015	2363	2368	2372	rBV	229846	372764	6.77%	0.769%
38	16.056	2372	2375	2380	rVB3	99794	155725	2.83%	0.321%
39	16.533	2451	2456	2463	rBV2	98406	215810	3.92%	0.445%


Sum of corrected areas: 48501190

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122018\
Data File : BF111633.D
Acq On : 20 Dec 2018 12:21
Operator : JU/SJ
Sample : J6490-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
72-11929

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

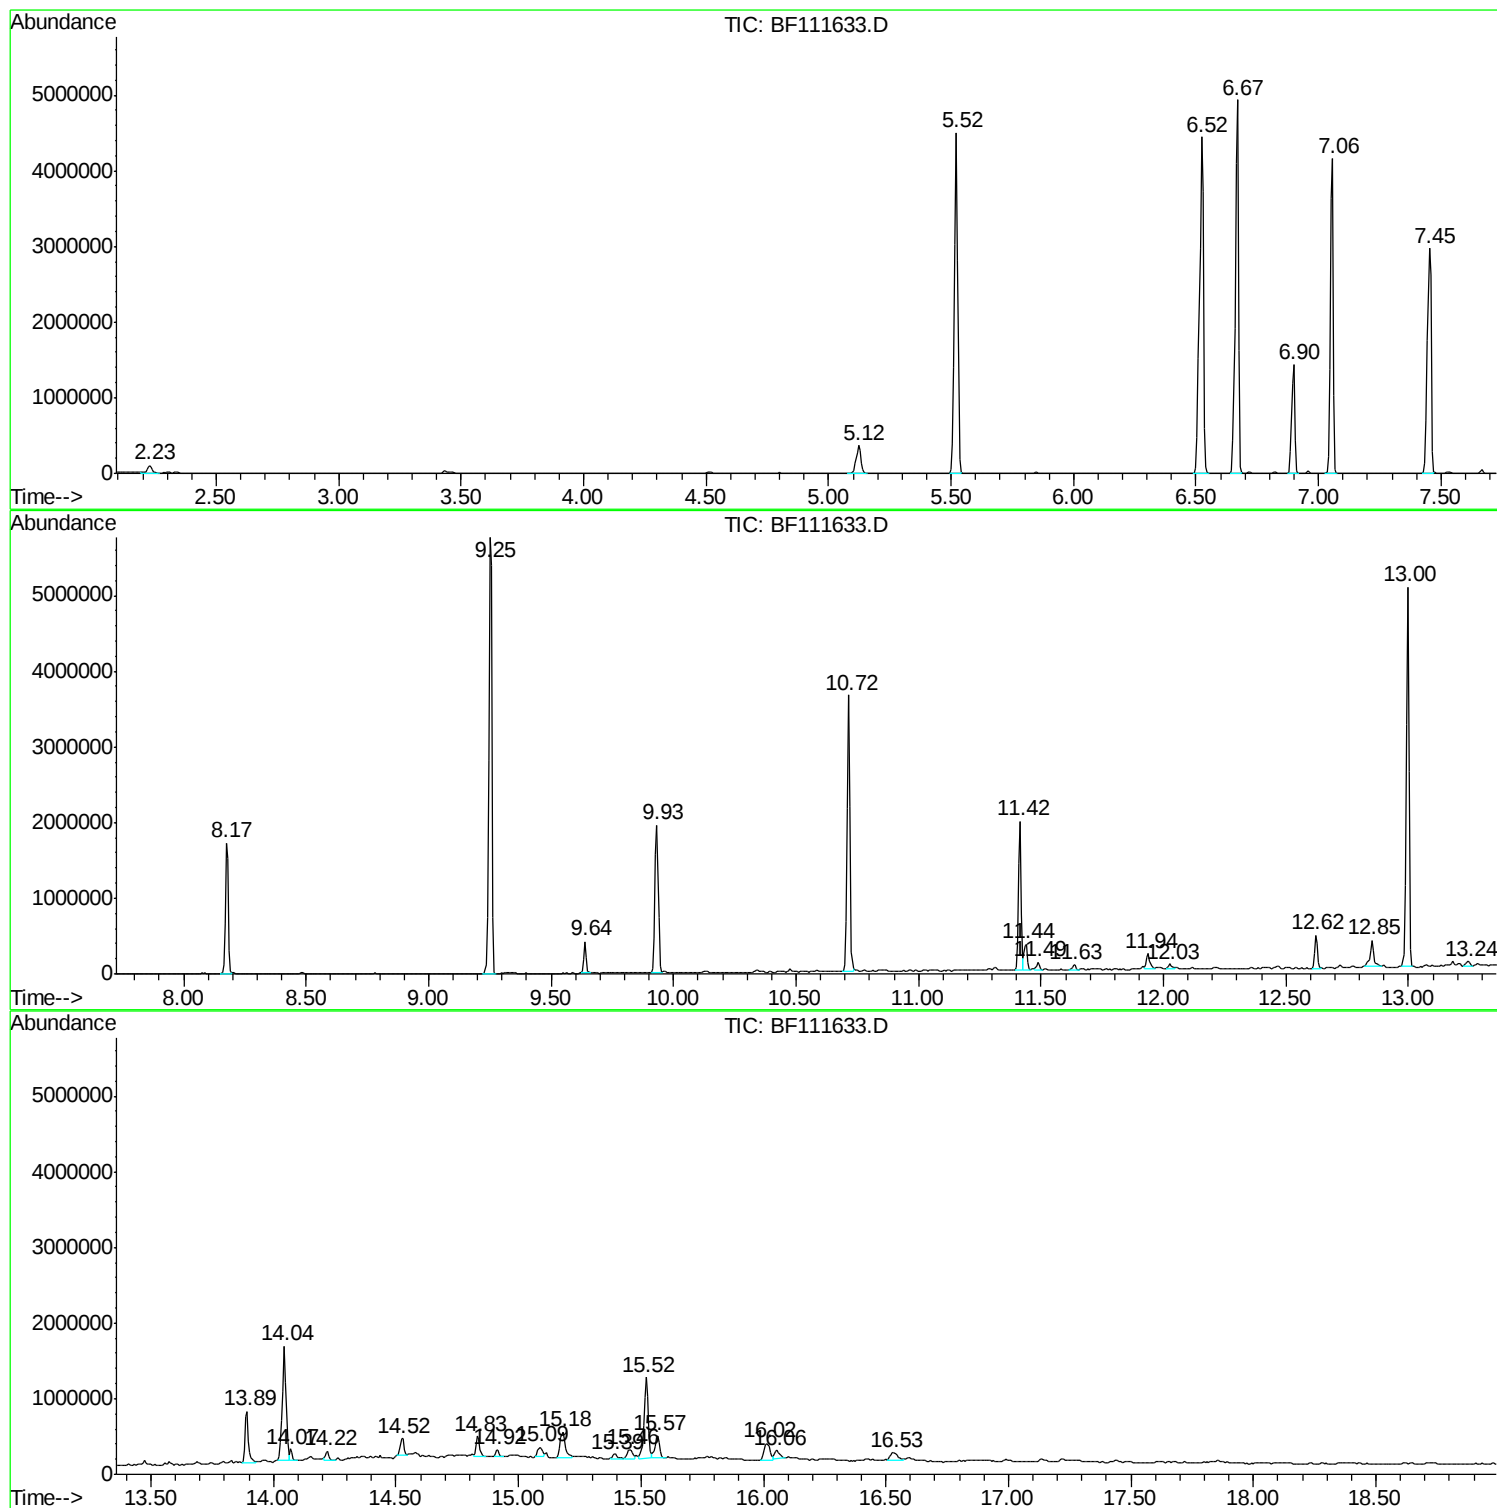

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122018\
Data_File : BF111633.D
Acq_On : 20-Dec-2018 12:211
Operator : JU/SJJ
Sample : J6490-011
Misc :
ALS_Vial : 6 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
72-11929

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
