


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF122018\  
 Data File : BF111667.D  
 Acq On : 21 Dec 2018 4:49  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF121918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Dec 19 17:39:39 2018

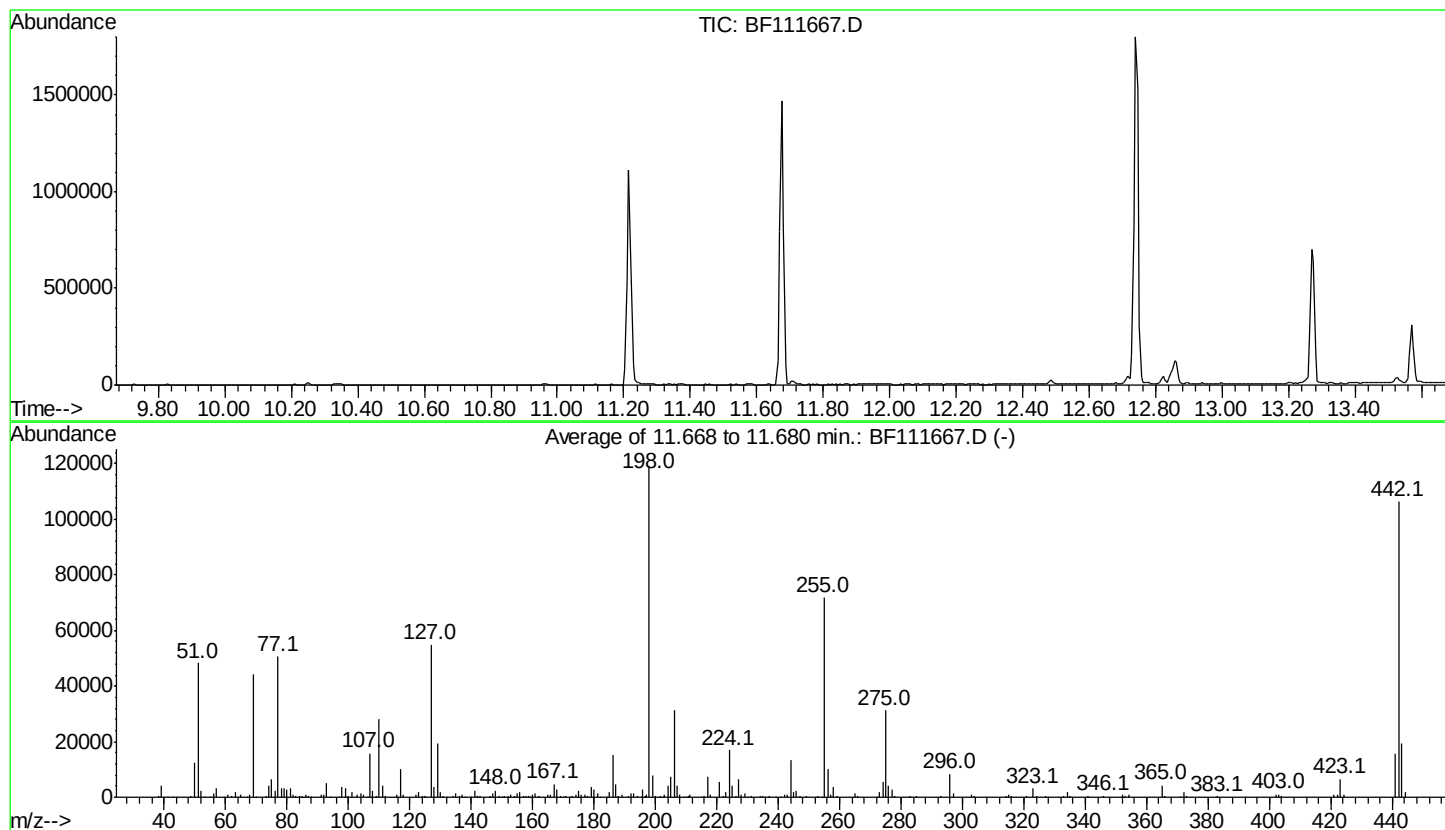

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.4      | 48253   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.7       | 761     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.9      | 44053   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 158     | PASS             |
| 127         | 198          | 10           | 80           | 46.1      | 54954   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 764     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 119314  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 8035    | PASS             |
| 275         | 198          | 10           | 60           | 26.1      | 31178   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 4210    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.3      | 15890   | PASS             |
| 442         | 198          | 50           | 100          | 89.0      | 106210  | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 19483   | PASS             |