
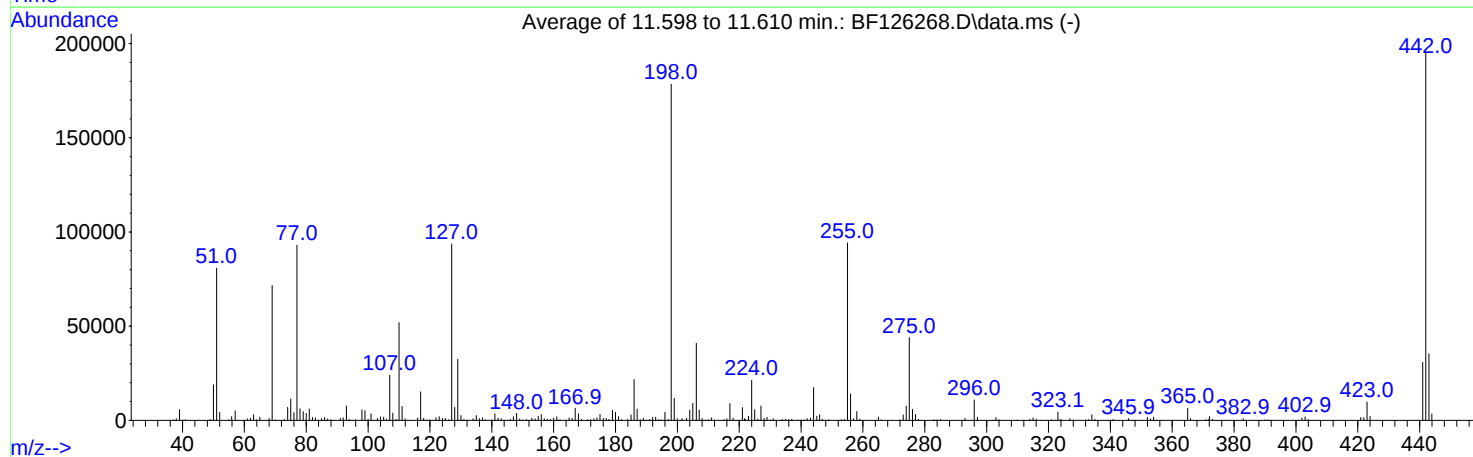


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122021\
 Data File : BF126268.D
 Acq On : 20 Dec 2021 9:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

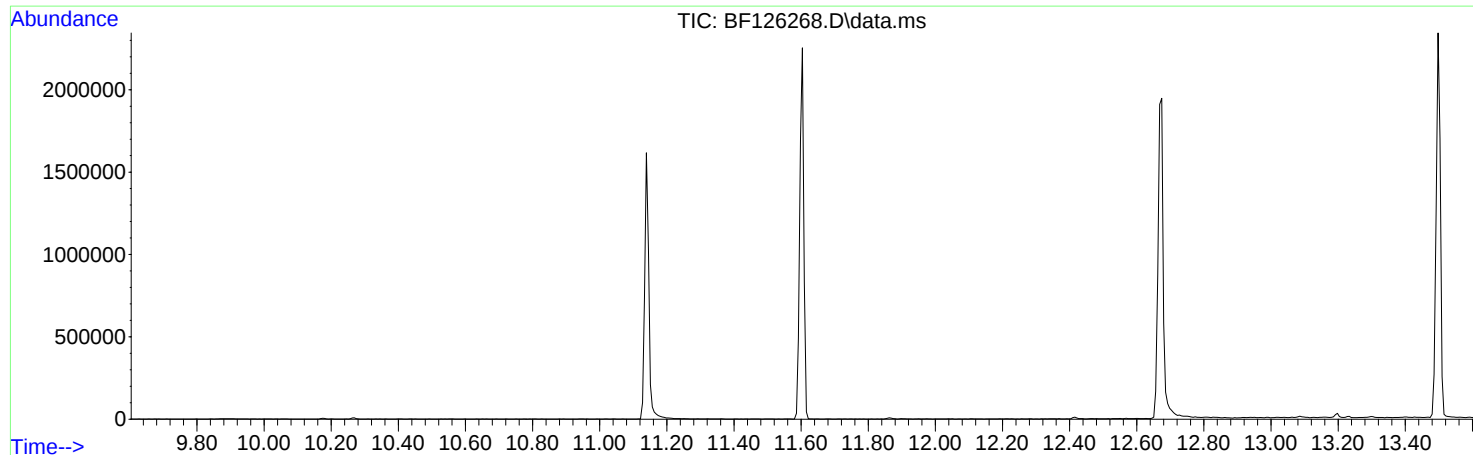




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	80805	PASS
68	69	0.00	2	1.5	1045	PASS
69	198	0.00	100	40.1	71608	PASS
70	69	0.00	2	0.4	279	PASS
127	198	10	80	52.4	93579	PASS
197	198	0.00	2	0.3	511	PASS
198	198	100	100	100.0	178440	PASS
199	198	5	9	6.6	11742	PASS
275	198	10	60	24.6	43984	PASS
365	198	1	100	3.6	6382	PASS
441	198	0.01	100	17.2	30704	PASS
442	442	50	100	100.0	195248	PASS
443	442	15	24	18.1	35413	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122021\
 Data File : BF126268.D
 Acq On : 20 Dec 2021 9:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 20 14:05:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

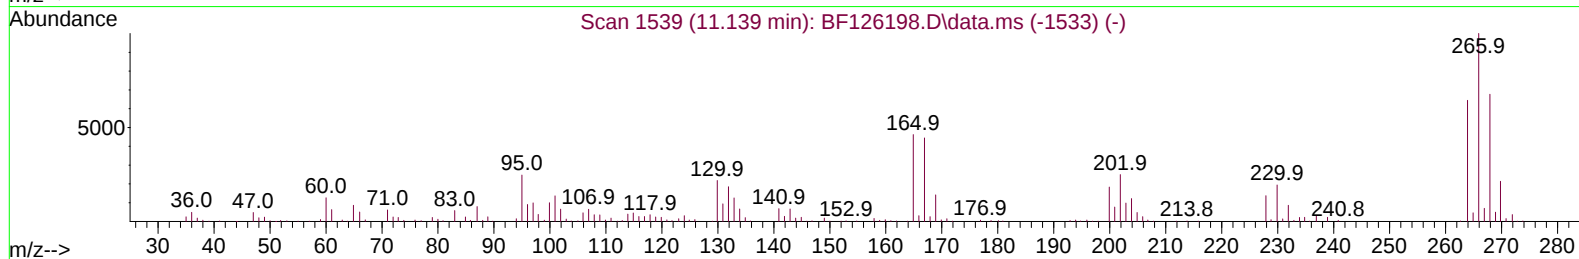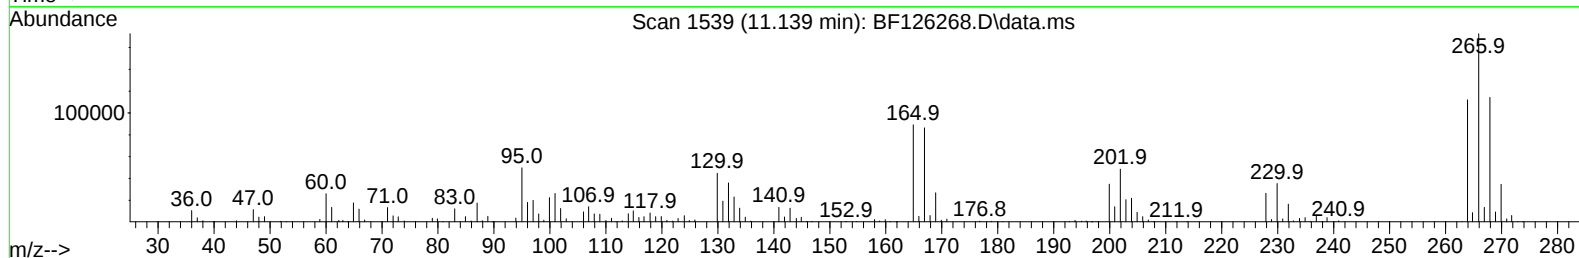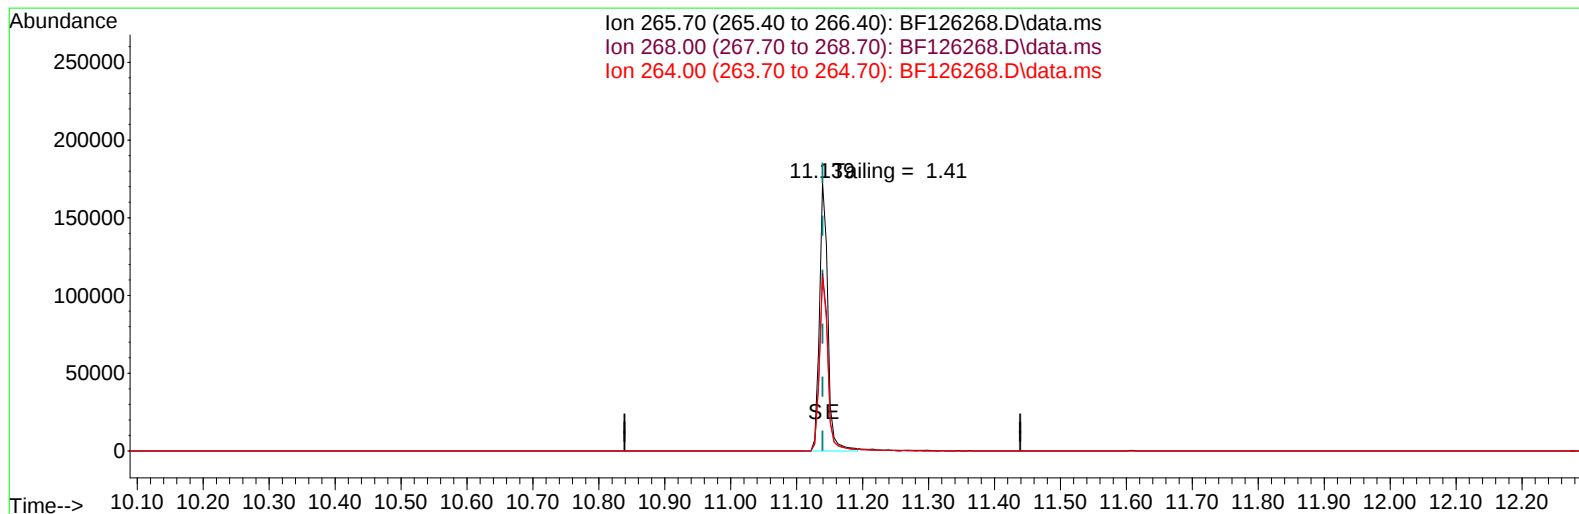

TIC: BF126268.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 53340.97 ng




response 155877

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	66.23
264.00	69.90	64.95
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122021\
Data File : BF126268.D
Acq On : 20 Dec 2021 9:46
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 20 14:05:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

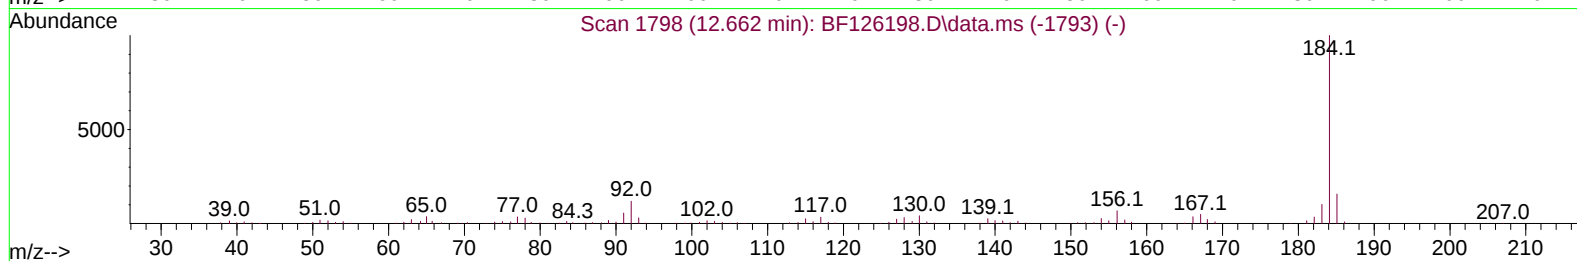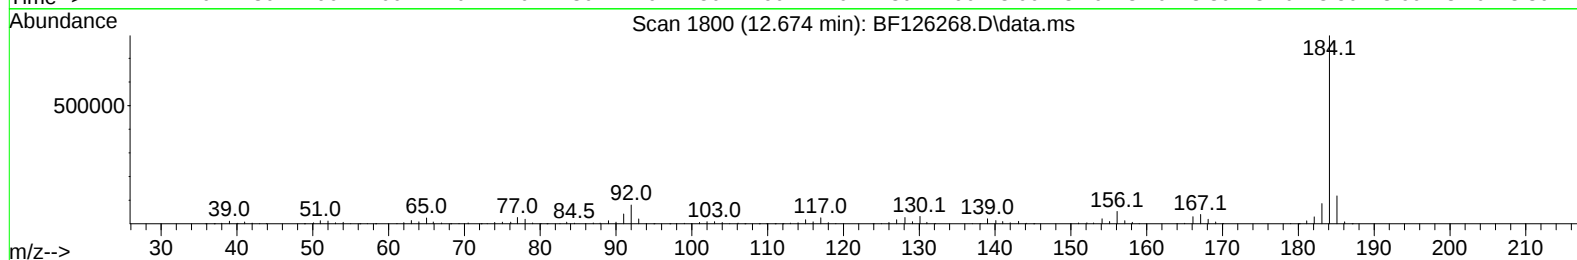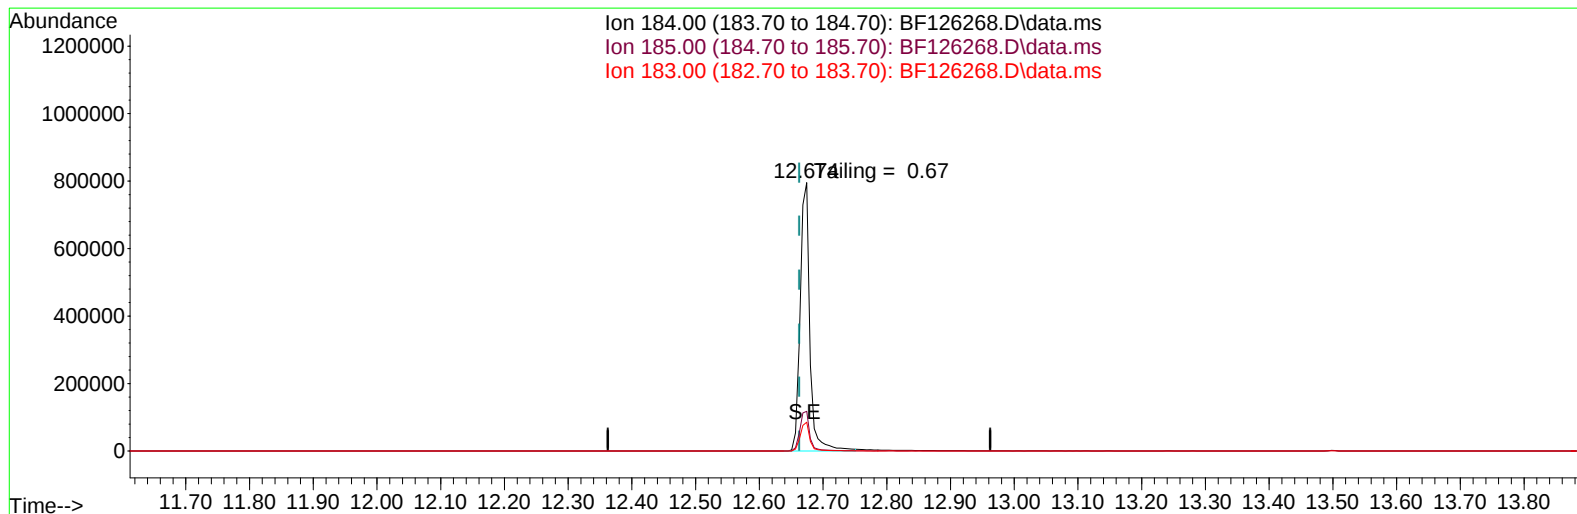

TIC: BF126268.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 856869

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.83
183.00	10.10	10.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/20/2021	BNA_F	<u>BF126268.D</u>
Compound Name	Response	Retention Time
DDT	390618	13.49
DDD	4716	13.19
DDE	295	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5011	395629	1.27