

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122118\
 Data File : BF111698.D
 Acq On : 21 Dec 2018 20:14
 Operator : JU/SJ
 Sample : J6188-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BU-01-122018

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.951	141	147	154	rVB	342751	466387	9.43%	1.147%
2	3.093	166	171	180	rBV	64110	104901	2.12%	0.258%
3	4.728	445	449	454	rBV	259133	263929	5.34%	0.649%
4	5.145	515	520	527	rBV2	503686	806430	16.31%	1.984%
5	5.551	583	589	592	rBV	4195216	4037683	81.67%	9.934%
6	6.545	753	758	761	rBV	3884666	3689197	74.62%	9.076%
7	6.681	776	781	784	rBV	4854554	4508367	91.19%	11.092%
8	6.904	815	819	822	rBV	1174718	928046	18.77%	2.283%
9	7.063	842	846	849	rBV	4325671	3617923	73.18%	8.901%
10	7.463	909	914	917	rBV	3240434	2931307	59.29%	7.212%
11	8.186	1033	1037	1040	rBV	1195195	1094686	22.14%	2.693%
12	9.263	1215	1220	1223	rBV	5452625	4943817	100.00%	12.163%
13	9.939	1331	1335	1339	rBV	1297170	1083330	21.91%	2.665%
14	10.727	1464	1469	1473	rBV	3259629	2985426	60.39%	7.345%
15	11.427	1584	1588	1591	rBV	1091712	1036049	20.96%	2.549%
16	11.945	1672	1676	1681	rBV2	84061	117298	2.37%	0.289%
17	13.010	1853	1857	1860	rBV	4864905	4578826	92.62%	11.265%
18	13.210	1888	1891	1899	rVB2	81422	103378	2.09%	0.254%
19	13.862	1987	2002	2004	rBV6	400580	1442726	29.18%	3.549%
20	14.062	2032	2036	2040	rVB	933442	867729	17.55%	2.135%
21	14.533	2114	2116	2127	rVB	315062	458904	9.28%	1.129%
22	15.545	2284	2288	2292	rVB	498878	580169	11.74%	1.427%


Sum of corrected areas: 40646508

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122118\
Data File : BF111698.D
Acq On : 21 Dec 2018 20:14
Operator : JU/SJ
Sample : J6188-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BU-01-122018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

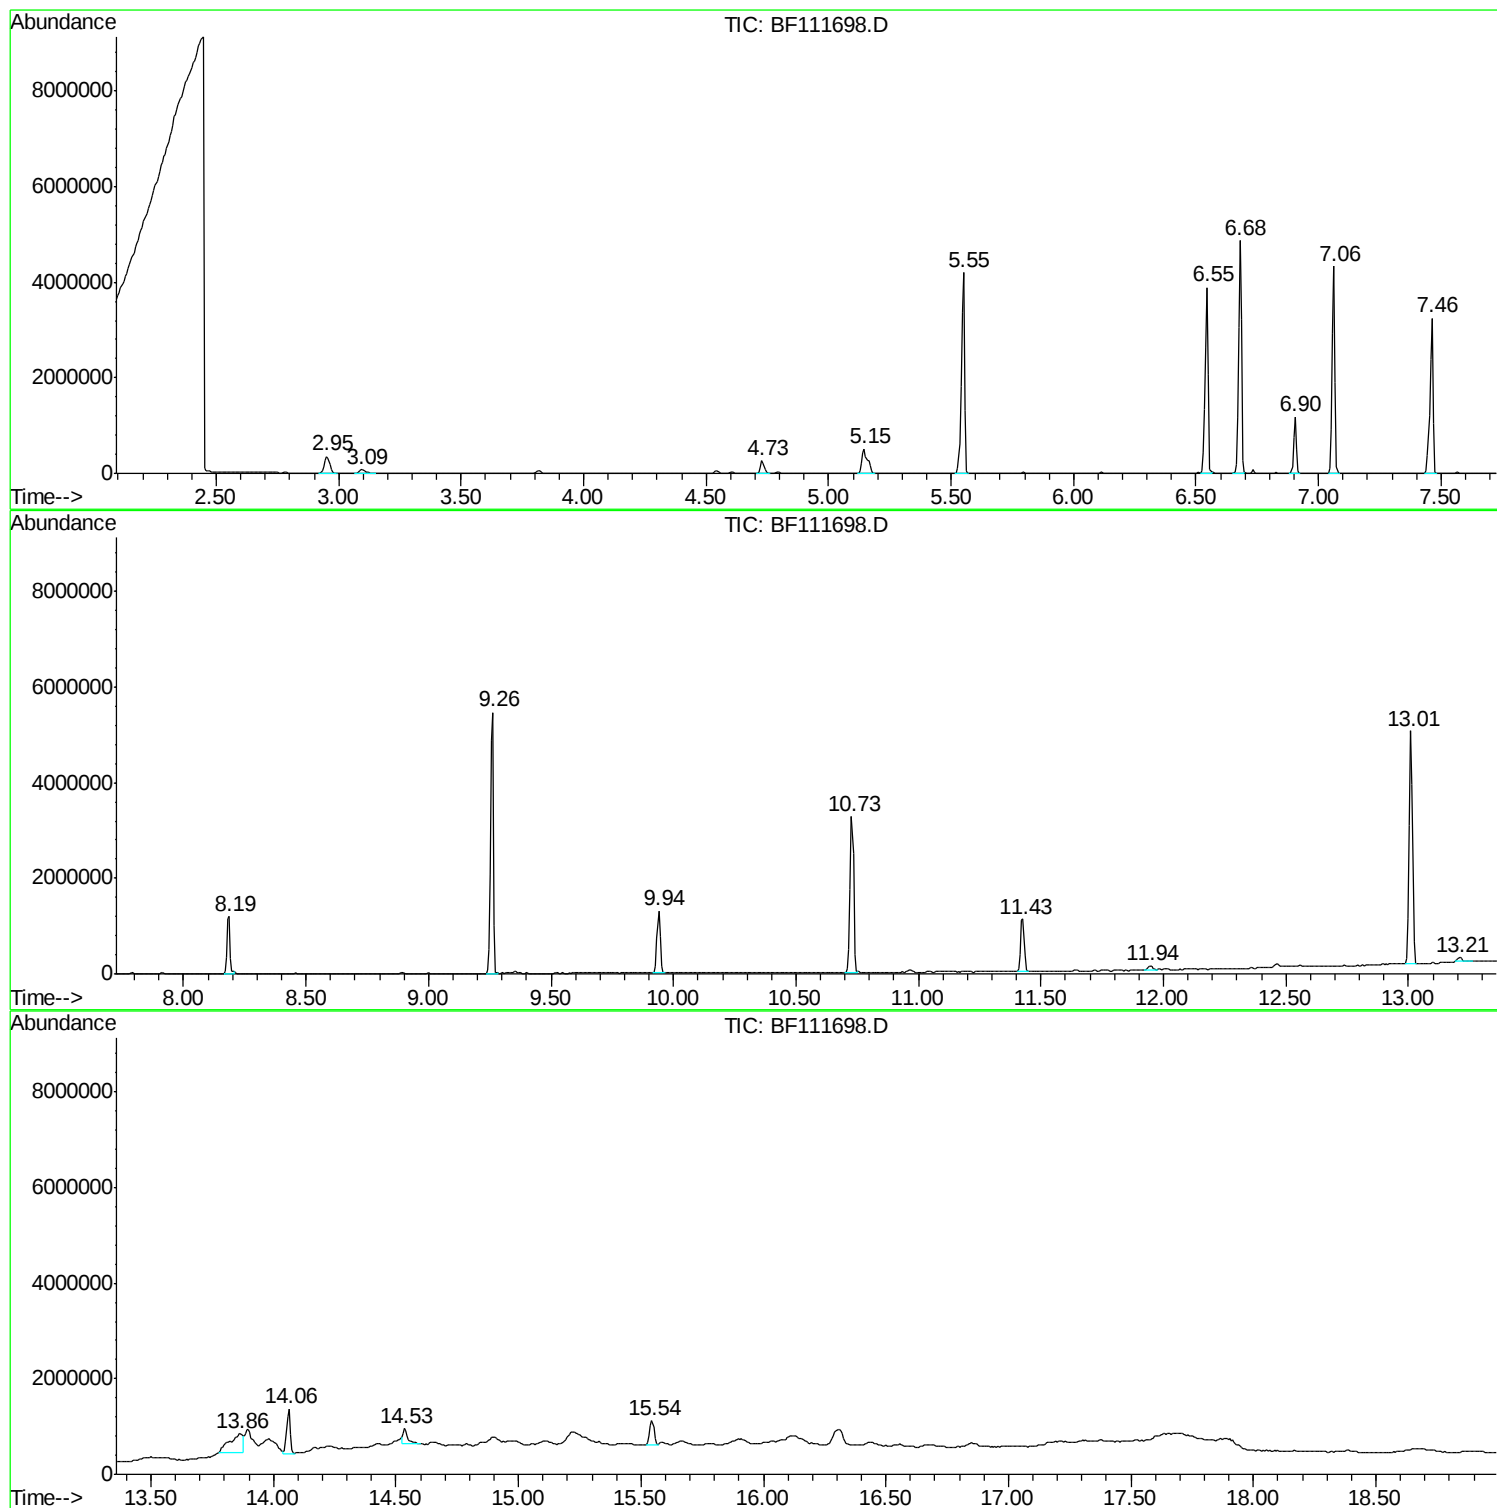

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122118\
Data_File : BF111698.D
Acq_On : 21-Dec-2018 20:144
Operator : JU/SJJ
Sample : J6188-044
Misc :
ALS_Vial : 19 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
BU-01-122018

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
