

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122118\
 Data File : BF111705.D
 Acq On : 21 Dec 2018 23:26
 Operator : JU/SJ
 Sample : PB115917BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB115917BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.140	511	519	528	rBV	195654	245837	5.58%	0.721%
2	5.540	582	587	590	rBV	4135358	4114199	93.39%	12.065%
3	6.540	751	757	760	rBV	3868892	4132714	93.81%	12.119%
4	6.675	775	780	784	rBV	4265011	4216160	95.70%	12.364%
5	6.898	815	818	822	rBV	955848	864812	19.63%	2.536%
6	7.063	841	846	849	rBV	3739705	3383035	76.79%	9.921%
7	7.463	908	914	917	rBV	2558356	2601432	59.05%	7.629%
8	8.181	1032	1036	1040	rBV	1107504	989730	22.47%	2.902%
9	9.257	1214	1219	1223	rBV	4672440	4405523	100.00%	12.919%
10	9.939	1331	1335	1339	rBV	1146861	952455	21.62%	2.793%
11	10.728	1464	1469	1472	rBV	2830412	2370073	53.80%	6.950%
12	11.422	1584	1587	1591	rBV	1034547	866993	19.68%	2.542%
13	13.010	1852	1857	1860	rBV	4127140	3726034	84.58%	10.927%
14	13.898	2004	2008	2014	rBV3	65784	105313	2.39%	0.309%
15	14.063	2032	2036	2039	rBV	710495	668120	15.17%	1.959%
16	15.545	2284	2288	2293	rVB	360975	458325	10.40%	1.344%


Sum of corrected areas: 34100755

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122118\
Data File : BF111705.D
Acq On : 21 Dec 2018 23:26
Operator : JU/SJ
Sample : PB115917BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB115917BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

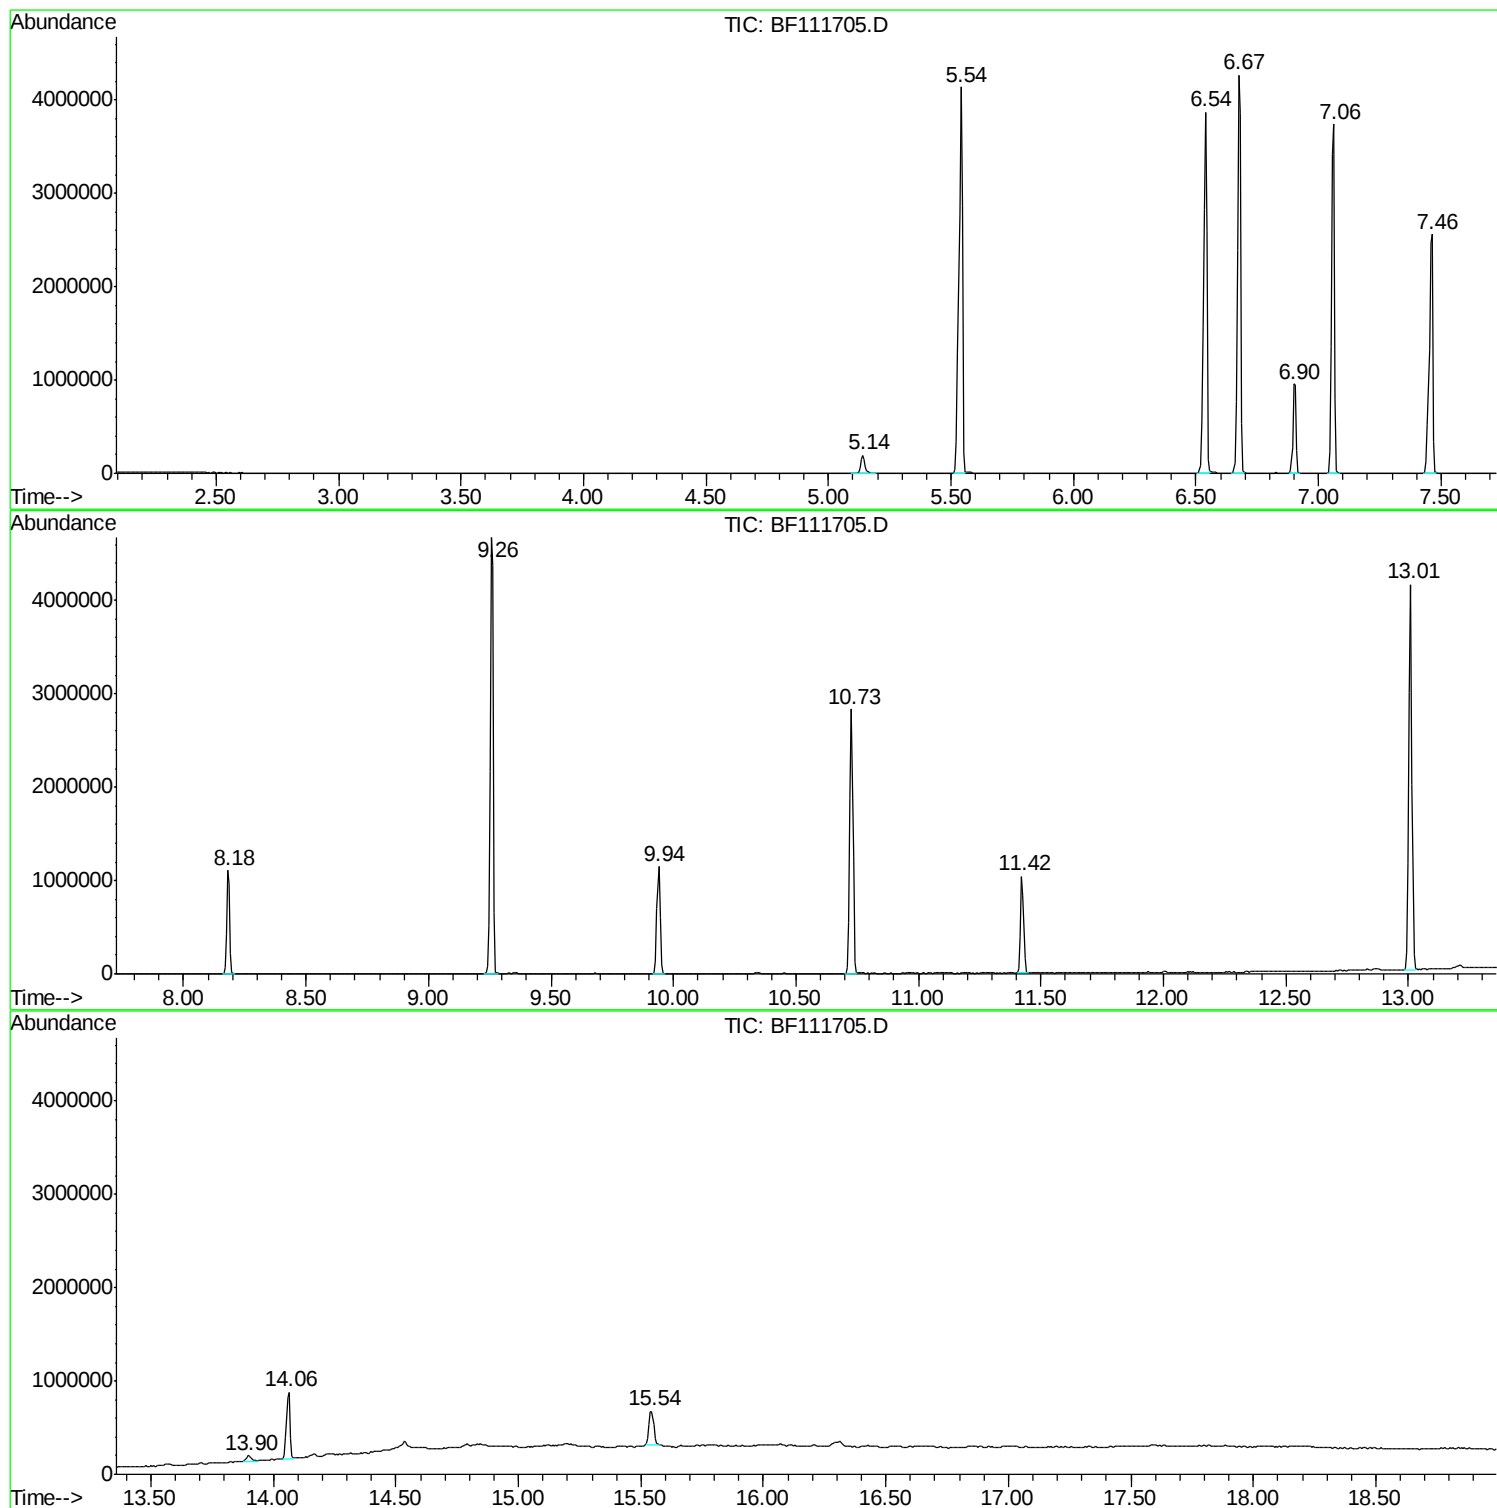

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122118\
Data_File : BF111705.D
Acq_On : 21-Dec-2018 23:266
Operator : JU/SJJ
Sample : PB115917BLL
Misc :
ALS_Vial : 26 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
PB115917BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
