


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122118\
 Data File : BF111680.D
 Acq On : 21 Dec 2018 11:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

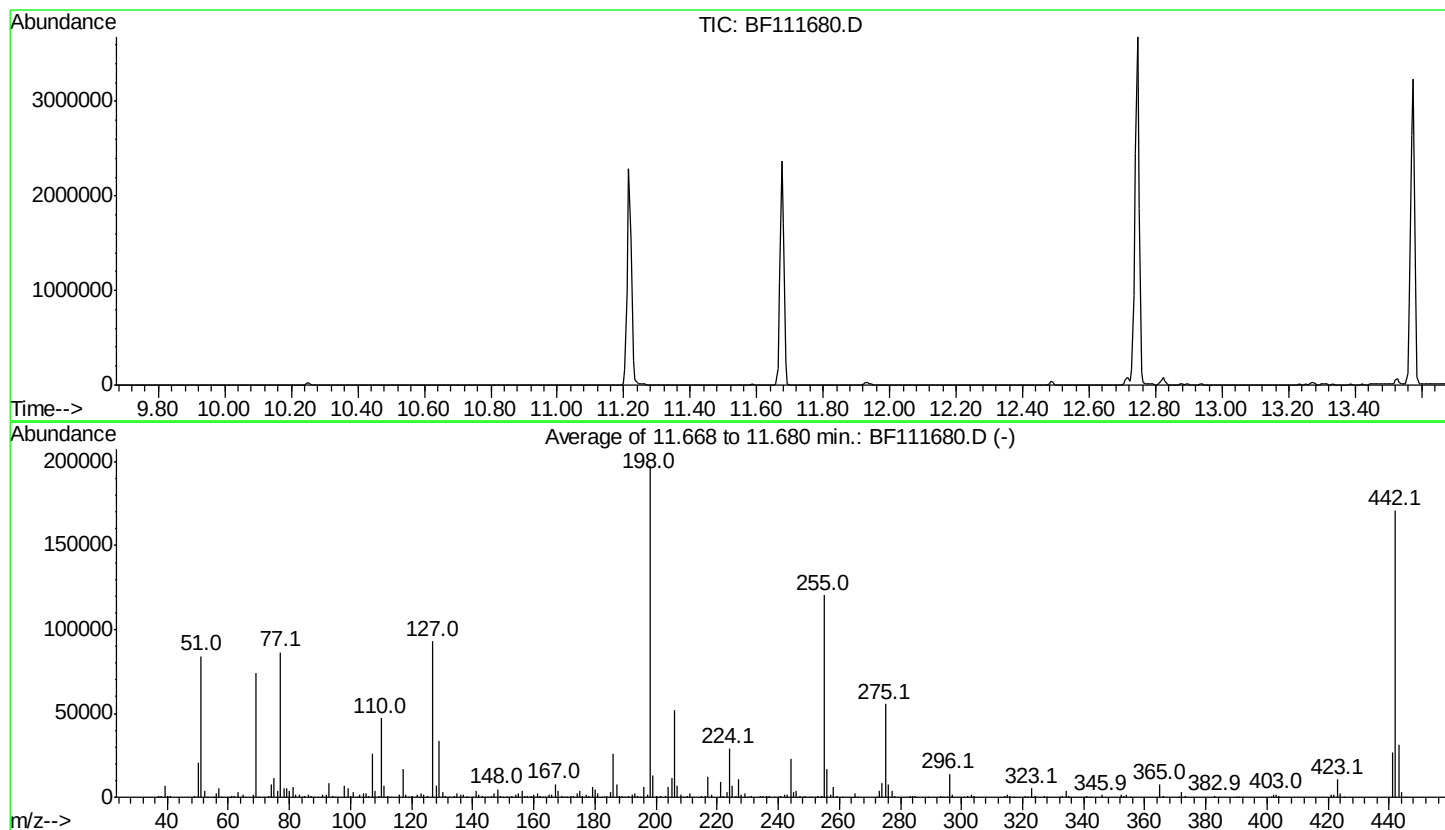

AutoFind: Scans 1629, 1630, 1631; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.5	84053	PASS
68	69	0.00	2	1.8	1345	PASS
69	198	0.00	100	37.3	73794	PASS
70	69	0.00	2	0.5	386	PASS
127	198	10	80	46.9	92752	PASS
197	198	0.00	2	0.8	1489	PASS
198	198	100	100	100.0	197704	PASS
199	198	5	9	6.5	12905	PASS
275	198	10	60	28.1	55554	PASS
365	198	1	100	3.8	7423	PASS
441	198	0.01	100	13.6	26800	PASS
442	198	50	100	86.3	170645	PASS
443	442	15	24	18.3	31244	PASS