
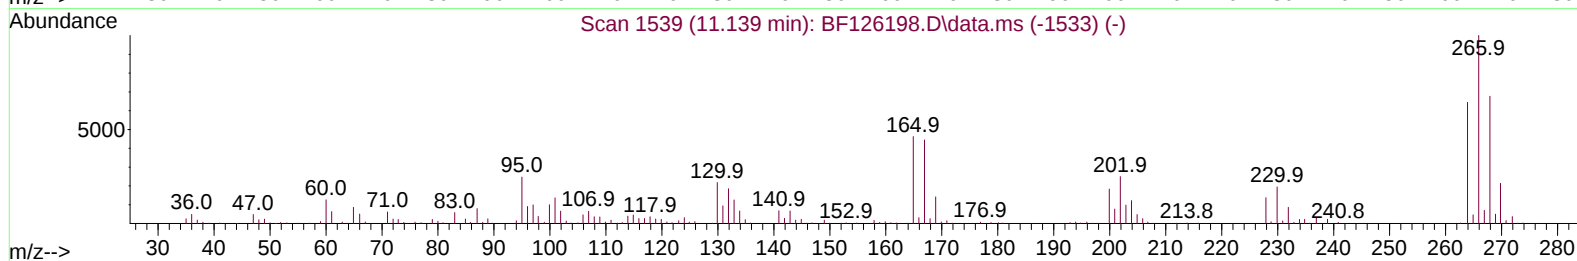
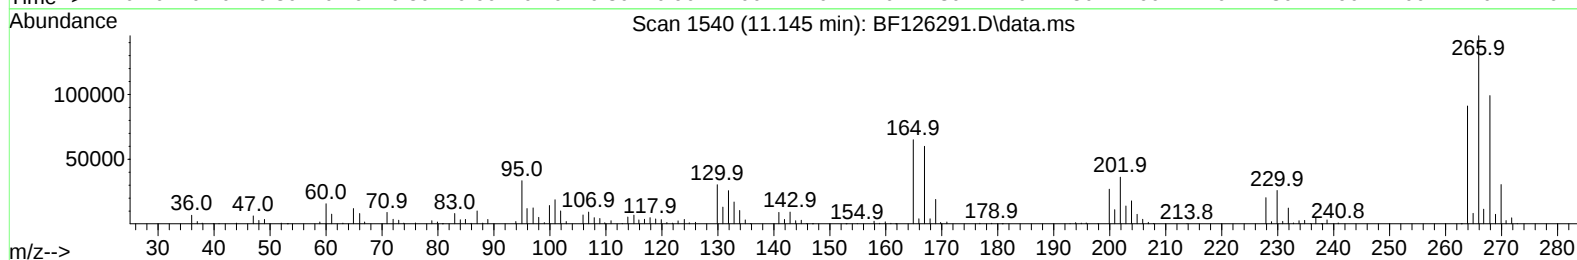


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126291.D
 Acq On : 21 Dec 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:34:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

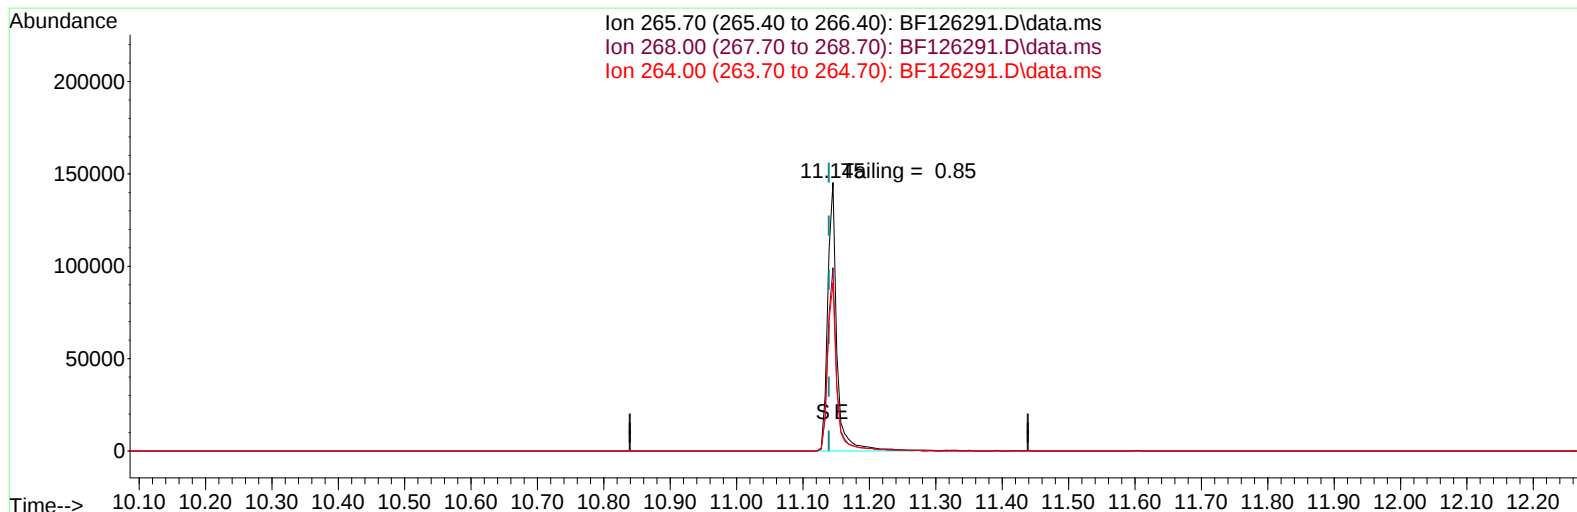

TIC: BF126291.D\data.ms

(70) Pentachlorophenol (C)




11.145min (+ 0.006) 38244.17 ng

response 139929

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.25
264.00	69.90	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126291.D
Acq On : 21 Dec 2021 9:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:34:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

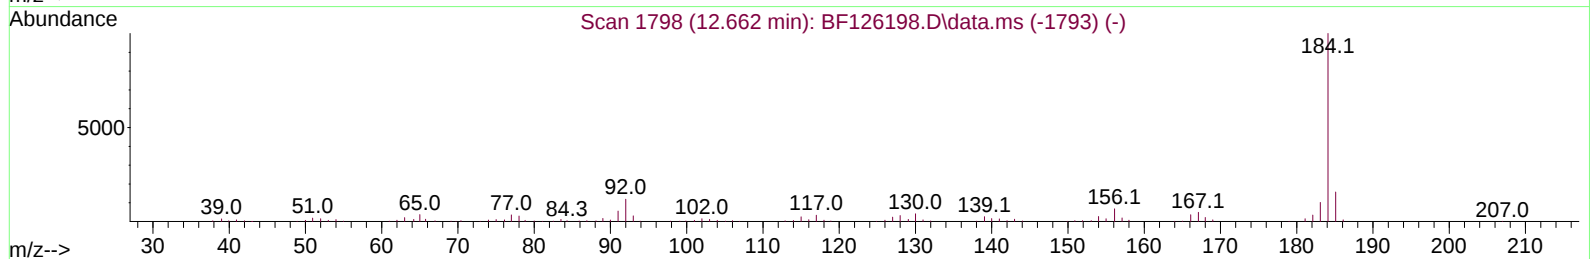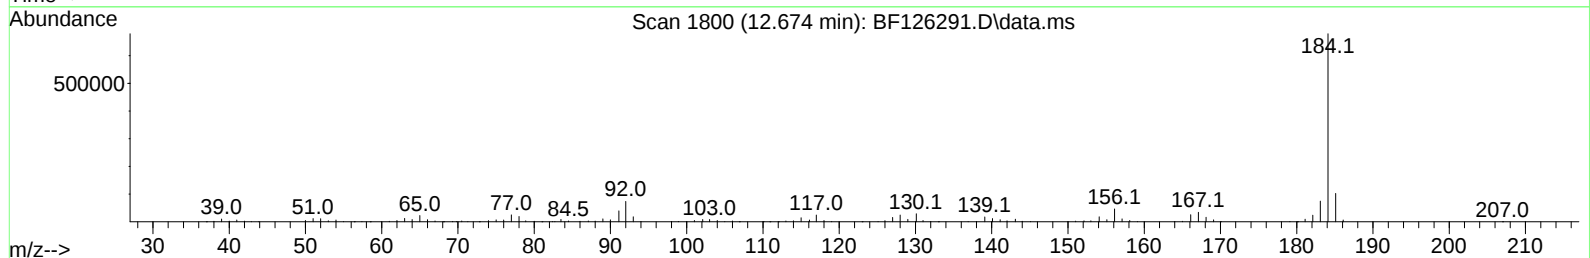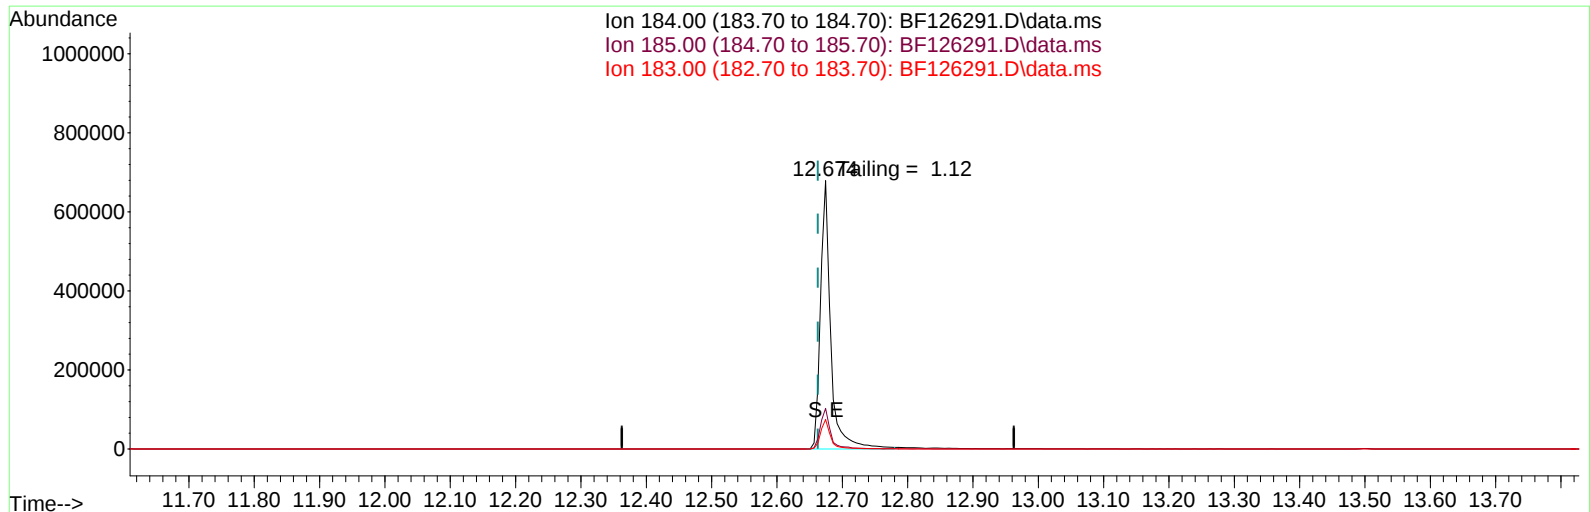

TIC: BF126291.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 749986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.15
183.00	10.10	11.01
0.00	0.00	0.00