
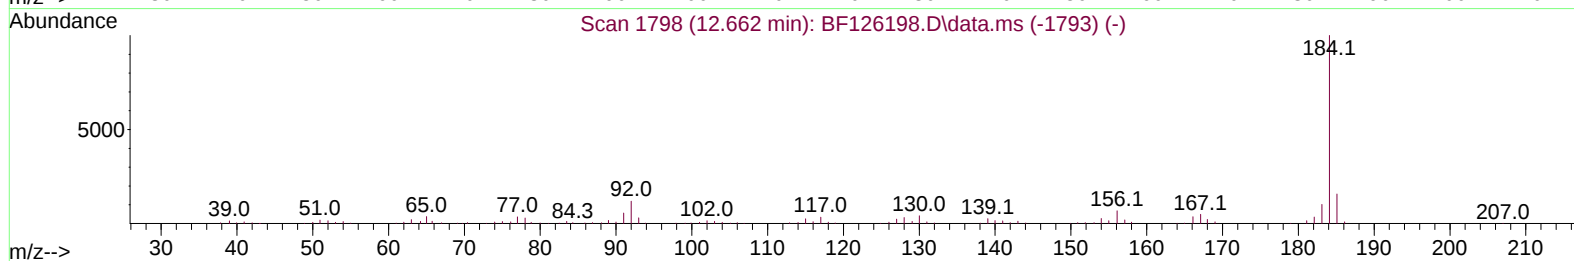
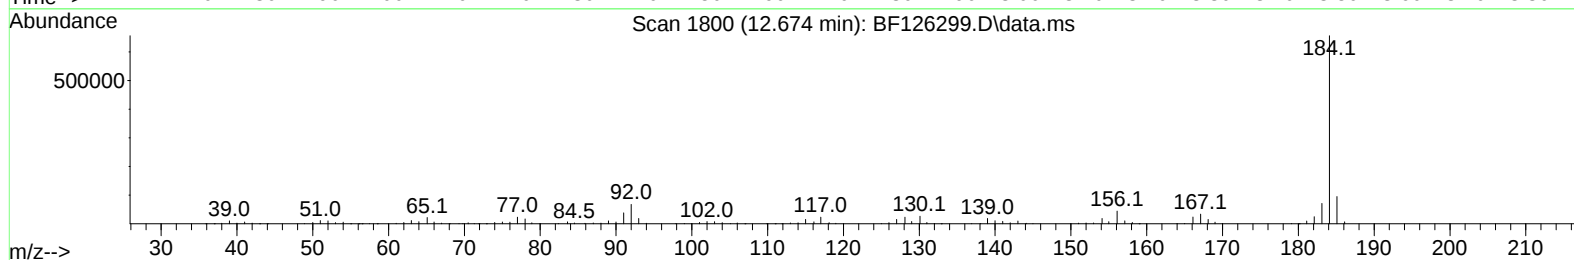


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126299.D
Acq On : 21 Dec 2021 16:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:36:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

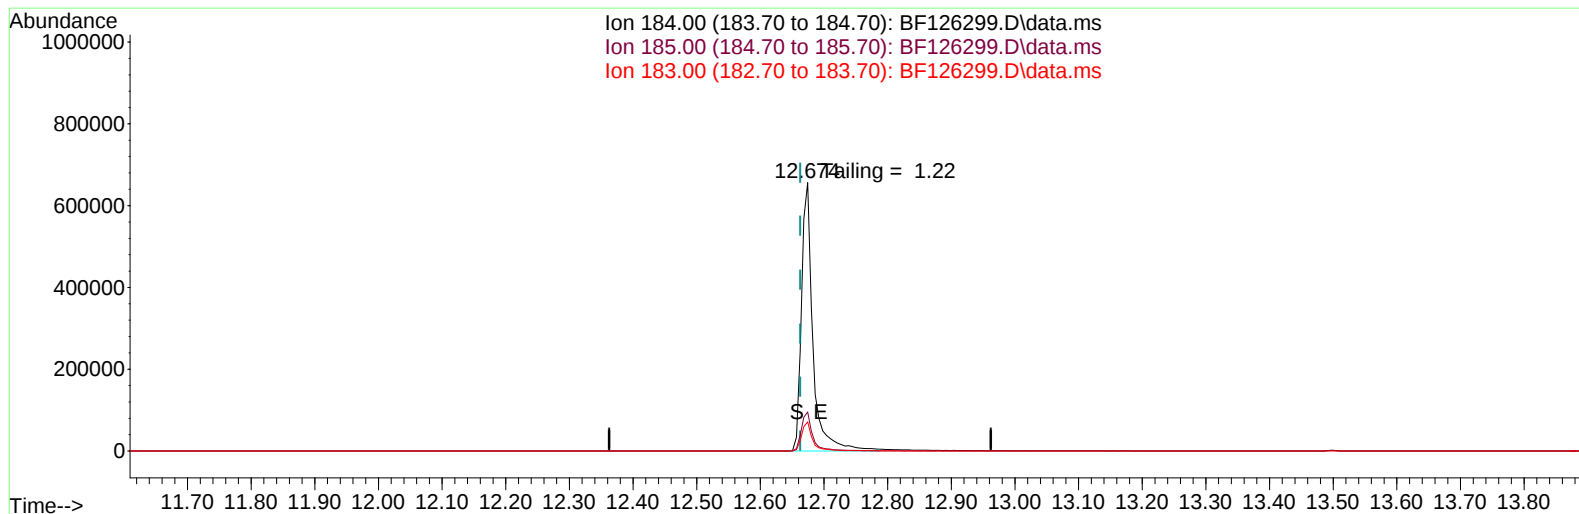

TIC: BF126299.D\data.ms

(77) Benzidine




12.674min (+ 0.012) 0.00 ng

response 837013

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.54
183.00	10.10	10.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126299.D
Acq On : 21 Dec 2021 16:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 22 08:36:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

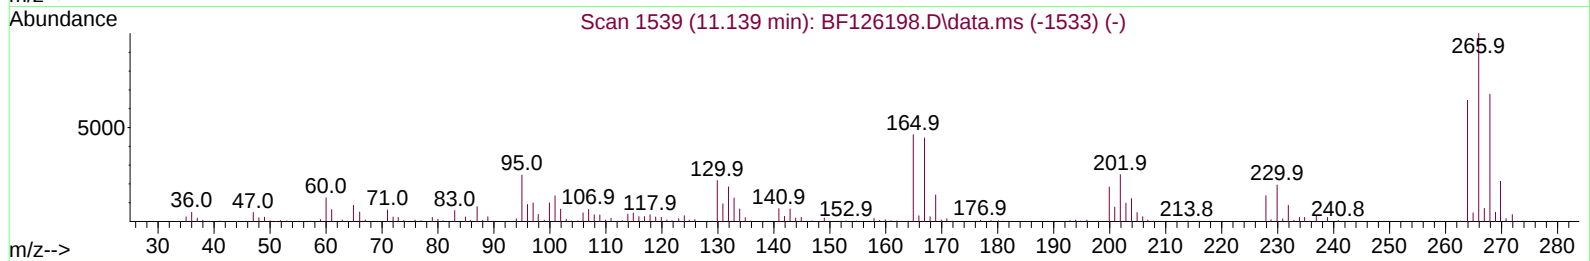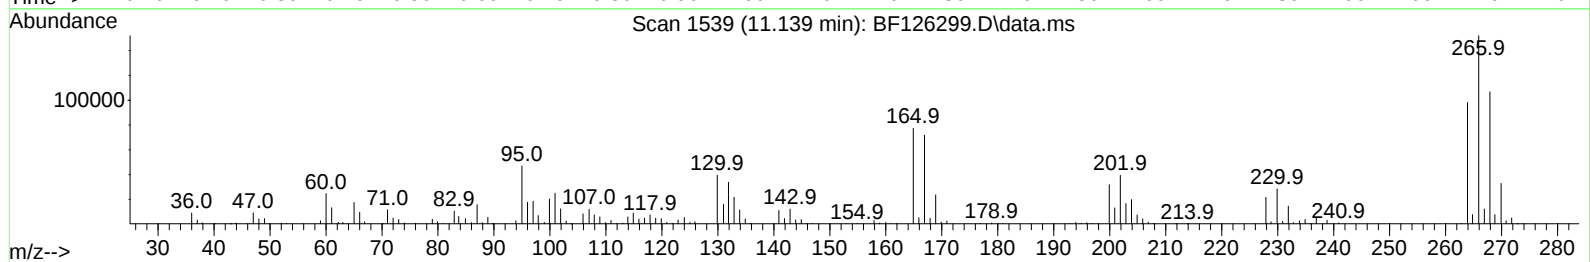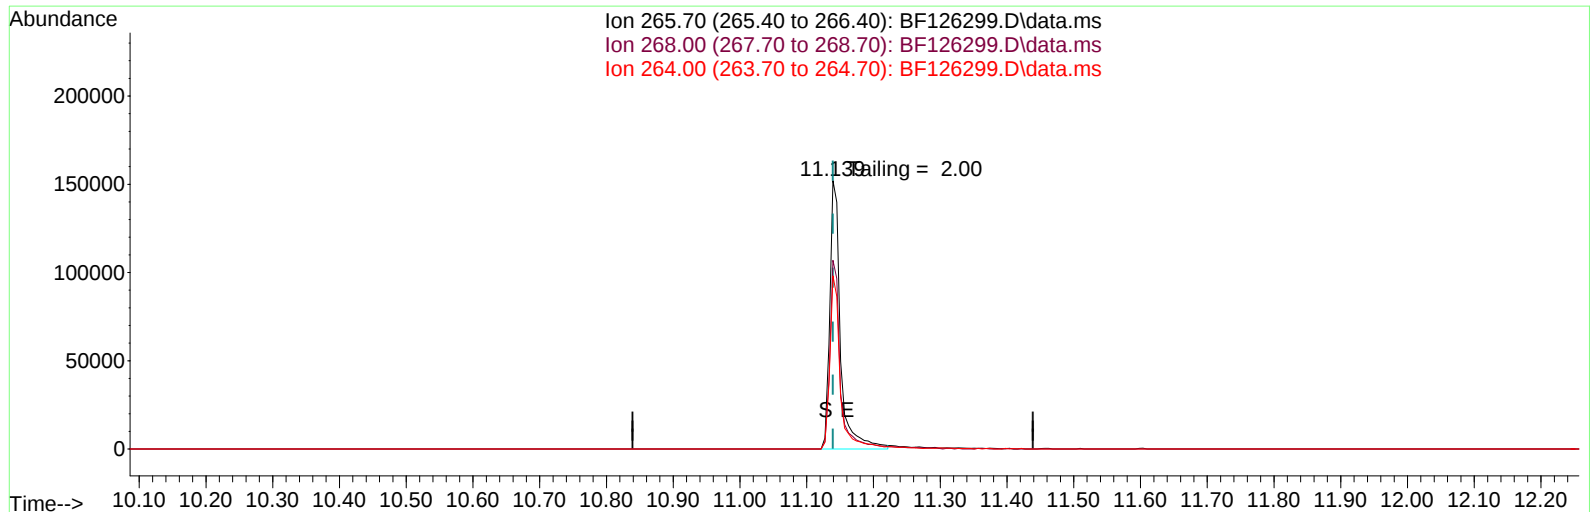

TIC: BF126299.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 38962.83 ng

response 174290

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.30
264.00	69.90	64.55
0.00	0.00	0.00