

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126320.D
 Acq On : 22 Dec 2021 3:31
 Operator : JU/CG
 Sample : M5178-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-122021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.869	298	303	311	rVB	24763	35393	2.20%	0.130%
2	5.422	563	567	582	rVB	891681	913743	56.80%	3.361%
3	6.434	735	739	753	rBV	999145	928713	57.73%	3.416%
4	6.645	772	775	780	rBV3	15024	20088	1.25%	0.074%
5	6.816	800	804	807	rBV	1441580	1196193	74.36%	4.400%
6	7.075	845	848	855	rVB	44193	42831	2.66%	0.158%
7	7.375	892	899	905	rBV	610972	619843	38.53%	2.280%
8	7.880	982	985	991	rVB2	14714	19176	1.19%	0.071%
9	8.098	1017	1022	1024	rBV	1888707	1608612	100.00%	5.917%
10	8.116	1024	1025	1032	rVB	240917	213858	13.29%	0.787%
11	8.698	1121	1124	1127	rBV	24364	22291	1.39%	0.082%
12	8.810	1138	1143	1150	rBV	374708	334520	20.80%	1.231%
13	8.910	1155	1160	1169	rVB	361975	326270	20.28%	1.200%
14	9.175	1201	1205	1216	rBV	1090611	970247	60.32%	3.569%
15	9.263	1216	1220	1225	rVV2	39999	57704	3.59%	0.212%
16	9.369	1236	1238	1243	rVB	37773	42581	2.65%	0.157%
17	9.439	1245	1250	1254	rBV	143500	197814	12.30%	0.728%
18	9.510	1258	1262	1265	rVV	237379	245661	15.27%	0.904%
19	9.539	1265	1267	1270	rVV	163009	140687	8.75%	0.518%
20	9.580	1270	1274	1278	rVV3	38155	48304	3.00%	0.178%
21	9.627	1279	1282	1288	rVB	109957	120981	7.52%	0.445%
22	9.710	1293	1296	1301	rVB	170539	145958	9.07%	0.537%
23	9.792	1308	1310	1314	rVB	28724	23755	1.48%	0.087%
24	9.851	1314	1320	1323	rBV	1658982	1571683	97.70%	5.781%
25	9.886	1323	1326	1330	rVB	369129	355942	22.13%	1.309%
26	9.957	1335	1338	1343	rVB2	31307	48707	3.03%	0.179%
27	10.010	1343	1347	1349	rBV3	16632	19660	1.22%	0.072%
28	10.057	1351	1355	1358	rVB	160167	141280	8.78%	0.520%
29	10.092	1358	1361	1365	rVB	52853	48417	3.01%	0.178%
30	10.169	1369	1374	1377	rBV2	62780	76440	4.75%	0.281%
31	10.198	1377	1379	1385	rVB	52744	42882	2.67%	0.158%
32	10.263	1385	1390	1391	rBV2	45861	56333	3.50%	0.207%
33	10.351	1399	1405	1407	rBV4	27433	35525	2.21%	0.131%
34	10.398	1410	1413	1419	rVV	423383	397292	24.70%	1.461%
35	10.451	1419	1422	1423	rVV2	29451	29649	1.84%	0.109%
36	10.463	1423	1424	1426	rVV	56403	44774	2.78%	0.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126320.D
 Acq On : 22 Dec 2021 3:31
 Operator : JU/CG
 Sample : M5178-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-122021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	10.486	1426	1428	1430	rVV2	51774	45980	2.86%	0.169%
38	10.510	1430	1432	1434	rVV2	42137	39116	2.43%	0.144%
39	10.557	1438	1440	1443	rVB	63374	55081	3.42%	0.203%
40	10.633	1448	1453	1458	rBV	462463	521943	32.45%	1.920%
41	10.763	1472	1475	1480	rVB3	63977	77334	4.81%	0.284%
42	10.945	1501	1506	1509	rBV2	89581	119375	7.42%	0.439%
43	10.974	1509	1511	1514	rVV2	67966	62371	3.88%	0.229%
44	11.027	1517	1520	1524	rVB	48222	50217	3.12%	0.185%
45	11.098	1530	1532	1534	rVB3	27920	22765	1.42%	0.084%
46	11.139	1537	1539	1543	rVB4	21969	24172	1.50%	0.089%
47	11.186	1544	1547	1549	rVV2	27782	31237	1.94%	0.115%
48	11.233	1552	1555	1561	rVB	171770	169762	10.55%	0.624%
49	11.339	1569	1573	1575	rBV	1505540	1487743	92.49%	5.473%
50	11.363	1575	1577	1580	rVV	1924312	1473566	91.60%	5.421%
51	11.410	1582	1585	1589	rVV	507539	455722	28.33%	1.676%
52	11.445	1589	1591	1595	rVB2	52596	51286	3.19%	0.189%
53	11.563	1608	1611	1614	rBV	89568	91715	5.70%	0.337%
54	11.592	1614	1616	1620	rVB4	21616	19679	1.22%	0.072%
55	11.633	1620	1623	1626	rBV	62543	56578	3.52%	0.208%
56	11.668	1626	1629	1638	rVV2	63547	98294	6.11%	0.362%
57	11.751	1640	1643	1646	rVB	50277	52588	3.27%	0.193%
58	11.839	1655	1658	1660	rBV	205577	182048	11.32%	0.670%
59	11.868	1660	1663	1666	rVV	239801	223397	13.89%	0.822%
60	11.910	1667	1670	1673	rVV2	88213	94543	5.88%	0.348%
61	11.951	1673	1677	1679	rVV	384681	384048	23.87%	1.413%
62	11.968	1679	1680	1686	rVB2	133134	114037	7.09%	0.419%
63	12.015	1686	1688	1690	rBV3	19178	18929	1.18%	0.070%
64	12.045	1690	1693	1695	rVB2	29783	23060	1.43%	0.085%
65	12.133	1705	1708	1710	rBV	138474	121843	7.57%	0.448%
66	12.280	1731	1733	1736	rVB	26505	23034	1.43%	0.085%
67	12.315	1736	1739	1741	rBV2	36131	40062	2.49%	0.147%
68	12.386	1747	1751	1754	rBV2	97479	113158	7.03%	0.416%
69	12.427	1754	1758	1763	rVB3	85360	128722	8.00%	0.474%
70	12.474	1763	1766	1771	rBV5	45023	87847	5.46%	0.323%
71	12.551	1775	1779	1782	rBV	1439274	1300649	80.86%	4.784%
72	12.639	1792	1794	1797	rBV	32635	29934	1.86%	0.110%
73	12.698	1802	1804	1807	rVV	50953	49256	3.06%	0.181%
74	12.774	1811	1817	1821	rBV	1164106	1340083	83.31%	4.930%
75	12.827	1823	1826	1831	rVB2	106714	147494	9.17%	0.543%
76	12.898	1835	1838	1839	rBV	58021	55530	3.45%	0.204%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126320.D
 Acq On : 22 Dec 2021 3:31
 Operator : JU/CG
 Sample : M5178-01 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-122021

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	12.921	1839	1842	1849	rVB	705444	656386	40.80%	2.415%
78	12.992	1851	1854	1857	rBV2	68083	92131	5.73%	0.339%
79	13.080	1867	1869	1870	rBV2	42010	33223	2.07%	0.122%
80	13.104	1870	1873	1876	rVB	204472	197217	12.26%	0.725%
81	13.168	1881	1884	1887	rVB	172804	155173	9.65%	0.571%
82	13.210	1887	1891	1893	rBV2	105062	110203	6.85%	0.405%
83	13.298	1904	1906	1909	rVB	49389	44247	2.75%	0.163%
84	13.333	1909	1912	1915	rBV	59425	57950	3.60%	0.213%
85	13.504	1939	1941	1944	rBV3	42730	42888	2.67%	0.158%
86	13.721	1976	1978	1981	rVB	54299	42675	2.65%	0.157%
87	13.751	1981	1983	1985	rBV	75520	54332	3.38%	0.200%
88	13.774	1985	1987	1991	rVV2	64278	69010	4.29%	0.254%
89	13.974	2016	2021	2023	rBV2	996587	1279312	79.53%	4.706%
90	13.998	2023	2025	2031	rVB	464102	420400	26.13%	1.546%
91	14.074	2034	2038	2043	rVB2	410525	477003	29.65%	1.755%
92	14.457	2100	2103	2105	rBV2	67896	64400	4.00%	0.237%
93	15.004	2192	2196	2206	rBV	397211	809165	50.30%	2.977%
94	15.298	2243	2246	2252	rVB	229017	298219	18.54%	1.097%
95	15.362	2253	2257	2263	rBV	344245	433922	26.97%	1.596%
96	15.427	2263	2268	2271	rBV	601950	790785	49.16%	2.909%
97	16.856	2506	2511	2519	rVB2	142890	283173	17.60%	1.042%
98	17.280	2580	2583	2588	rVB	85896	144948	9.01%	0.533%


Sum of corrected areas: 27184767

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

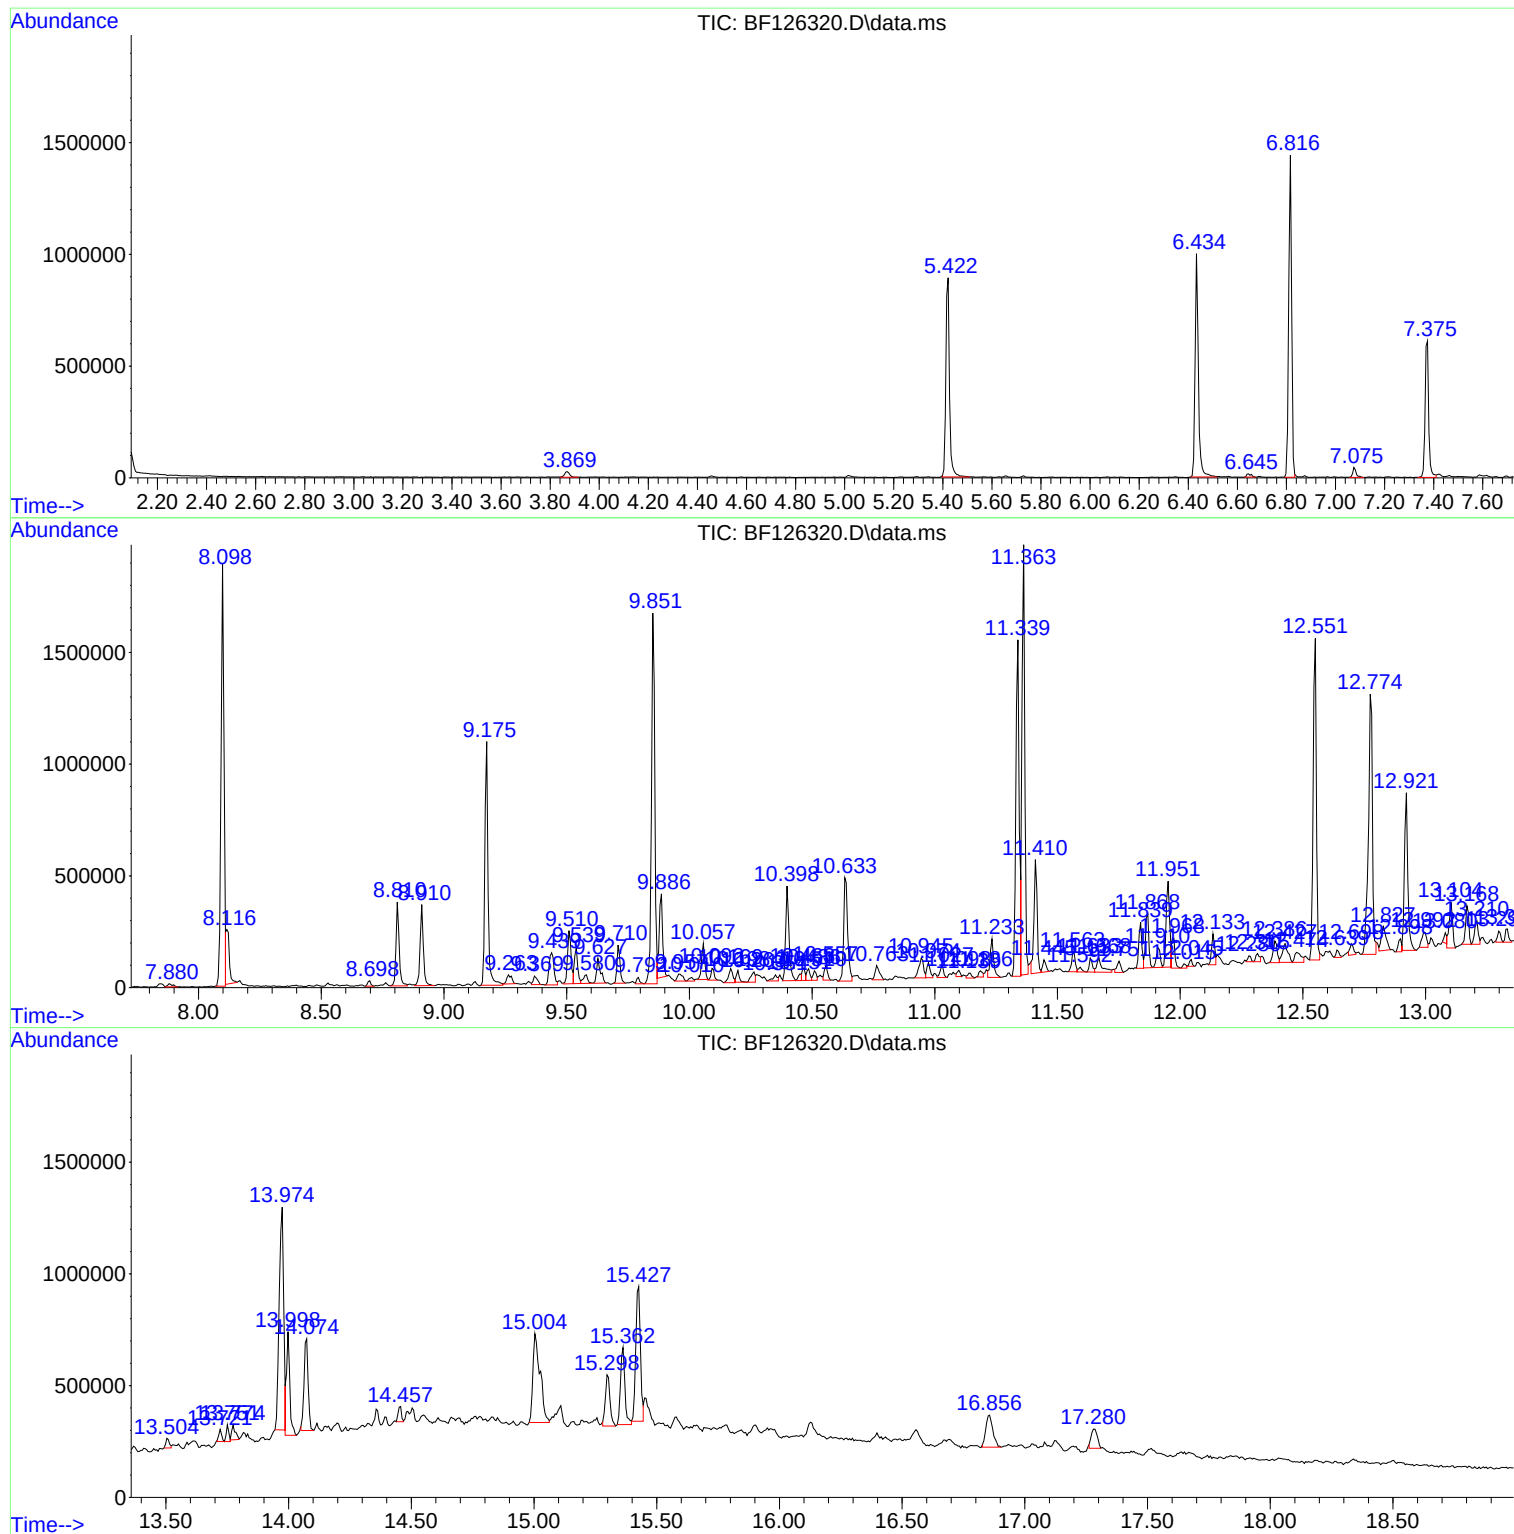

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Naphthalene, 2,6-dimethyl- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.439	2.52 ng	197814	Acenaphthene-d10	9.851

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 2,6-dimethyl-	156	C12H12	000581-42-0	98
2			Naphthalene, 1,6-dimethyl-	156	C12H12	000575-43-9	98
3			Naphthalene, 1,3-dimethyl-	156	C12H12	000575-41-7	96
4			Naphthalene, 1,7-dimethyl-	156	C12H12	000575-37-1	96
5			Naphthalene, 2,7-dimethyl-	156	C12H12	000582-16-1	96

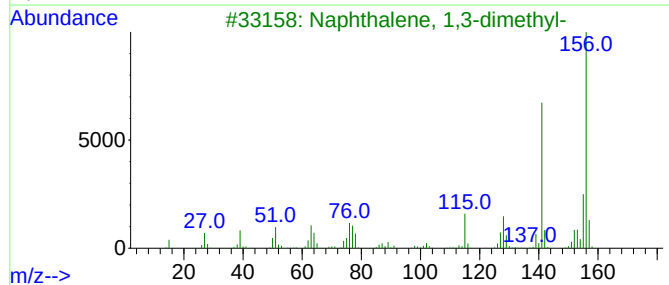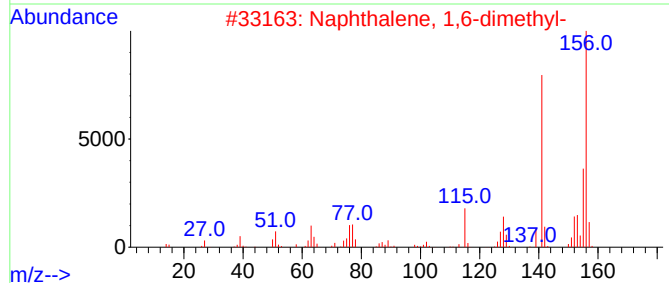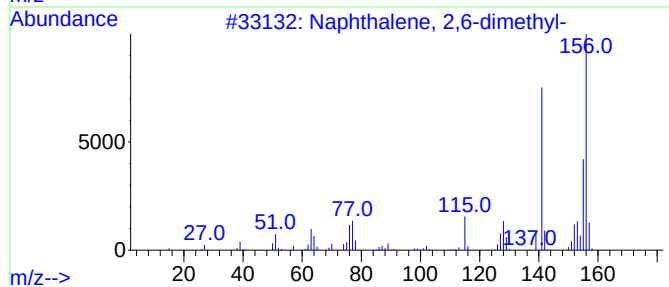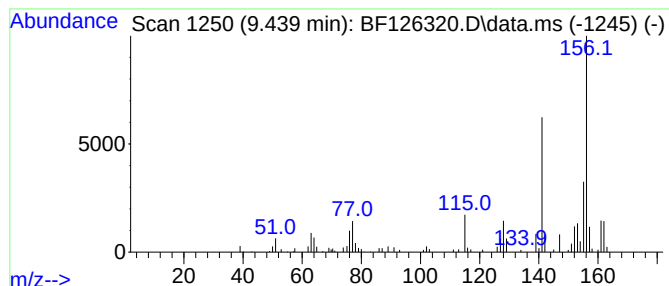

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Naphthalene, 1,7-dimethyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
9.510	3.13 ng	245661	Acenaphthene-d10	9.851

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Naphthalene, 1,7-dimethyl-	156	C12H12	000575-37-1	98
2			Naphthalene, 2,3-dimethyl-	156	C12H12	000581-40-8	98
3			Naphthalene, 1,3-dimethyl-	156	C12H12	000575-41-7	98
4			Naphthalene, 1,4-dimethyl-	156	C12H12	000571-58-4	97
5			Naphthalene, 1,6-dimethyl-	156	C12H12	000575-43-9	97

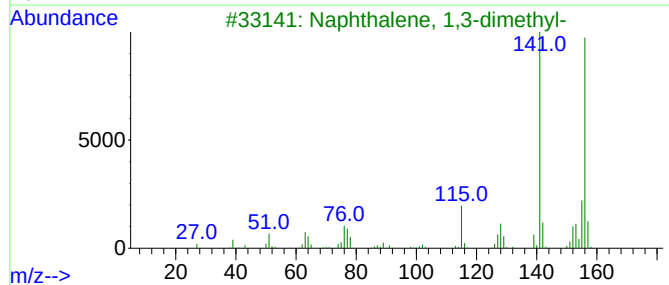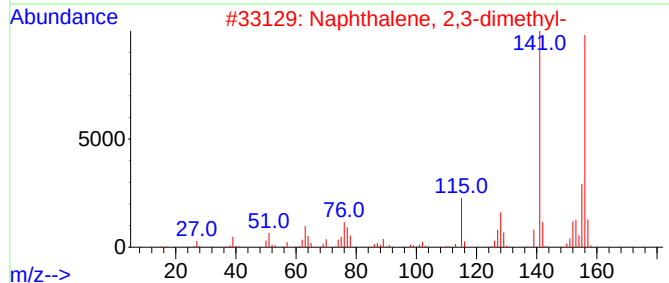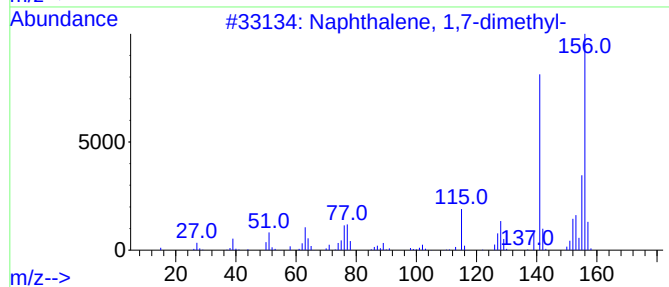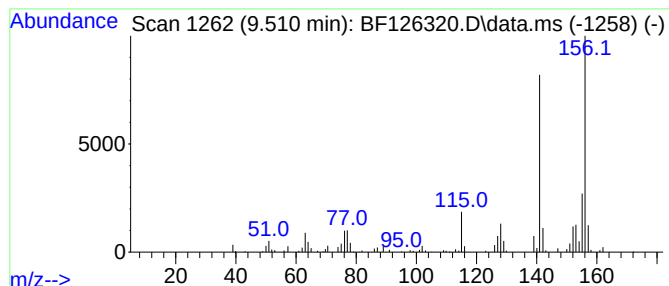

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Dibenzothiophene Concentration Rank 10

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.233	2.28 ng	169762	Phenanthrene-d10	11.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dibenzothiophene	184	C12H8S	000132-65-0	96
2			Naphtho[1,2-b]thiophene	184	C12H8S	000234-41-3	96
3			Naphtho[2,3-b]thiophene	184	C12H8S	000268-77-9	95
4			Azuleno(2,1-b)thiophene	184	C12H8S	000248-13-5	94
5			Naphtho[2,1-b]thiophene	184	C12H8S	000233-02-3	86

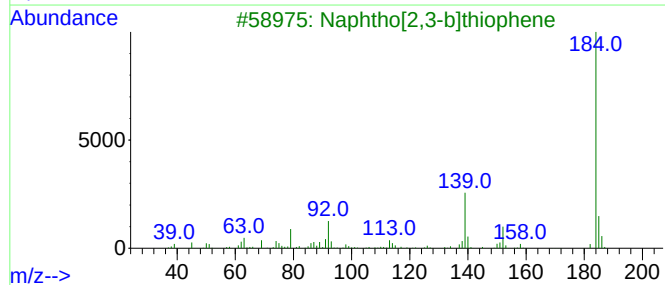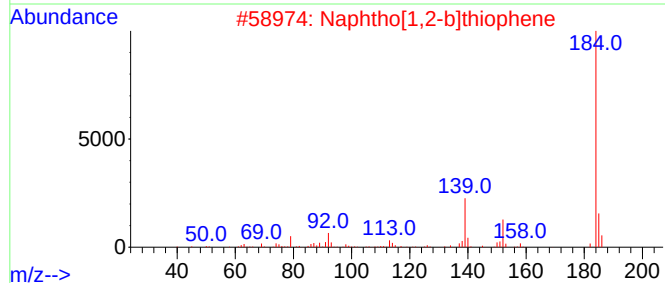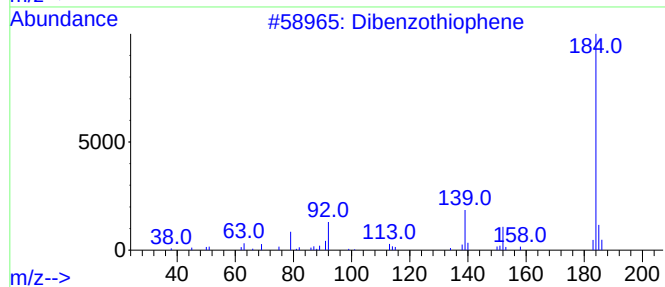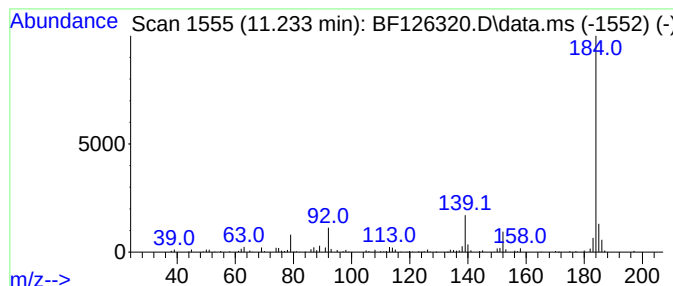

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Anthracene, 2-methyl- Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.839	2.45 ng	182048	Phenanthrene-d10	11.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Anthracene, 2-methyl-	192	C15H12	000613-12-7	95
2			Anthracene, 1-methyl-	192	C15H12	000610-48-0	94
3			Anthracene, 9-methyl-	192	C15H12	000779-02-2	93
4			Phenanthrene, 2-methyl-	192	C15H12	002531-84-2	92
5			Naphtho[2,3-b]norbornadiene	192	C15H12	107426-38-0	87

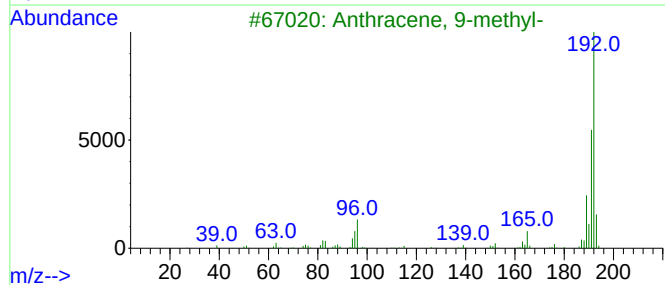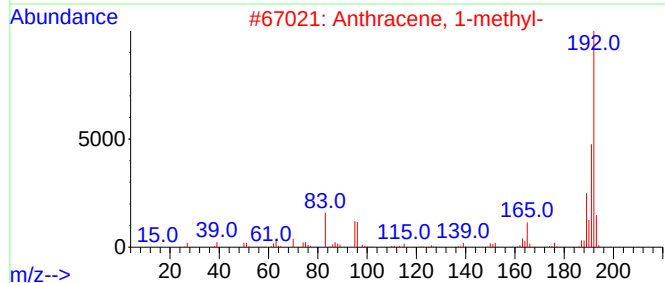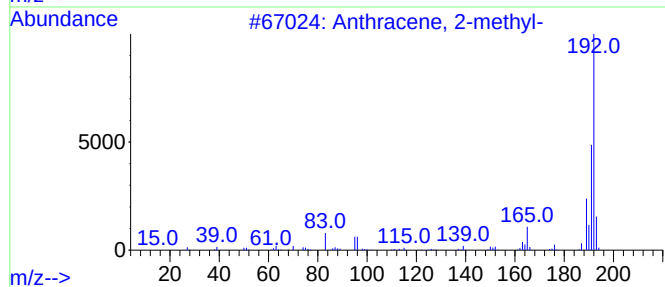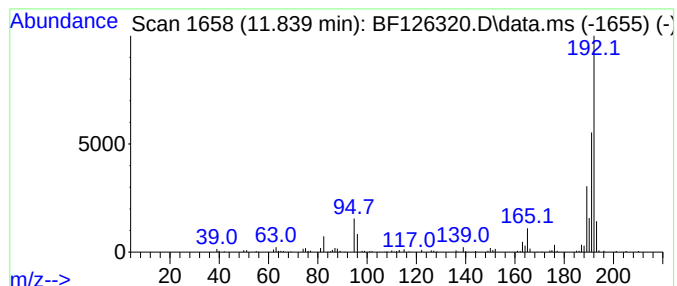

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Phenanthrene, 2-methyl- Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.868	3.00 ng	223397	Phenanthrene-d10	11.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Phenanthrene, 2-methyl-	192	C15H12	002531-84-2	97
2			Phenanthrene, 1-methyl-	192	C15H12	000832-69-9	96
3			Anthracene, 2-methyl-	192	C15H12	000613-12-7	96
4			Anthracene, 9-methyl-	192	C15H12	000779-02-2	96
5			Phenanthrene, 3-methyl-	192	C15H12	000832-71-3	94

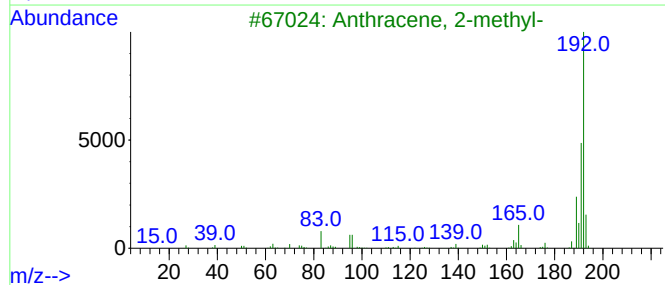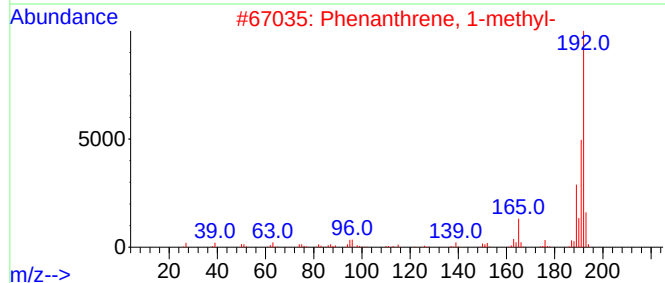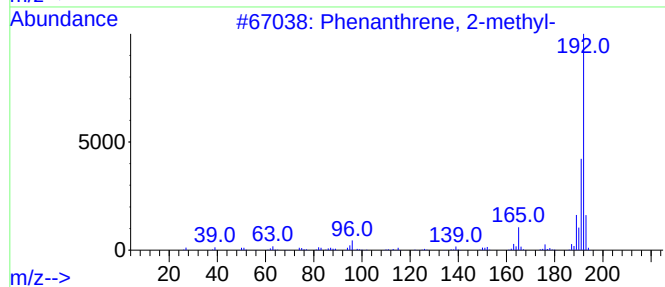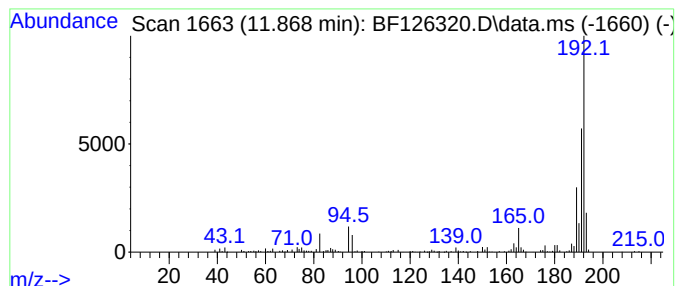

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 4H-Cyclopenta[def]phenanthrene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.951	5.16 ng	384048	Phenanthrene-d10	11.339

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4H-Cyclopenta[def]phenanthrene	190	C15H10	000203-64-5	81
2			Thiophene-3-carboxaldehyde, 5-ch...	190	C5H4BClO3S	036155-87-0	50
3			2,3,5,6-Tetramethylterephthalald...	190	C12H14O2	007072-01-7	47
4			2,2'-Bis(4,5-dimethylimidazole)	190	C10H14N4	069286-06-2	47
5			2,4(1H,3H)-Pyrimidinedione, 5-br...	190	C4H3BrN2O2	000051-20-7	16

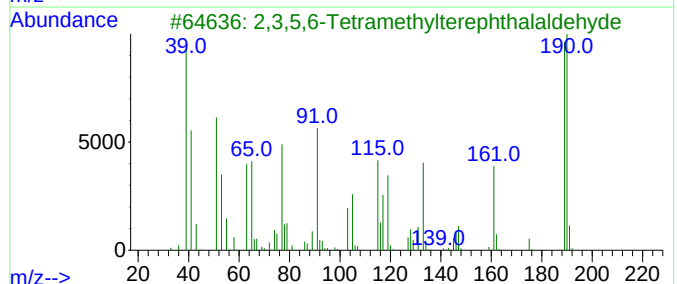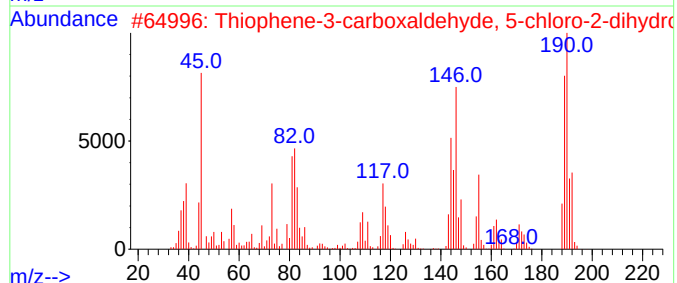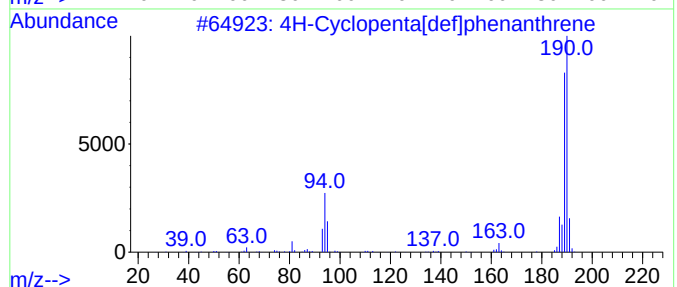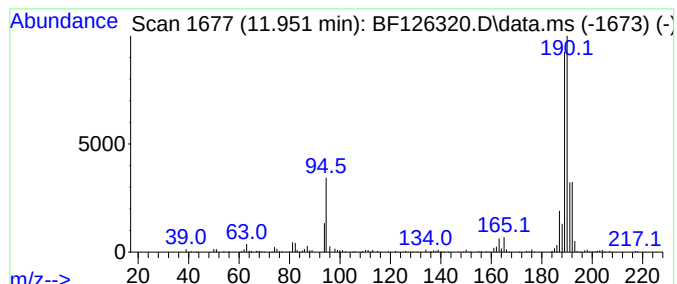

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 11H-Benzo[b]fluorene Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.104	3.08 ng	197217	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			11H-Benzo[b]fluorene	216	C17H12	000243-17-4	93
2			11H-Benzo[a]fluorene	216	C17H12	000238-84-6	90
3			Fluoranthene, 2-methyl-	216	C17H12	033543-31-6	90
4			Pyrene, 1-methyl-	216	C17H12	002381-21-7	87
5			7H-Benzo[c]fluorene	216	C17H12	000205-12-9	81

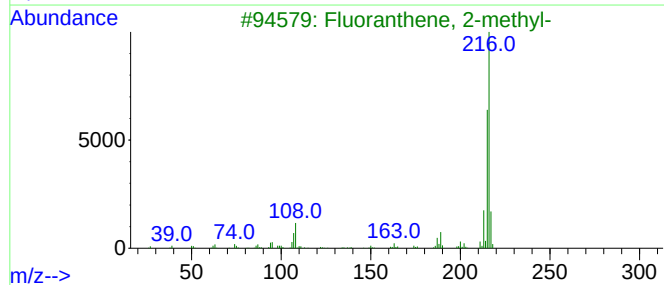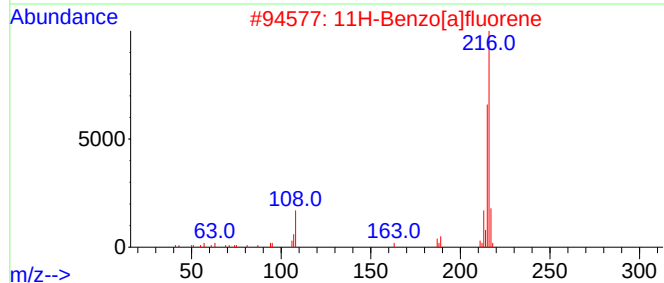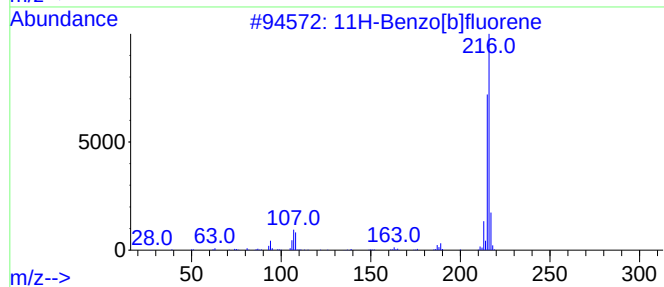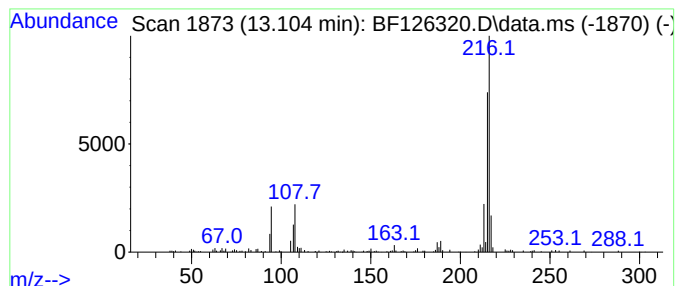

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Pyrene, 1-methyl- Concentration Rank 9

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.168	2.43 ng	155173	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			11H-Benzo[b]fluorene	216	C17H12	000243-17-4	93
2			Pyrene, 1-methyl-	216	C17H12	002381-21-7	81
3			11H-Benzo[a]fluorene	216	C17H12	000238-84-6	76
4			7H-Benzo[c]fluorene	216	C17H12	000205-12-9	64
5			Fluoranthene, 2-methyl-	216	C17H12	033543-31-6	62

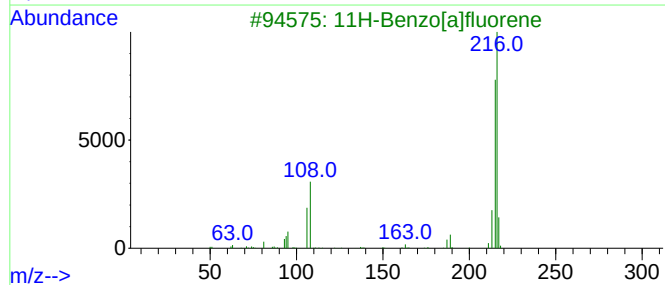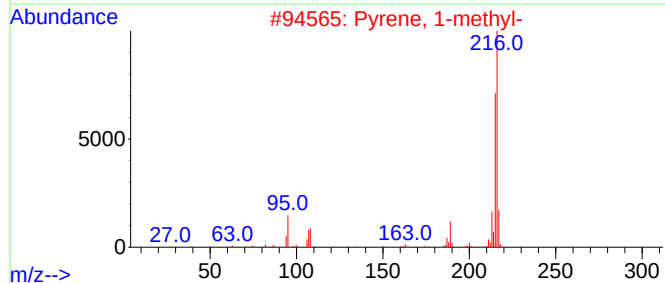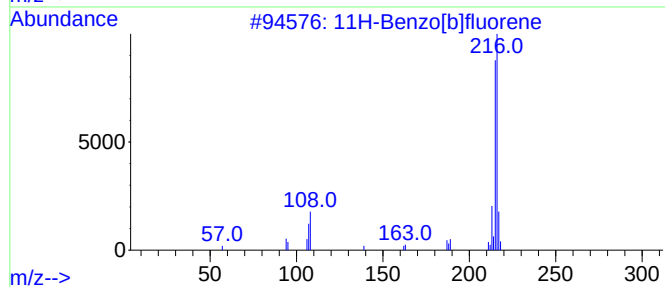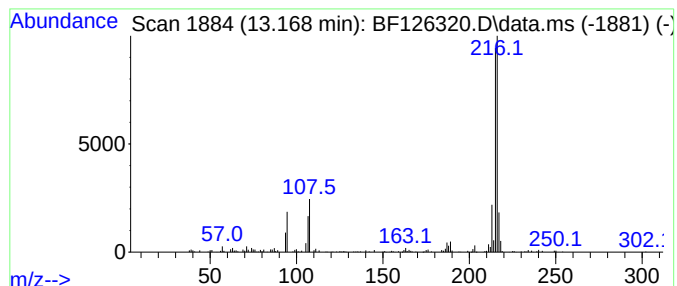

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 9 Triphenylphosphine oxide Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.074	7.46 ng	477003	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	90
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19N03S	1000483-83-4	68
3			(Carbethoxymethyl)-triphenylphos...	428	C22H22BrO2P	001530-45-6	53
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	43
5			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	40

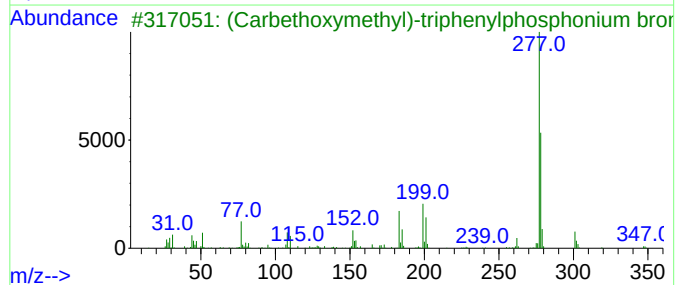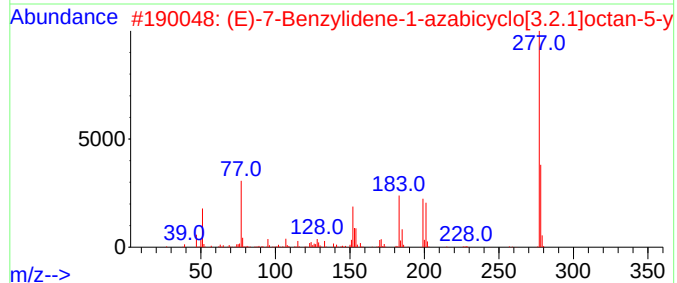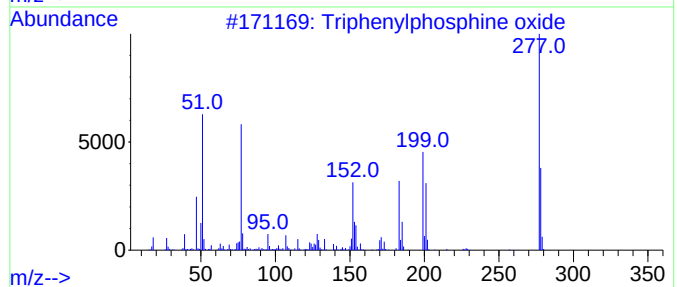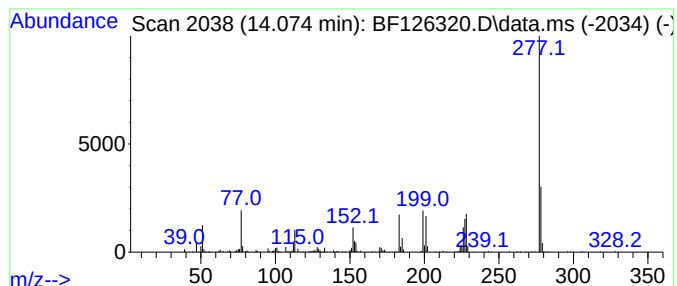

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 Perylene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.298	7.54 ng	298219	Perylene-d12	15.427

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Perylene	252	C20H12	000198-55-0	98
2			Benzo[e]pyrene	252	C20H12	000192-97-2	97
3			Benzo[b]fluoranthene	252	C20H12	000205-99-2	96
4			Benzo[a]pyrene	252	C20H12	000050-32-8	96
5			Benzo[k]fluoranthene	252	C20H12	000207-08-9	93

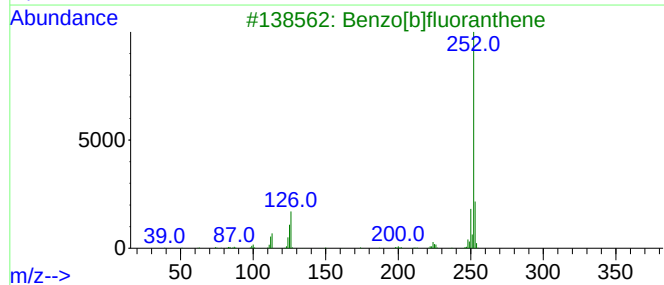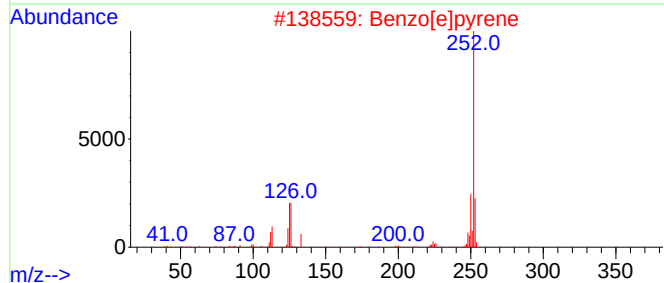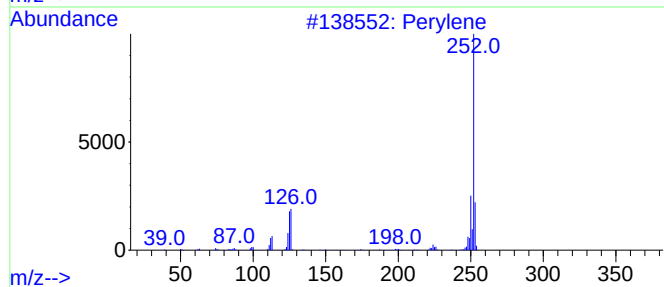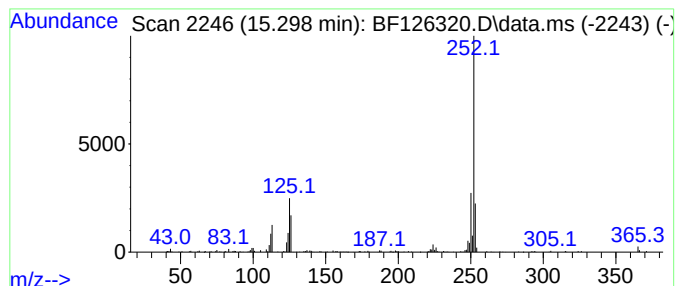

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126320.D
Acq On : 22 Dec 2021 3:31
Operator : JU/CG
Sample : M5178-01 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-122021

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Naphthalene, 2,...	9.439	2.5	ng	197814	3	9.851	1571680	20.0
Naphthalene, 1,...	9.510	3.1	ng	245661	3	9.851	1571680	20.0
Dibenzothiophene	11.233	2.3	ng	169762	4	11.339	1487740	20.0
Anthracene, 2-m...	11.839	2.5	ng	182048	4	11.339	1487740	20.0
Phenanthrene, 2...	11.868	3.0	ng	223397	4	11.339	1487740	20.0
4H-Cyclopenta[d...	11.951	5.2	ng	384048	4	11.339	1487740	20.0
11H-Benzo[b]flu...	13.104	3.1	ng	197217	5	13.974	1279310	20.0
Pyrene, 1-methyl-	13.168	2.4	ng	155173	5	13.974	1279310	20.0
Triphenylphosph...	14.074	7.5	ng	477003	5	13.974	1279310	20.0
Perylene	15.298	7.5	ng	298219	6	15.427	790785	20.0