


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126291.D
 Acq On : 21 Dec 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

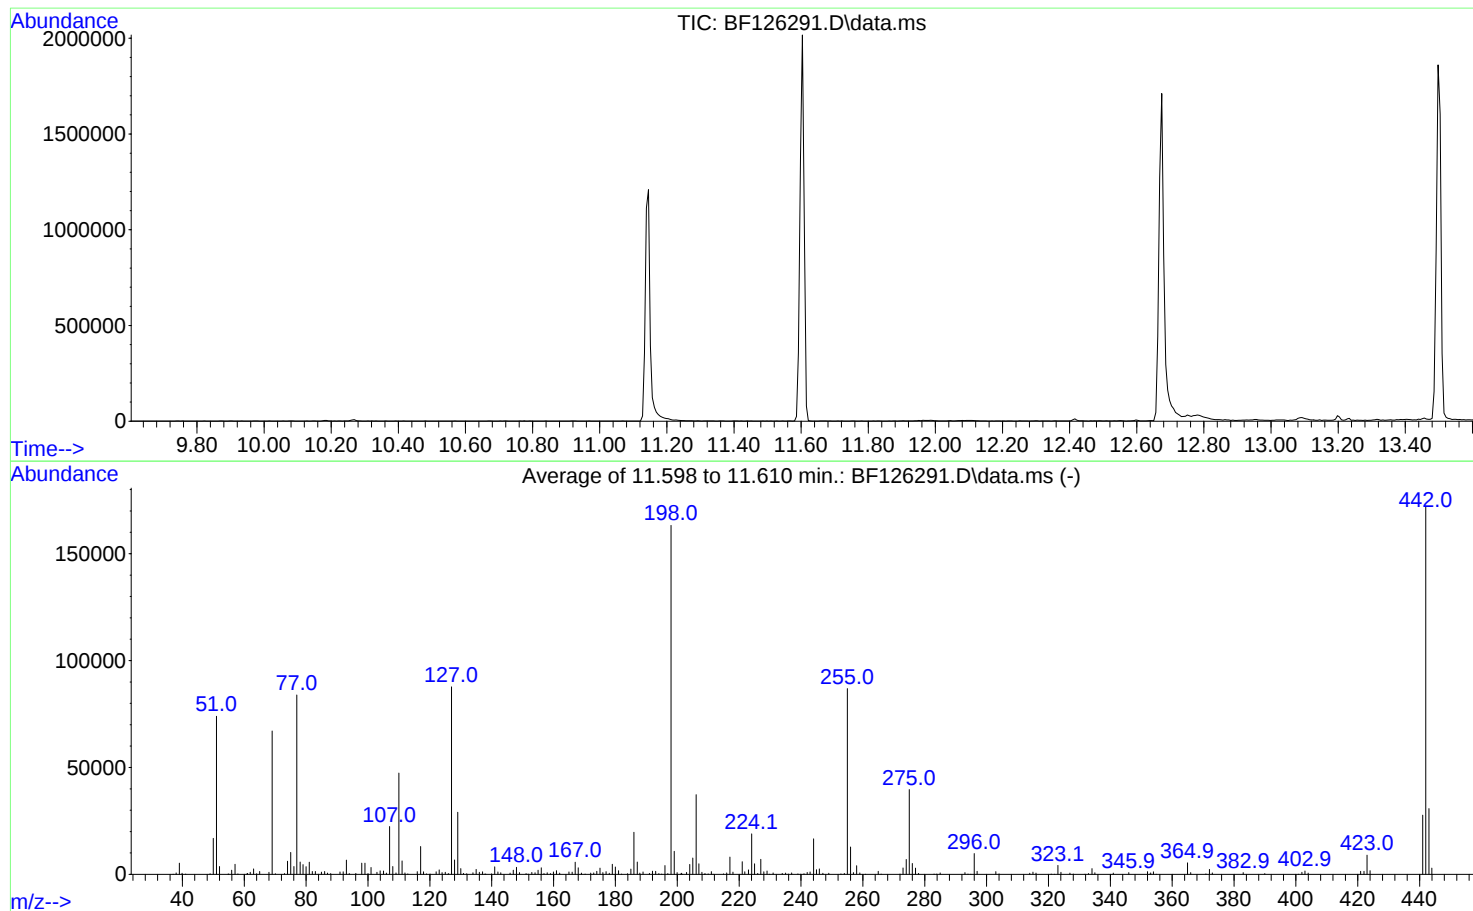

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	73955	PASS
68	69	0.00	2	1.4	958	PASS
69	198	0.00	100	41.1	67045	PASS
70	69	0.00	2	0.4	292	PASS
127	198	10	80	53.7	87696	PASS
197	198	0.00	2	0.2	386	PASS
198	198	100	100	100.0	163269	PASS
199	198	5	9	6.6	10751	PASS
275	198	10	60	24.3	39669	PASS
365	198	1	100	3.3	5421	PASS
441	198	0.01	100	17.0	27699	PASS
442	442	50	100	100.0	172085	PASS
443	442	15	24	17.9	30747	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
12/21/2021	BNA_F	<u>BF126291.D</u>
Compound Name	Response	Retention Time
DDT	329942	13.498
DDD	6273	13.198
DDE	416	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6689	336631	1.99

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126291.D
 Acq On : 21 Dec 2021 9:29
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 22 08:34:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

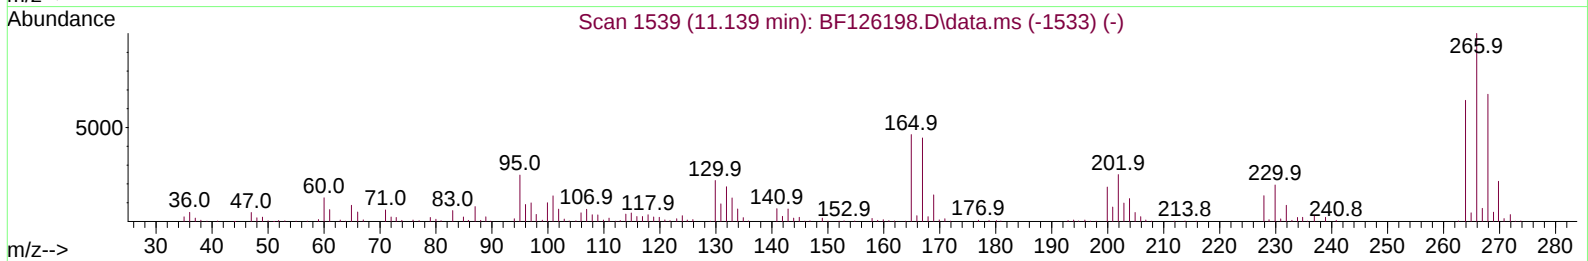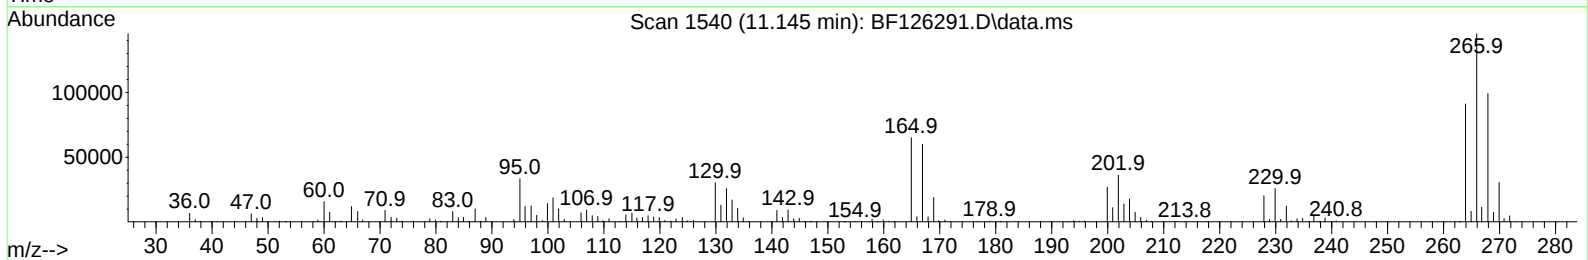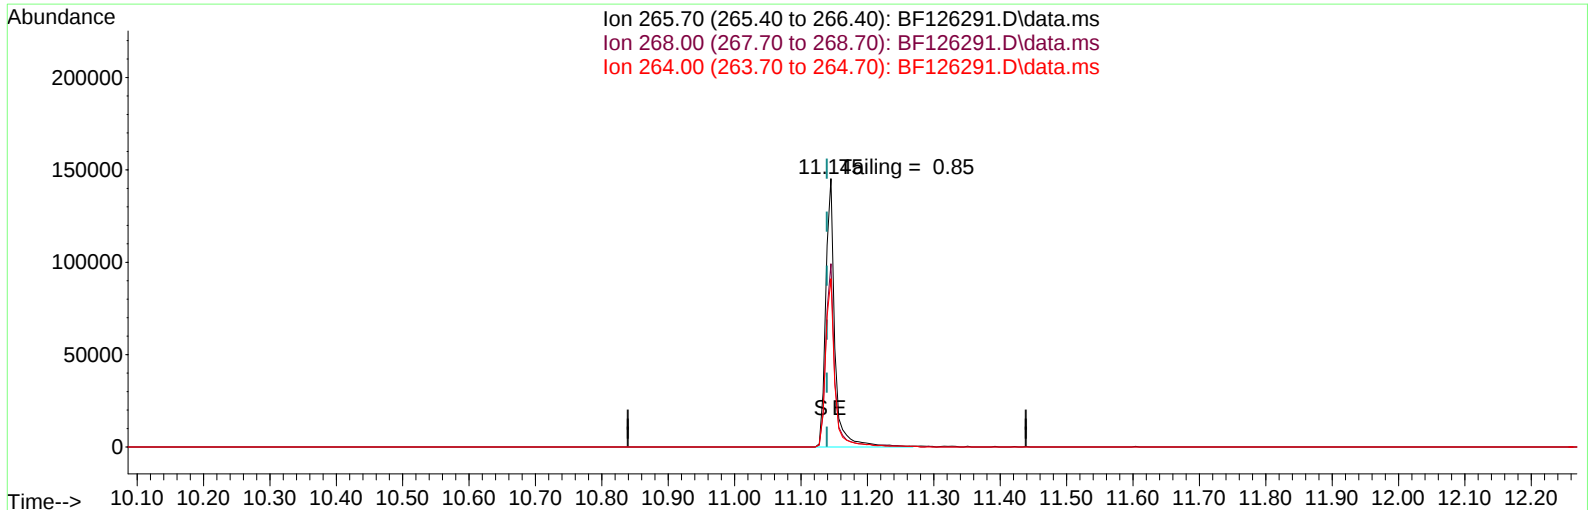

TIC: BF126291.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.006) 38244.17 ng




response 139929

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.25
264.00	69.90	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126291.D
Acq On : 21 Dec 2021 9:29
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 08:34:39 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

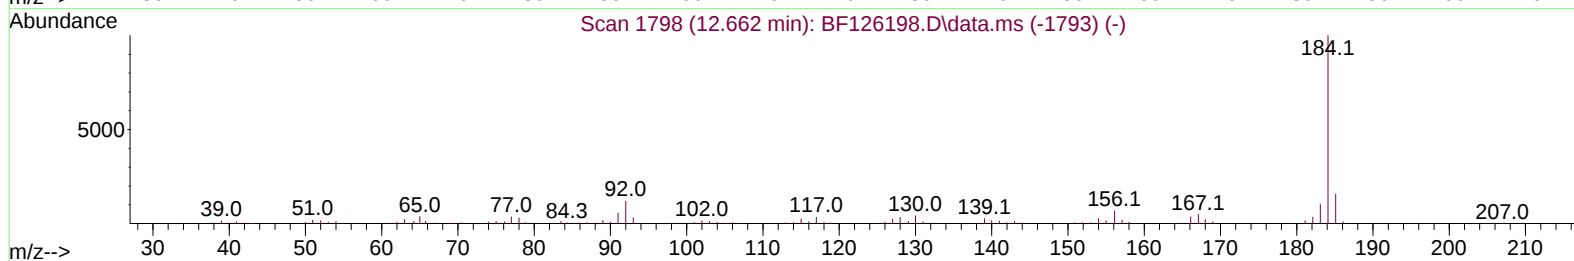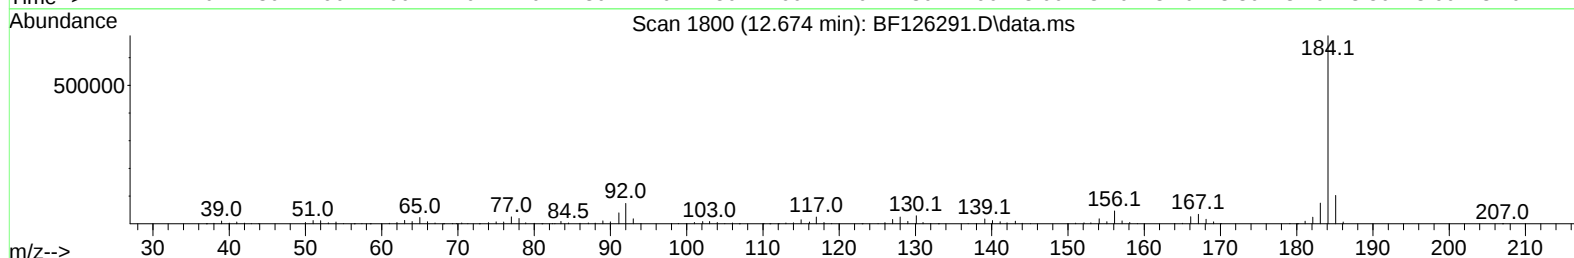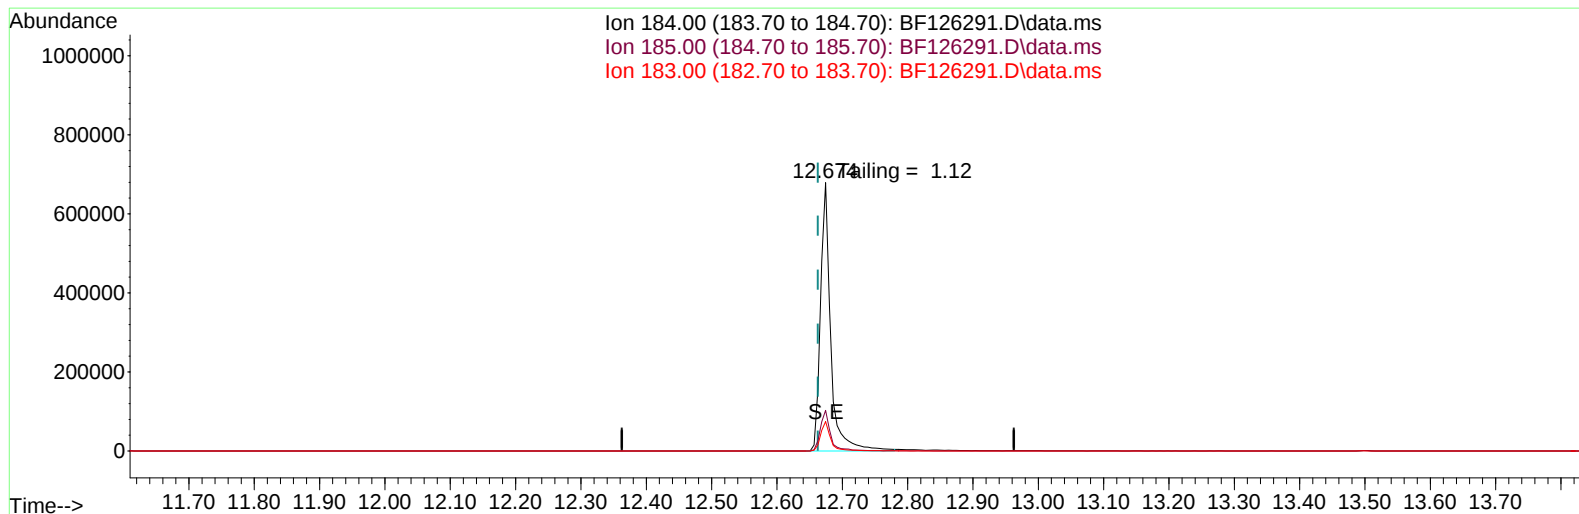

TIC: BF126291.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng

response 749986

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.15
183.00	10.10	11.01
0.00	0.00	0.00