
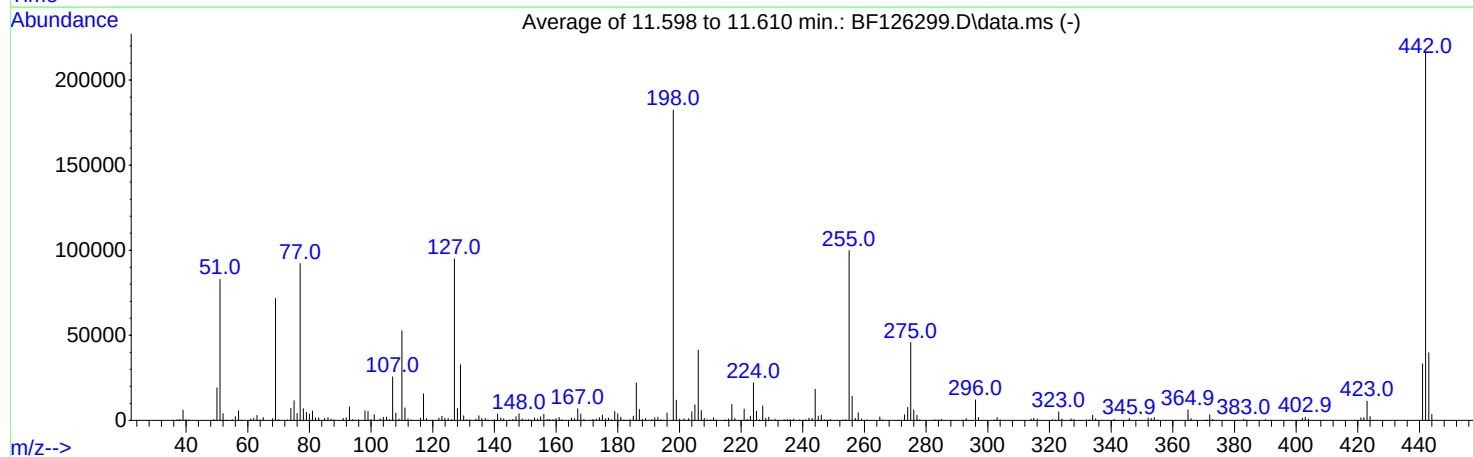


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126299.D
 Acq On : 21 Dec 2021 16:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

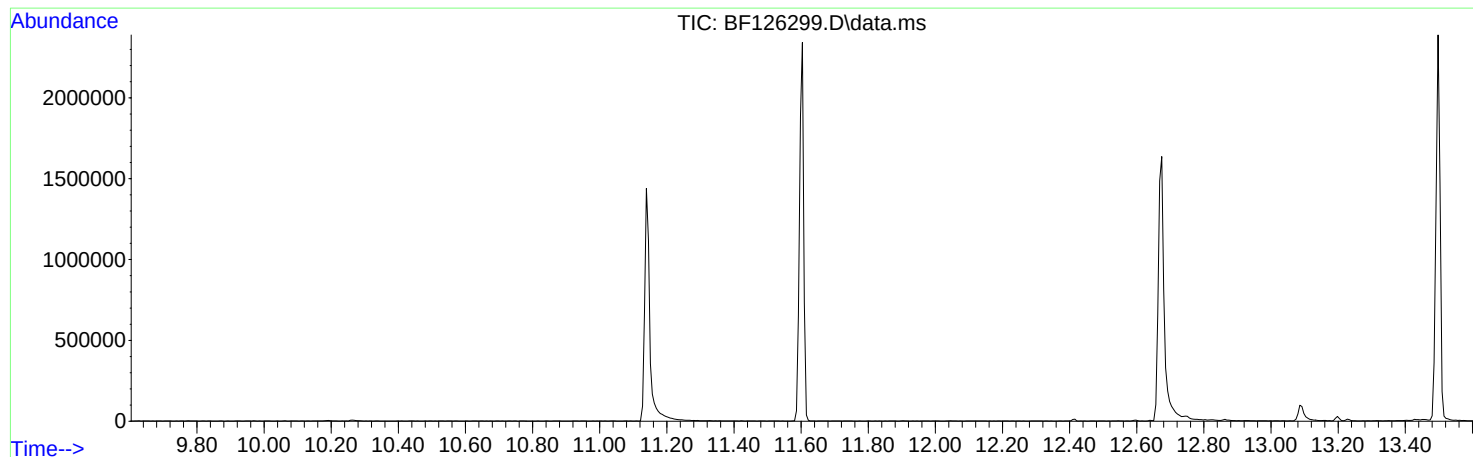

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	82856	PASS
68	69	0.00	2	1.4	1019	PASS
69	198	0.00	100	39.4	71792	PASS
70	69	0.00	2	0.3	245	PASS
127	198	10	80	52.0	94840	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	182296	PASS
199	198	5	9	6.5	11830	PASS
275	198	10	60	25.1	45672	PASS
365	198	1	100	3.4	6251	PASS
441	198	0.01	100	18.2	33192	PASS
442	442	50	100	100.0	216192	PASS
443	442	15	24	18.4	39803	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/21/2021	BNA_F	<u>BF126299.D</u>
Compound Name	Response	Retention Time
DDT	329839	13.498
DDD	8150	13.198
DDE	1940	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10090	339929	2.97

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
Data File : BF126299.D
Acq On : 21 Dec 2021 16:24
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 08:36:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

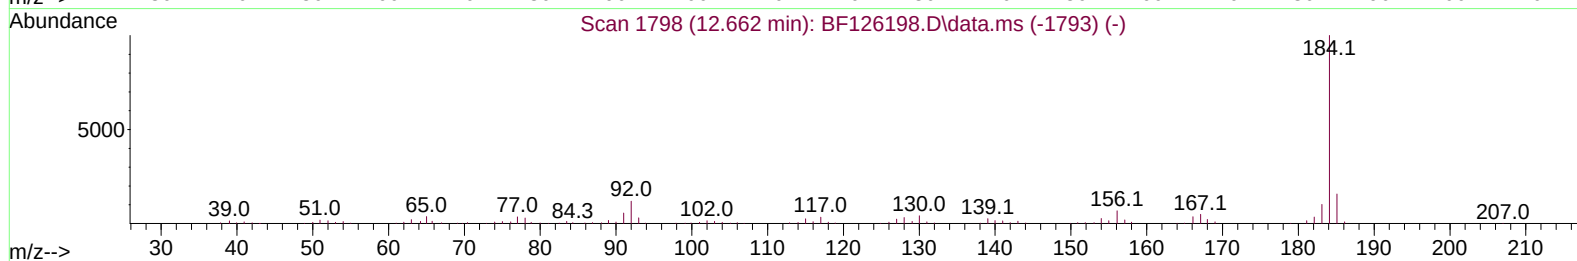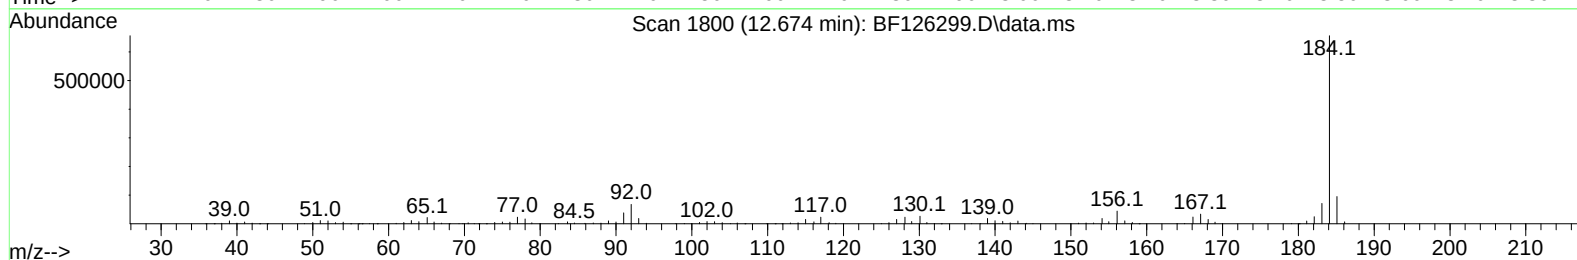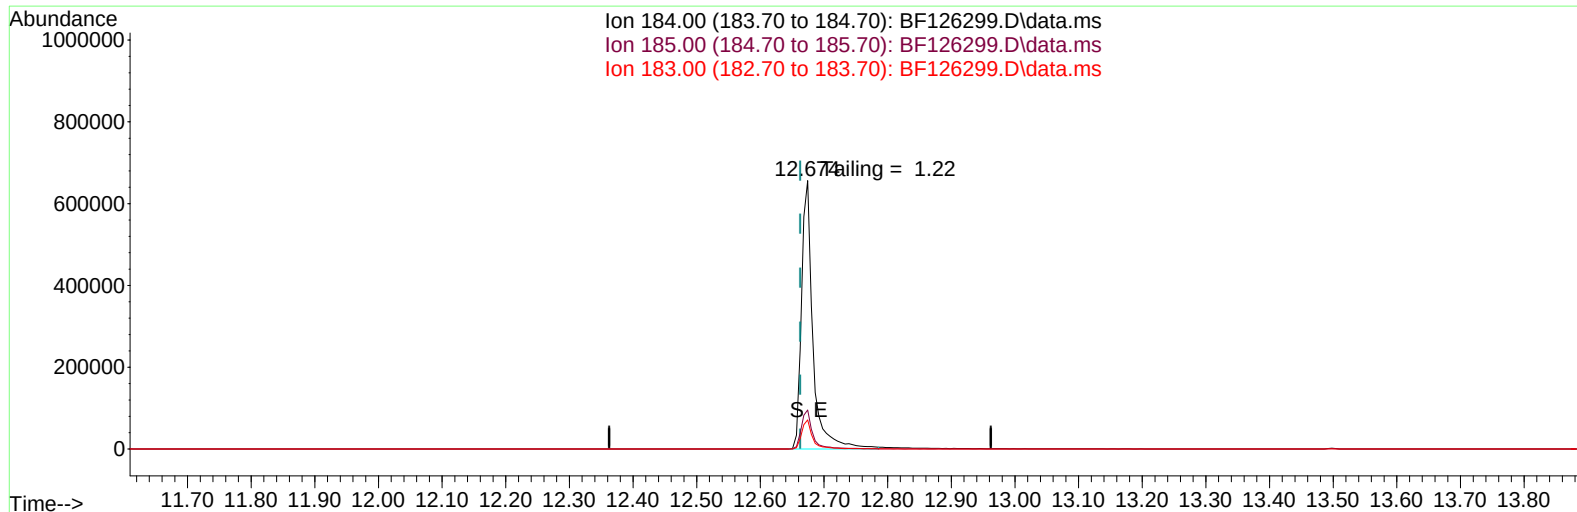

TIC: BF126299.D\data.ms

(77) Benzidine

12.674min (+ 0.012) 0.00 ng




response 837013

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.54
183.00	10.10	10.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122121\
 Data File : BF126299.D
 Acq On : 21 Dec 2021 16:24
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 22 08:36:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

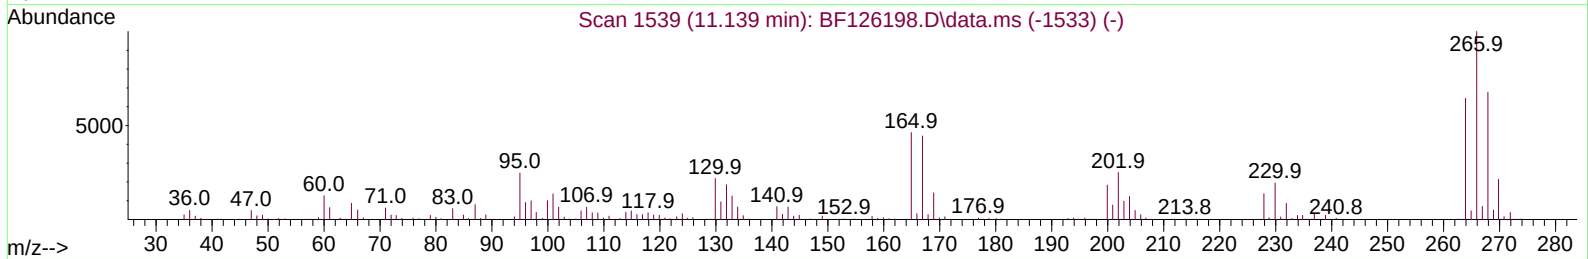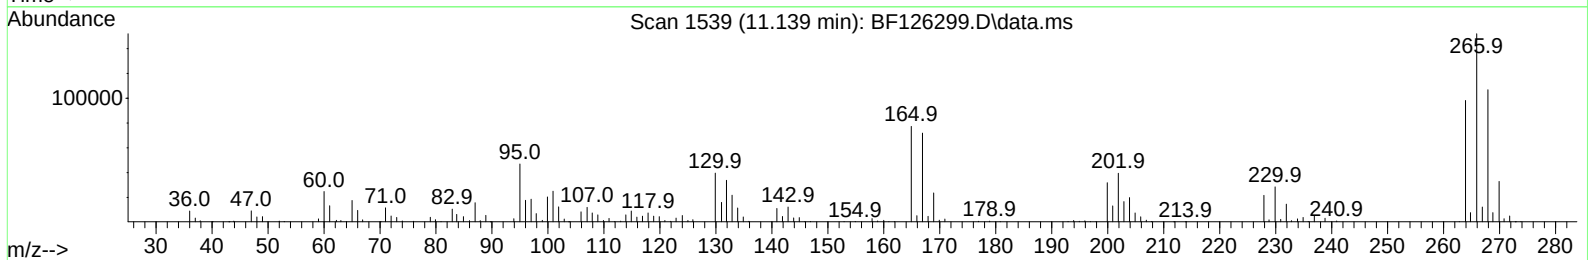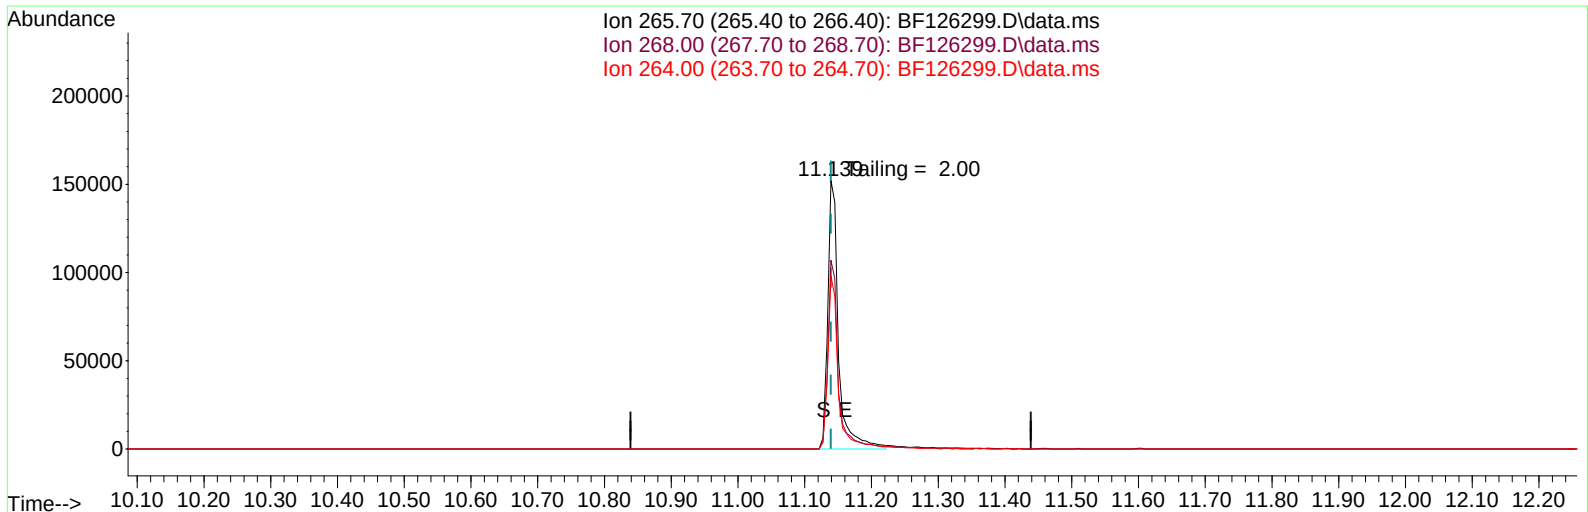

TIC: BF126299.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 38962.83 ng

response 174290

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	70.30
264.00	69.90	64.55
0.00	0.00	0.00