

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
 Data File : BF122810.D
 Acq On : 22 Dec 2020 12:20
 Operator : JU/CG
 Sample : PB133742BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB133742BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.451	567	572	575	rBV	4017338	4601846	71.78%	11.774%
2	6.457	737	743	746	rBV	3693648	4581807	71.47%	11.722%
3	6.816	800	804	820	rVB	1448983	1207657	18.84%	3.090%
4	7.386	894	901	904	rBV	2653030	3198796	49.89%	8.184%
5	8.104	1017	1023	1030	rBV	1502450	1622010	25.30%	4.150%
6	9.180	1199	1206	1209	rBV	5165176	5720460	89.23%	14.636%
7	9.857	1315	1321	1324	rBV	1999885	1854999	28.93%	4.746%
8	10.645	1449	1455	1483	rBV	3084420	3997621	62.35%	10.228%
9	11.345	1568	1574	1581	rBV	1876097	1979281	30.87%	5.064%
10	12.933	1837	1844	1848	rBV	5384834	6411250	100.00%	16.403%
11	13.986	2018	2023	2044	rBV	1808982	1985950	30.98%	5.081%
12	15.445	2265	2271	2293	rBV	1203671	1857694	28.98%	4.753%
13	16.739	2480	2491	2492	rBV5	25741	66464	1.04%	0.170%




Sum of corrected areas: 39085835

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122810.D
Acq On : 22 Dec 2020 12:20
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133742BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

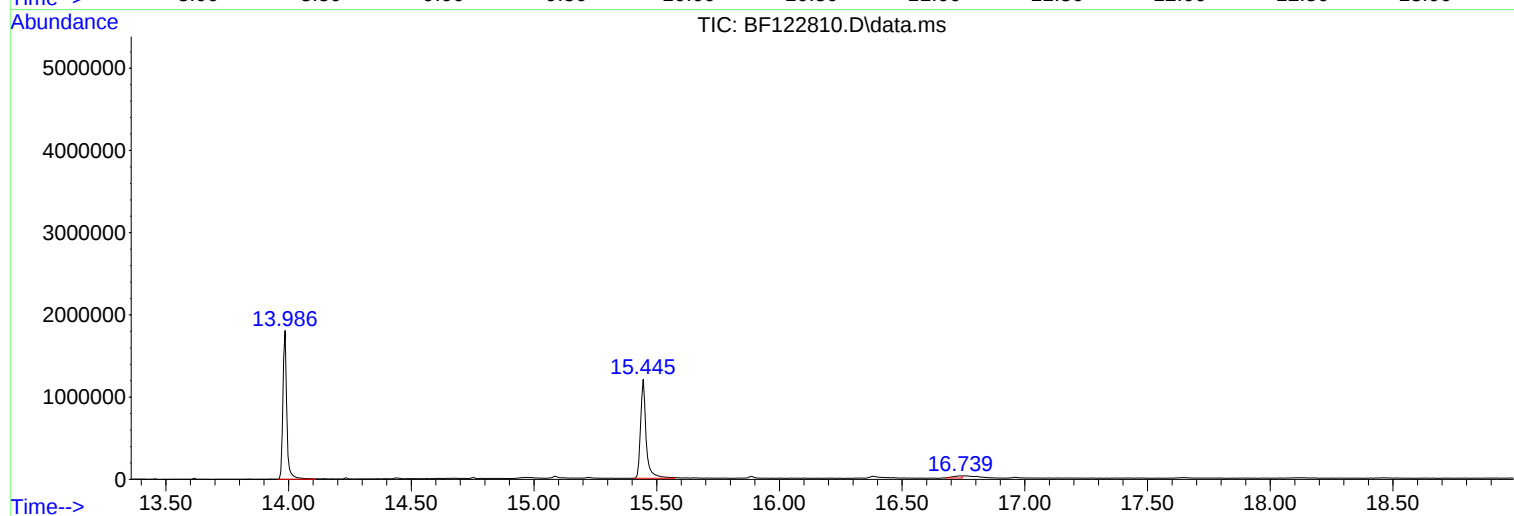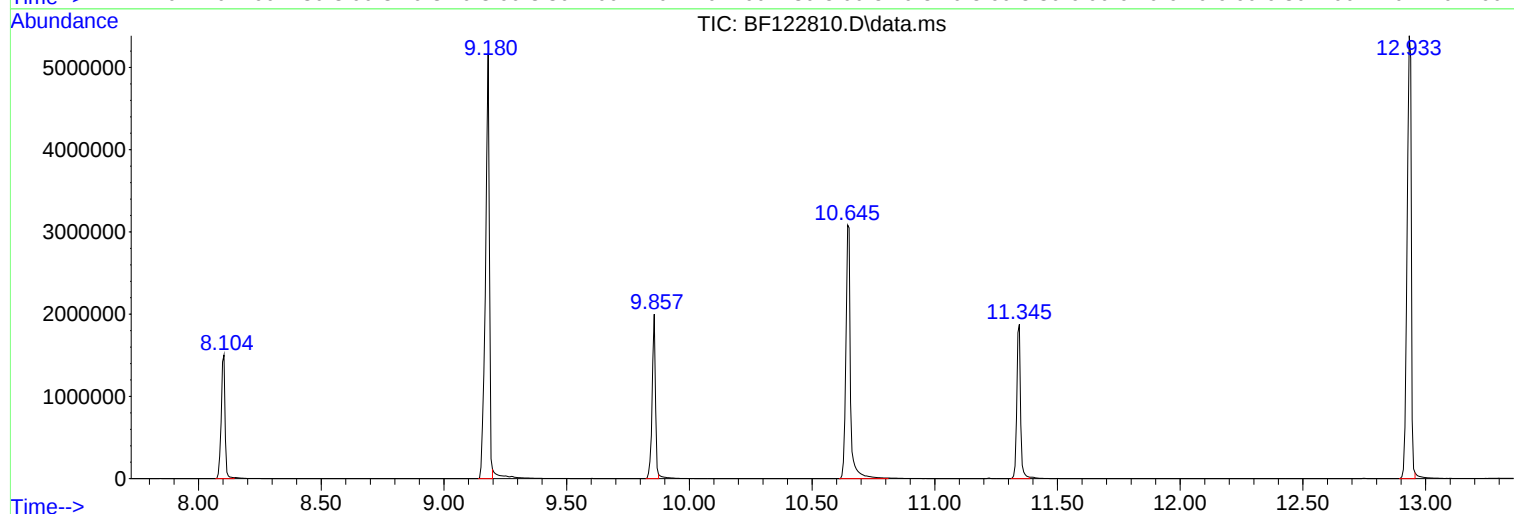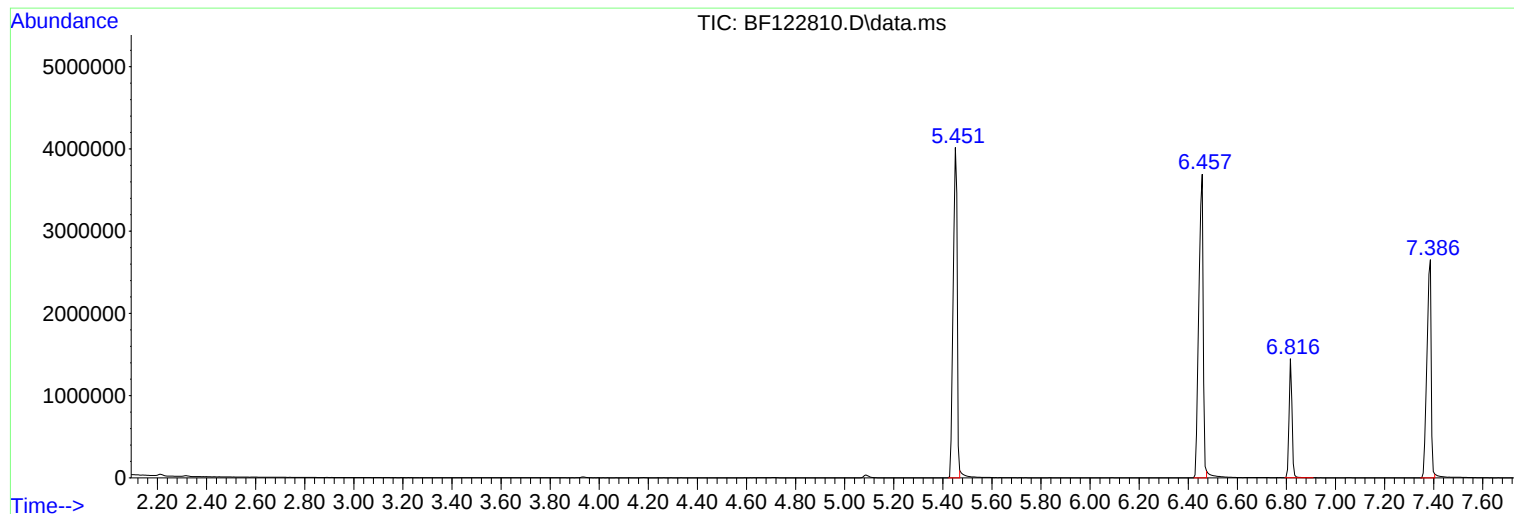

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122810.D
Acq On : 22 Dec 2020 12:20
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133742BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122810.D
Acq On : 22 Dec 2020 12:20
Operator : JU/CG
Sample : PB133742BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133742BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------