

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122819.D
Acq On : 22 Dec 2020 18:53
Operator : JU/CG
Sample : PB133764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133764BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122819.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.457	568	573	576	rBV	3736606	4023762	67.15%	11.535%
2	6.457	737	743	746	rBV	3581903	4118655	68.74%	11.807%
3	6.816	801	804	816	rVB	1139871	1009132	16.84%	2.893%
4	7.387	895	901	904	rBV	2481800	2791303	46.58%	8.002%
5	8.104	1018	1023	1042	rBV	1367893	1355531	22.62%	3.886%
6	9.181	1200	1206	1209	rBV	4674011	5189466	86.61%	14.877%
7	9.857	1315	1321	1339	rBV	1609668	1610920	26.88%	4.618%
8	10.651	1450	1456	1490	rBV	3223474	3803648	63.48%	10.904%
9	11.345	1568	1574	1582	rBV	1728960	1661079	27.72%	4.762%
10	12.939	1837	1845	1848	rBV	5397433	5991976	100.00%	17.177%
11	13.986	2019	2023	2036	rBV	1601855	1713333	28.59%	4.912%
12	15.451	2267	2272	2286	rBV2	1064930	1614395	26.94%	4.628%




Sum of corrected areas: 34883200

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122819.D
Acq On : 22 Dec 2020 18:53
Operator : JU/CG
Sample : PB133764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

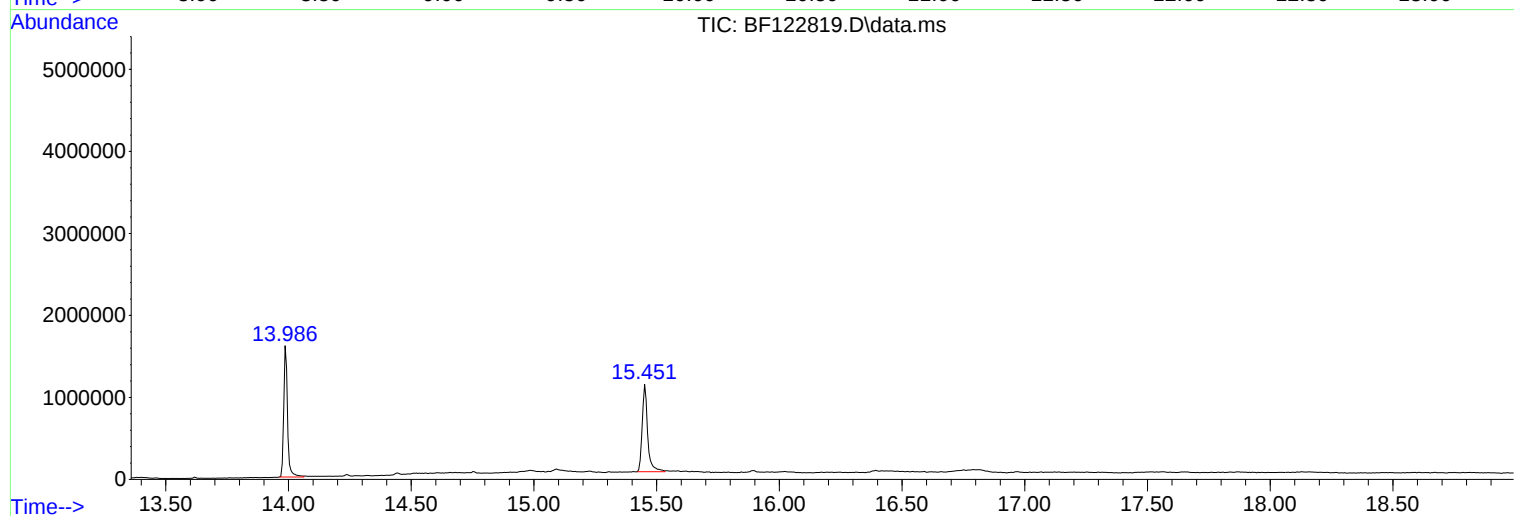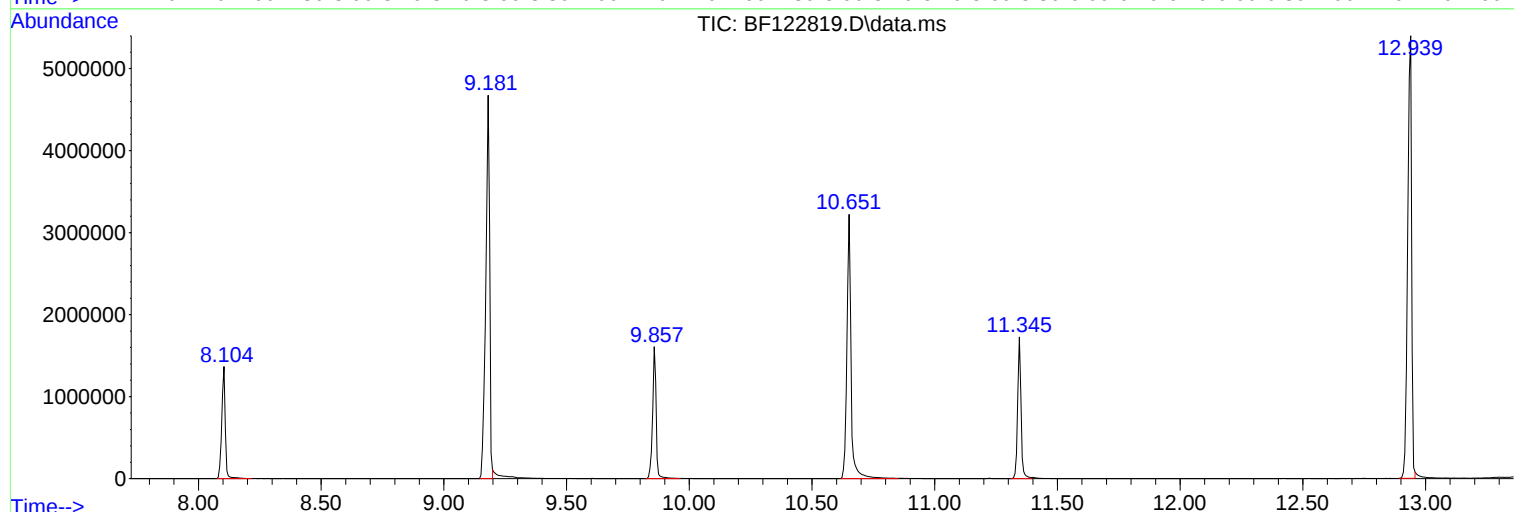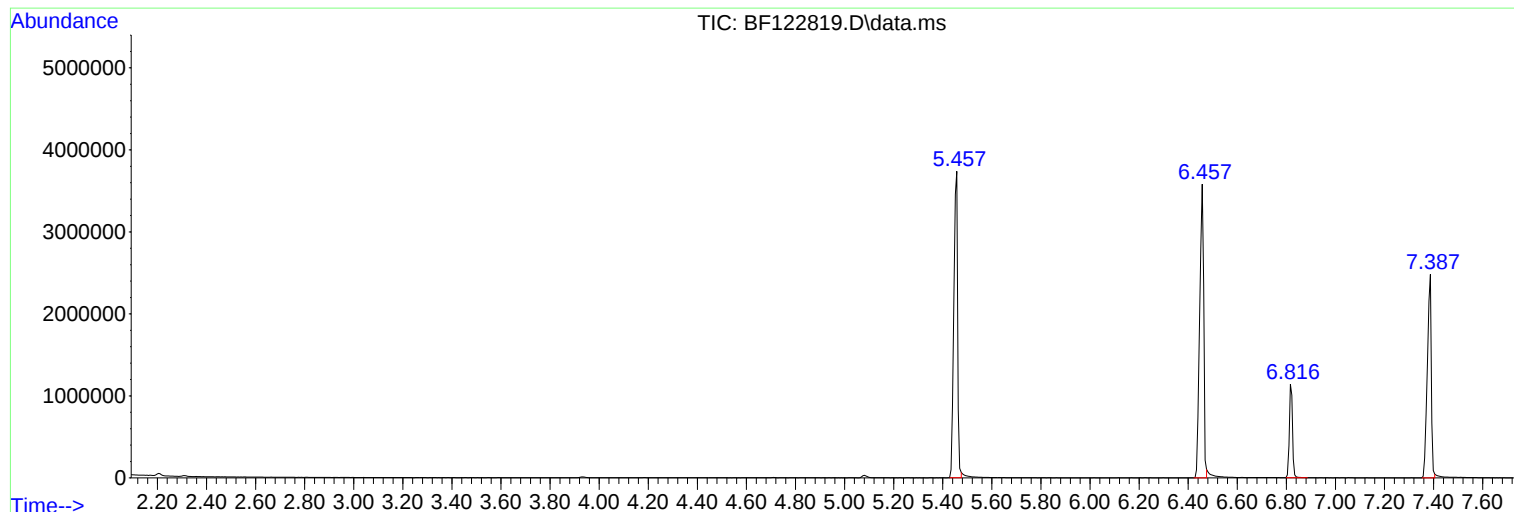

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122819.D
Acq On : 22 Dec 2020 18:53
Operator : JU/CG
Sample : PB133764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
Data File : BF122819.D
Acq On : 22 Dec 2020 18:53
Operator : JU/CG
Sample : PB133764BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB133764BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------