


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122220\
 Data File : BF122817.D
 Acq On : 22 Dec 2020 17:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

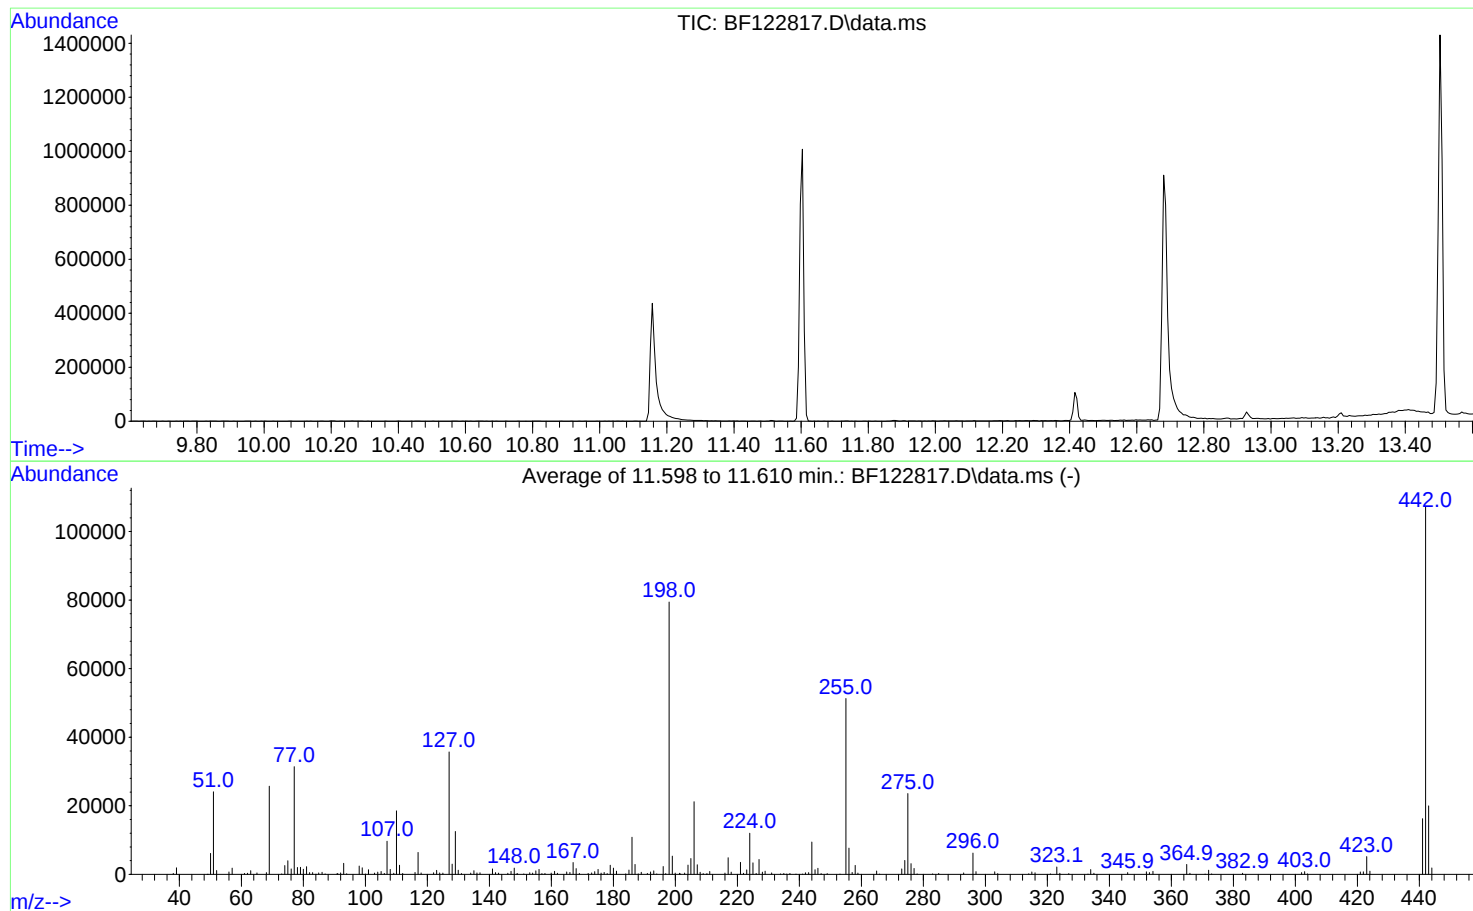

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	24065	PASS
68	69	0.00	2	1.9	493	PASS
69	198	0.00	100	32.4	25712	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	35688	PASS
197	198	0.00	2	0.3	241	PASS
198	198	100	100	100.0	79419	PASS
199	198	5	9	6.7	5300	PASS
275	198	10	60	29.7	23590	PASS
365	198	1	100	3.6	2872	PASS
441	198	0.01	100	20.4	16238	PASS
442	442	100	100	100.0	107291	PASS
443	442	15	24	18.6	19970	PASS