

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
 Data File : BF126326.D
 Acq On : 22 Dec 2021 13:24
 Operator : JU/CG
 Sample : PB141606BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141606BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126326.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.046	499	503	511	rVB	35438	46235	1.17%	0.186%
2	5.434	564	569	572	rBV	3539877	3764243	95.10%	15.109%
3	6.445	735	741	744	rBV	3362587	3711256	93.76%	14.896%
4	6.816	800	804	807	rBV	1049922	824476	20.83%	3.309%
5	7.375	894	899	911	rBV	2386260	2606471	65.85%	10.462%
6	8.098	1017	1022	1038	rBV	1207364	1165037	29.43%	4.676%
7	9.175	1200	1205	1226	rBV	3591500	3958221	100.00%	15.887%
8	9.851	1316	1320	1336	rBV	1151386	1190936	30.09%	4.780%
9	10.639	1450	1454	1480	rBV	2057229	2177030	55.00%	8.738%
10	11.339	1569	1573	1580	rBV	1029740	1078449	27.25%	4.329%
11	12.927	1838	1843	1866	rBV	2806494	3025411	76.43%	12.143%
12	13.974	2017	2021	2032	rBV	534873	629040	15.89%	2.525%
13	14.069	2034	2037	2047	rVB	70086	102181	2.58%	0.410%
14	15.421	2262	2267	2287	rBV	346709	635107	16.05%	2.549%




Sum of corrected areas: 24914093

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126326.D
Acq On : 22 Dec 2021 13:24
Operator : JU/CG
Sample : PB141606BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141606BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

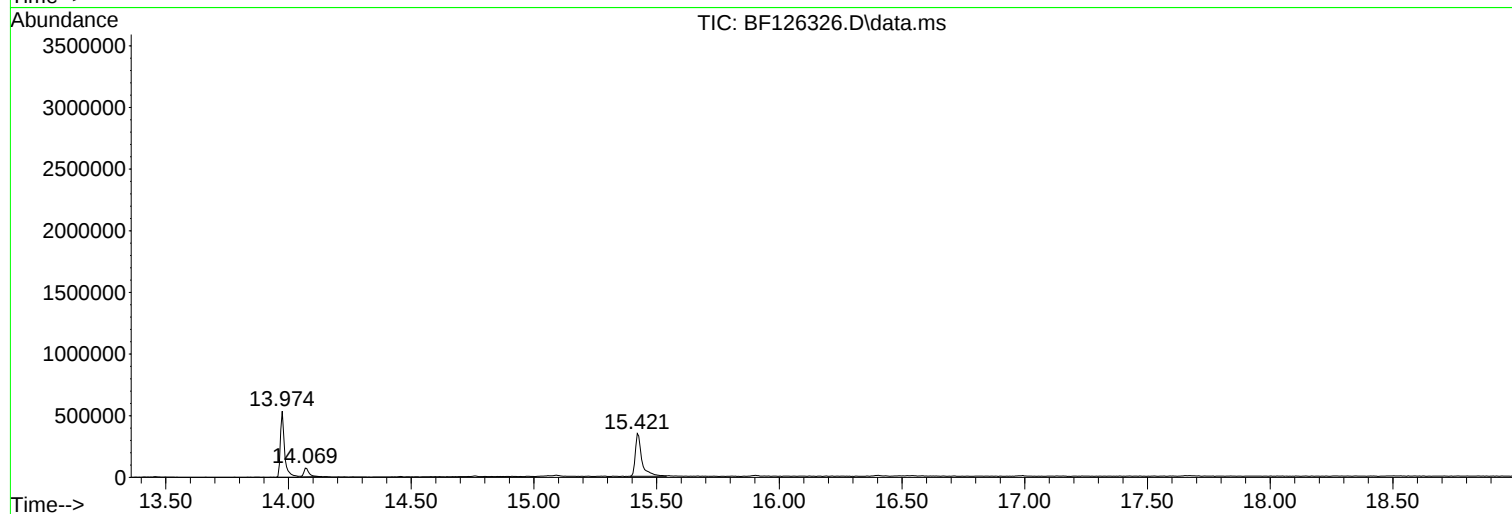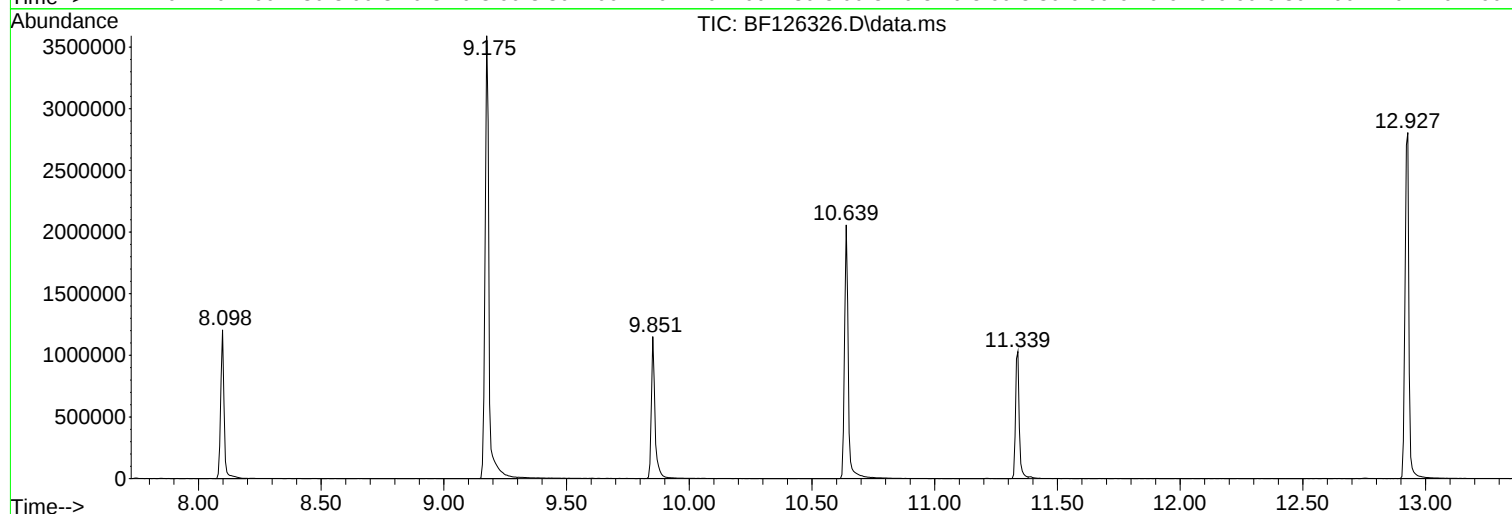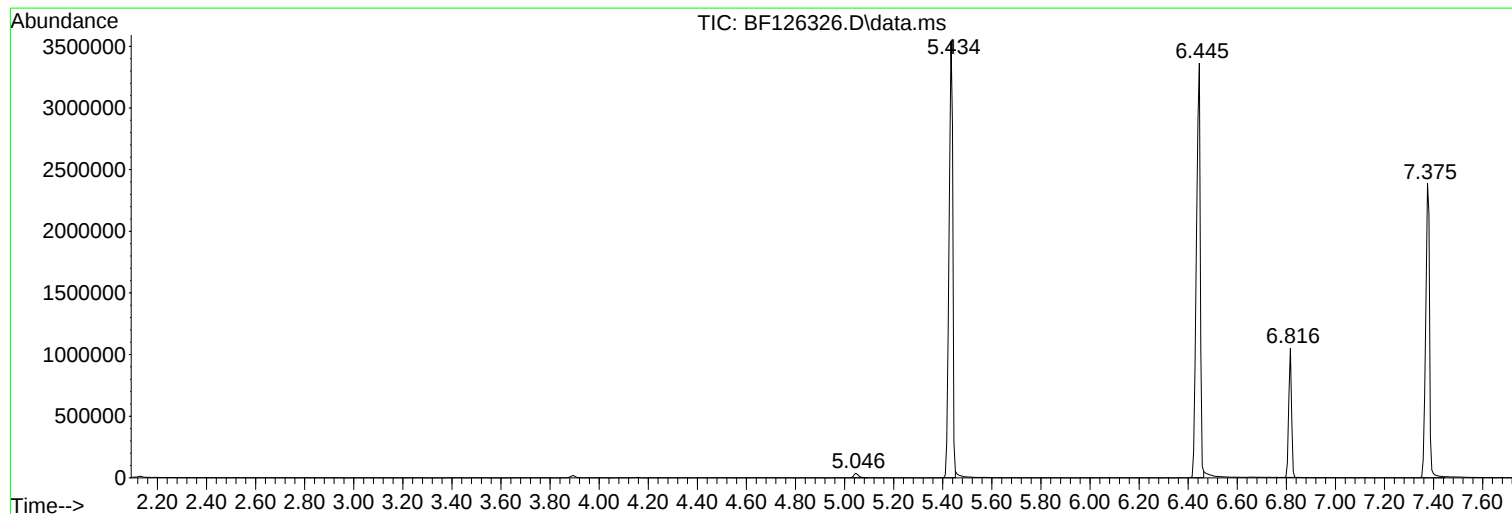

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126326.D
Acq On : 22 Dec 2021 13:24
Operator : JU/CG
Sample : PB141606BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141606BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.069	3.25 ng	102181	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...	293	C15H19NO3S	1000483-83-4	52
3			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	49
4			2-Phenyl-6-(trifluoromethyl)-1H...	277	C15H10F3NO	1000387-59-3	43
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	43

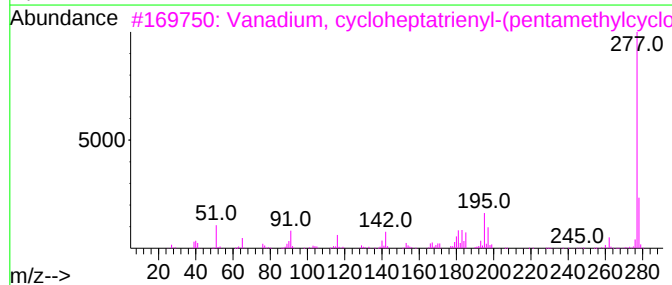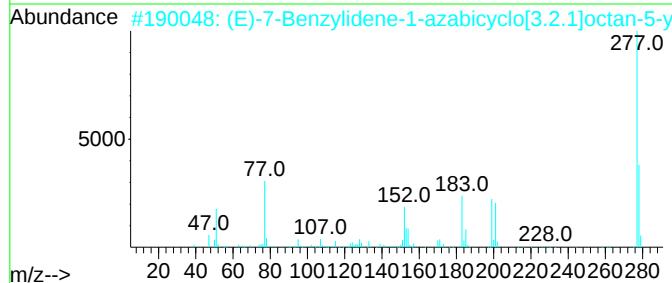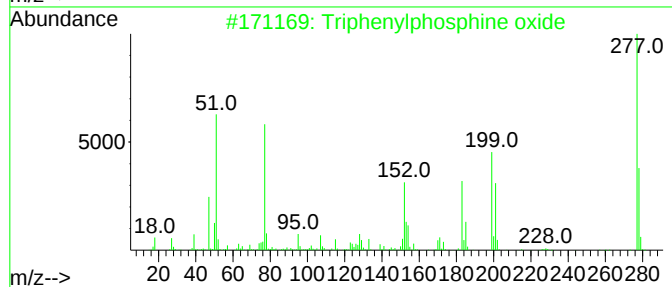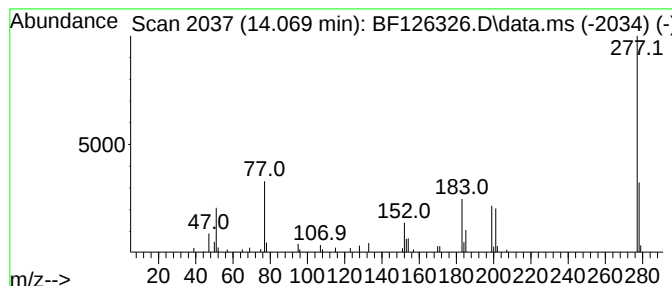

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126326.D
Acq On : 22 Dec 2021 13:24
Operator : JU/CG
Sample : PB141606BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141606BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.069	3.3	ng	102181	5	13.974	629040	20.0