

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
 Data File : BF126327.D
 Acq On : 22 Dec 2021 13:56
 Operator : JU/CG
 Sample : PB141608BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141608BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126327.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.045	496	503	513	rBV	38170	55334	1.38%	0.218%
2	5.434	564	569	573	rBV	3516719	3920791	97.59%	15.413%
3	6.445	735	741	744	rBV	3461631	3820881	95.10%	15.020%
4	6.816	800	804	807	rBV	1099104	865533	21.54%	3.402%
5	7.375	894	899	903	rBV	2348227	2652903	66.03%	10.429%
6	8.098	1017	1022	1039	rBV	1244371	1202784	29.94%	4.728%
7	9.175	1200	1205	1225	rBV	3659864	4017796	100.00%	15.794%
8	9.851	1316	1320	1334	rBV	1191315	1217254	30.30%	4.785%
9	10.639	1450	1454	1477	rBV	2071146	2189164	54.49%	8.606%
10	11.339	1569	1573	1590	rBV	1027121	1116729	27.79%	4.390%
11	12.927	1838	1843	1858	rBV	2866141	2973570	74.01%	11.689%
12	13.974	2017	2021	2033	rBV	556003	648232	16.13%	2.548%
13	14.068	2033	2037	2047	rVB	65242	96989	2.41%	0.381%
14	15.427	2262	2268	2283	rBV	374192	660788	16.45%	2.598%




Sum of corrected areas: 25438748

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126327.D
Acq On : 22 Dec 2021 13:56
Operator : JU/CG
Sample : PB141608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141608BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

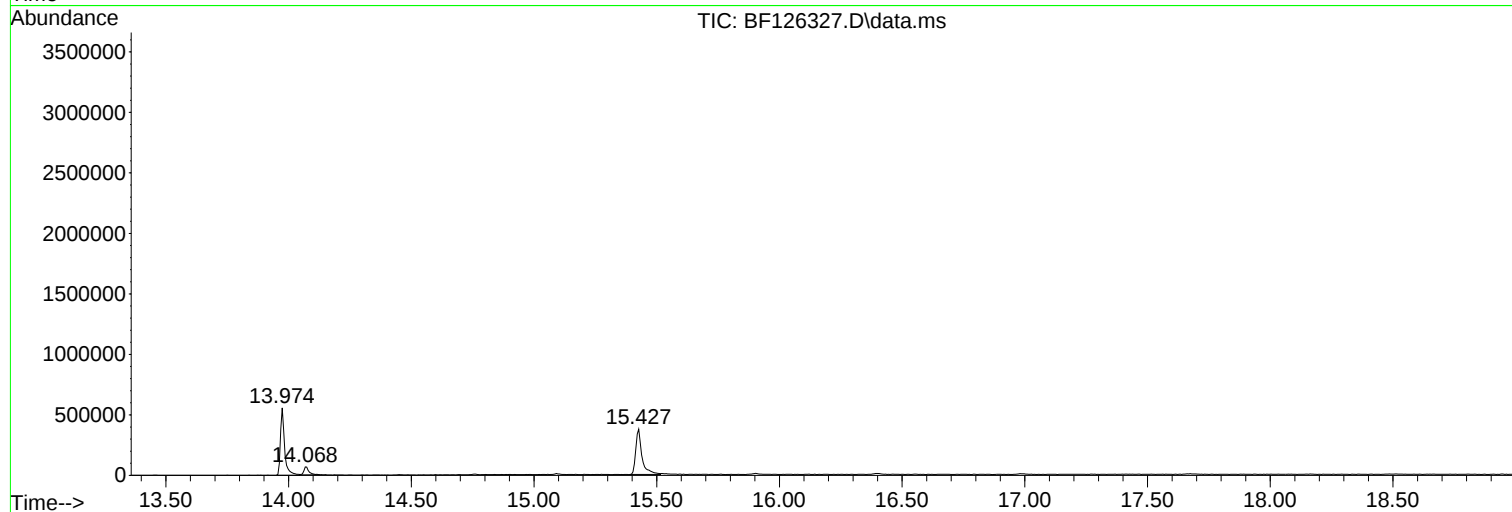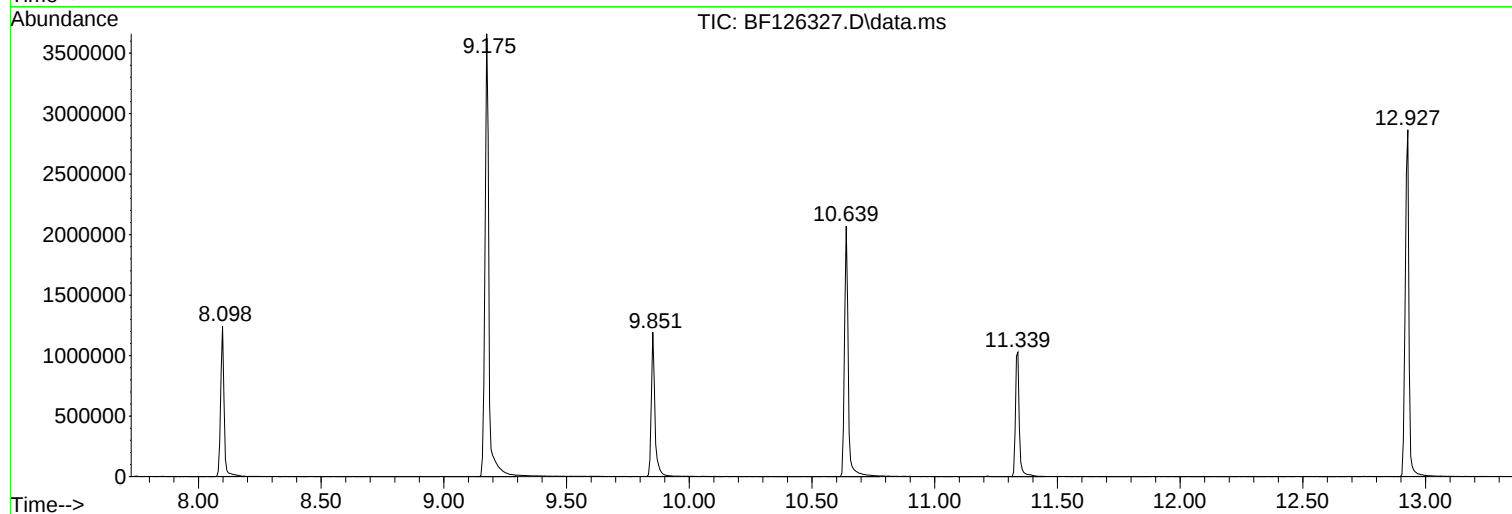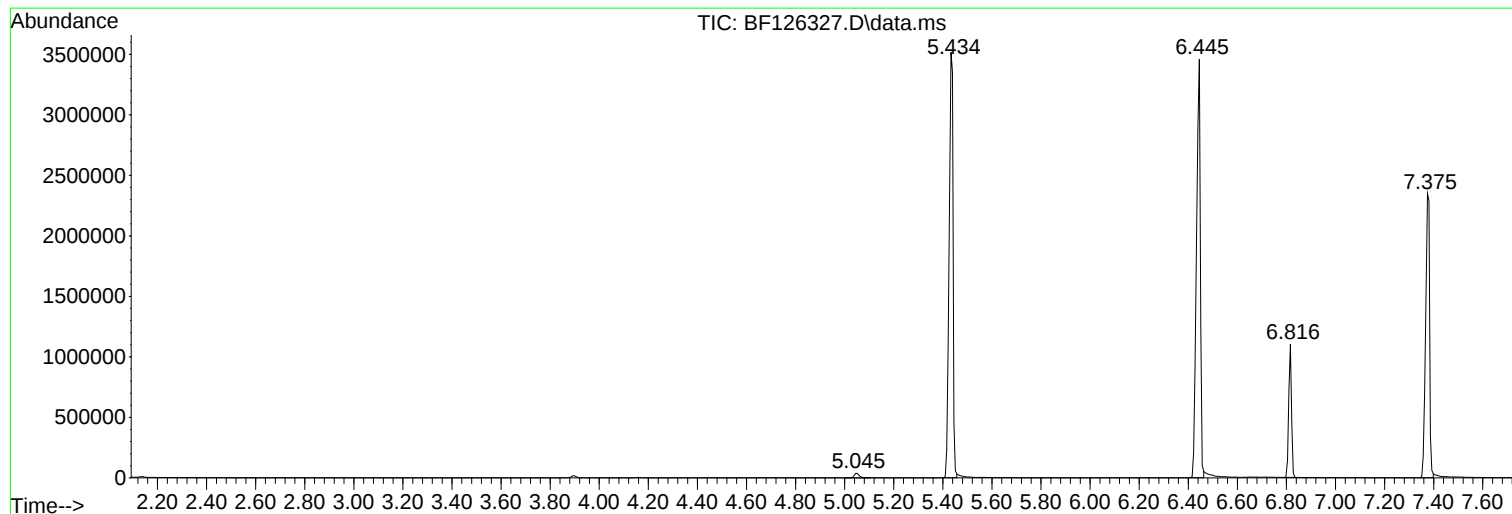

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126327.D
Acq On : 22 Dec 2021 13:56
Operator : JU/CG
Sample : PB141608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141608BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.068	2.99 ng	96989	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	94
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	90
3			Formaldehyde, (triphenylphosphor...]	304	C19H17N2P	015990-54-2	64
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	43
5			Vanadium, cycloheptatrienyl-(pen...	277	C17H22V	1000155-20-5	38

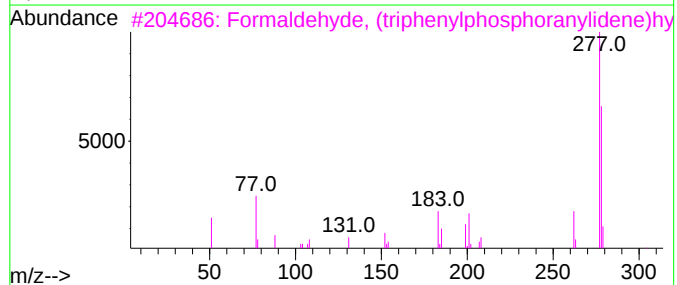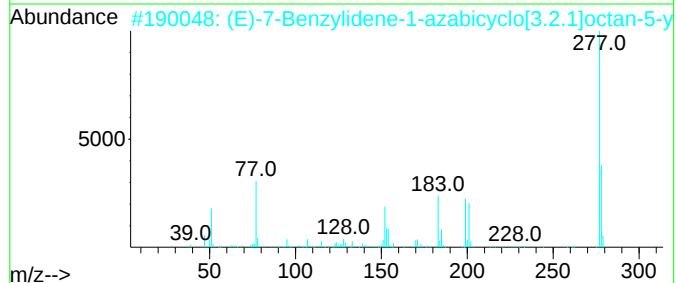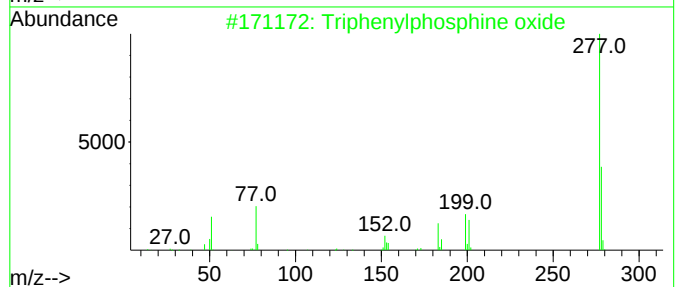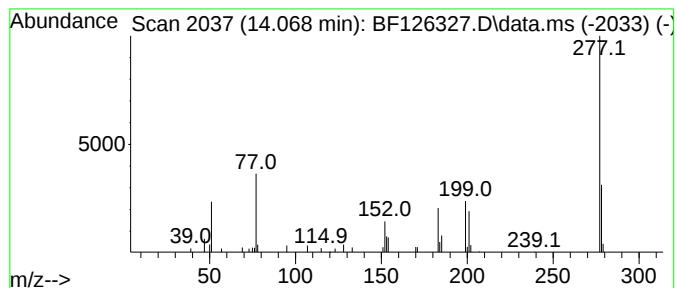

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126327.D
Acq On : 22 Dec 2021 13:56
Operator : JU/CG
Sample : PB141608BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141608BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.068	3.0	ng	96989	5	13.974	648232	20.0