
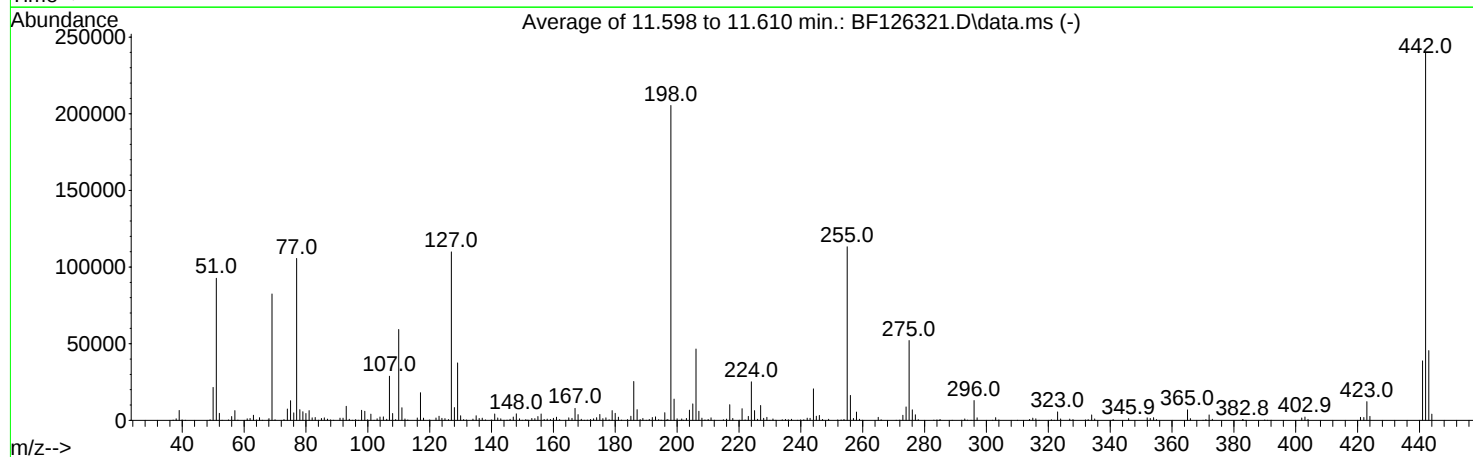


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
 Data File : BF126321.D
 Acq On : 22 Dec 2021 10:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

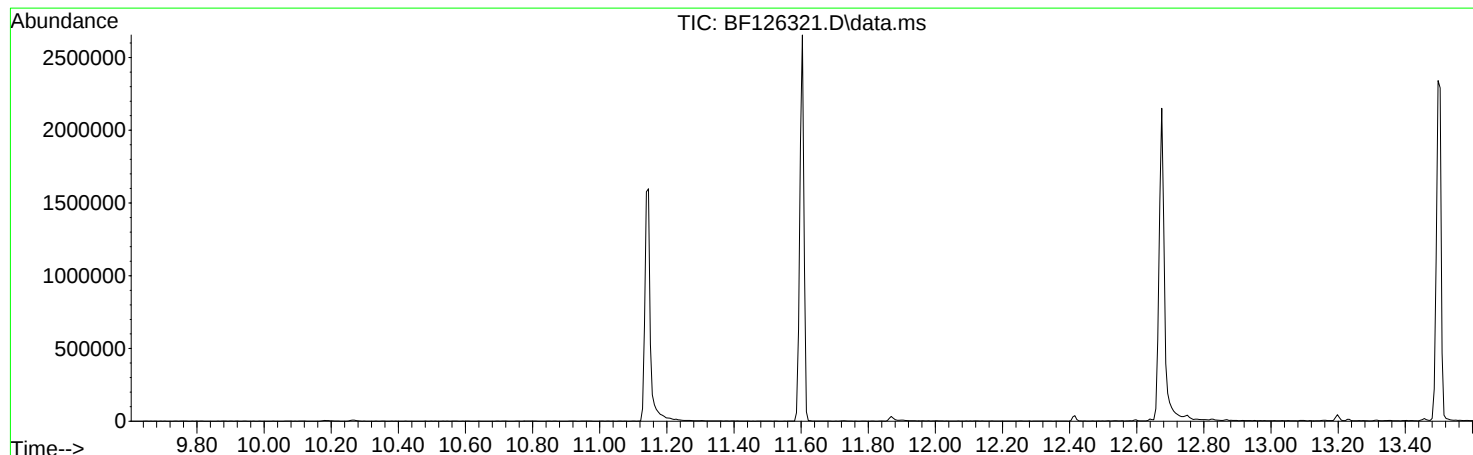




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	92707	PASS
68	69	0.00	2	1.4	1149	PASS
69	198	0.00	100	40.2	82445	PASS
70	69	0.00	2	0.5	419	PASS
127	198	10	80	53.5	109909	PASS
197	198	0.00	2	0.3	637	PASS
198	198	100	100	100.0	205336	PASS
199	198	5	9	6.8	13870	PASS
275	198	10	60	25.4	52123	PASS
365	198	1	100	3.4	6920	PASS
441	198	0.01	100	18.9	38797	PASS
442	442	50	100	100.0	239936	PASS
443	442	15	24	19.0	45544	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
 Data File : BF126321.D
 Acq On : 22 Dec 2021 10:39
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 22 13:07:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

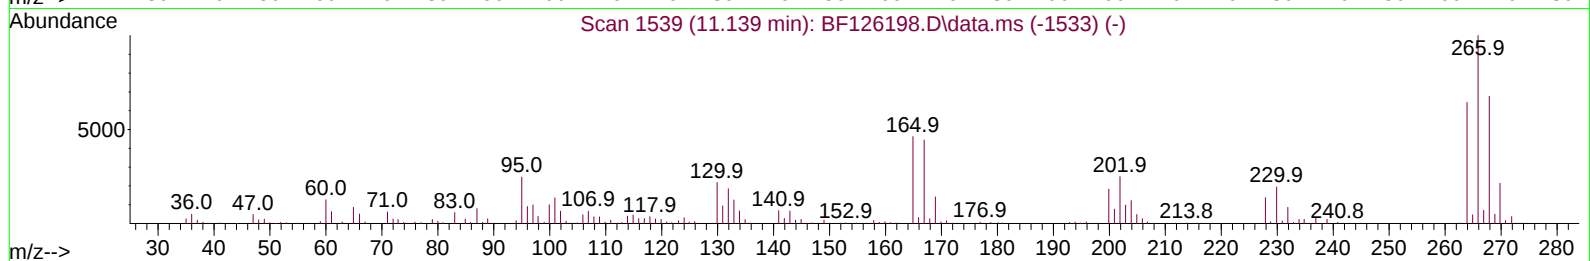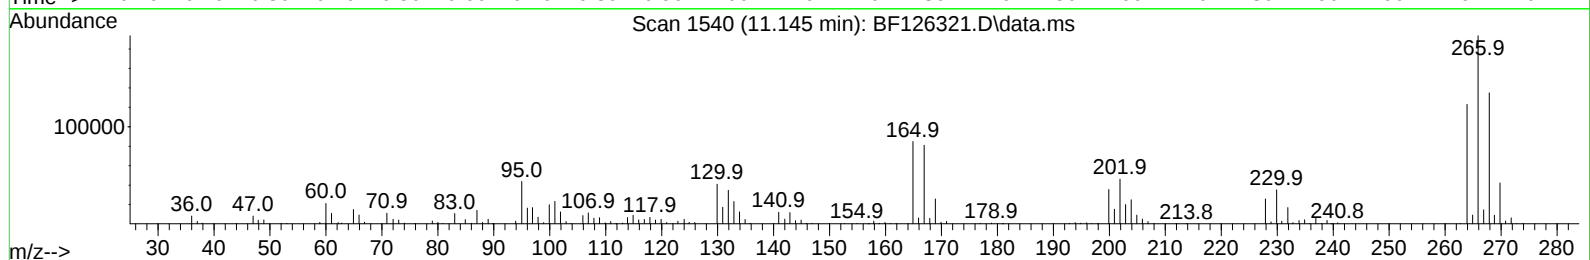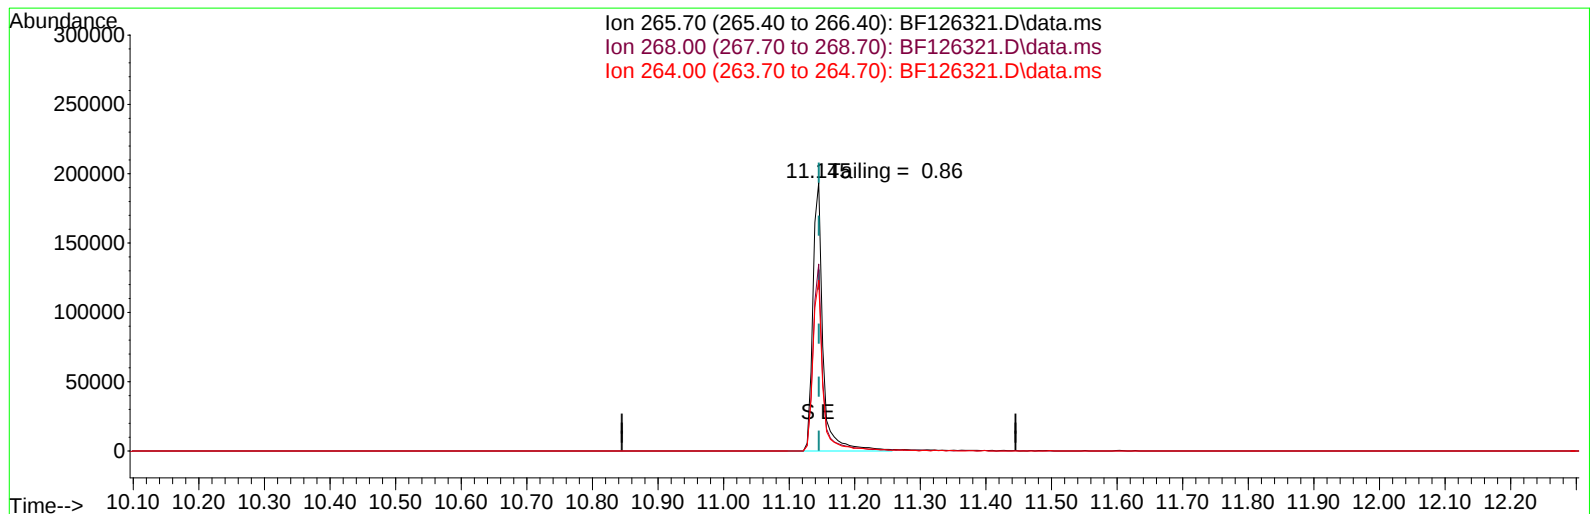

TIC: BF126321.D\data.ms

(70) Pentachlorophenol (C)

11.145min (+ 0.000) 66286.18 ng




response 209981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	69.65
264.00	69.90	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122221\
Data File : BF126321.D
Acq On : 22 Dec 2021 10:39
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 22 13:07:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 13:00:11 2021
Response via : Initial Calibration

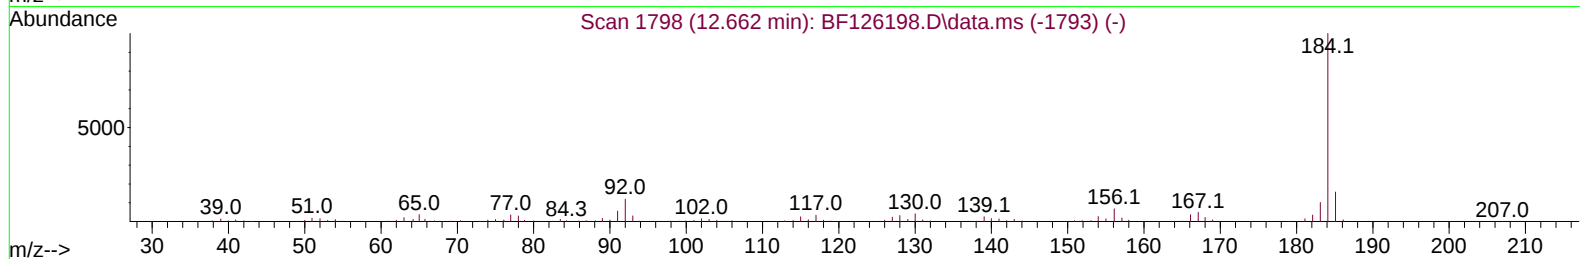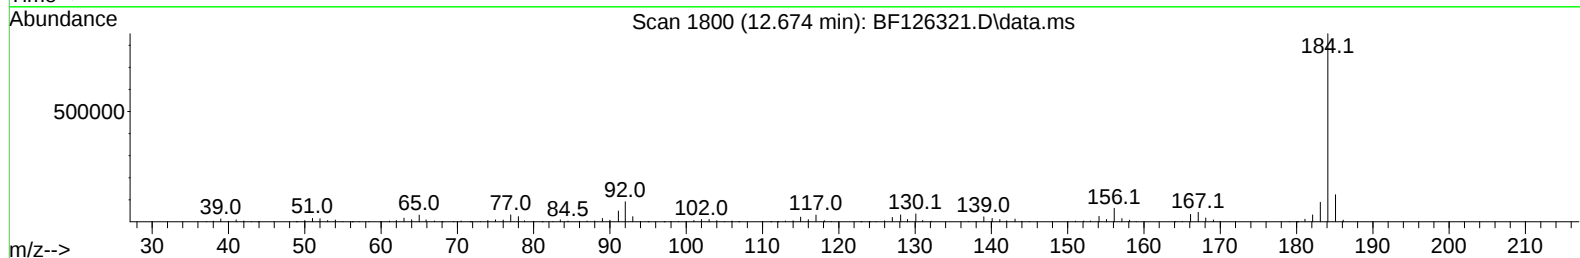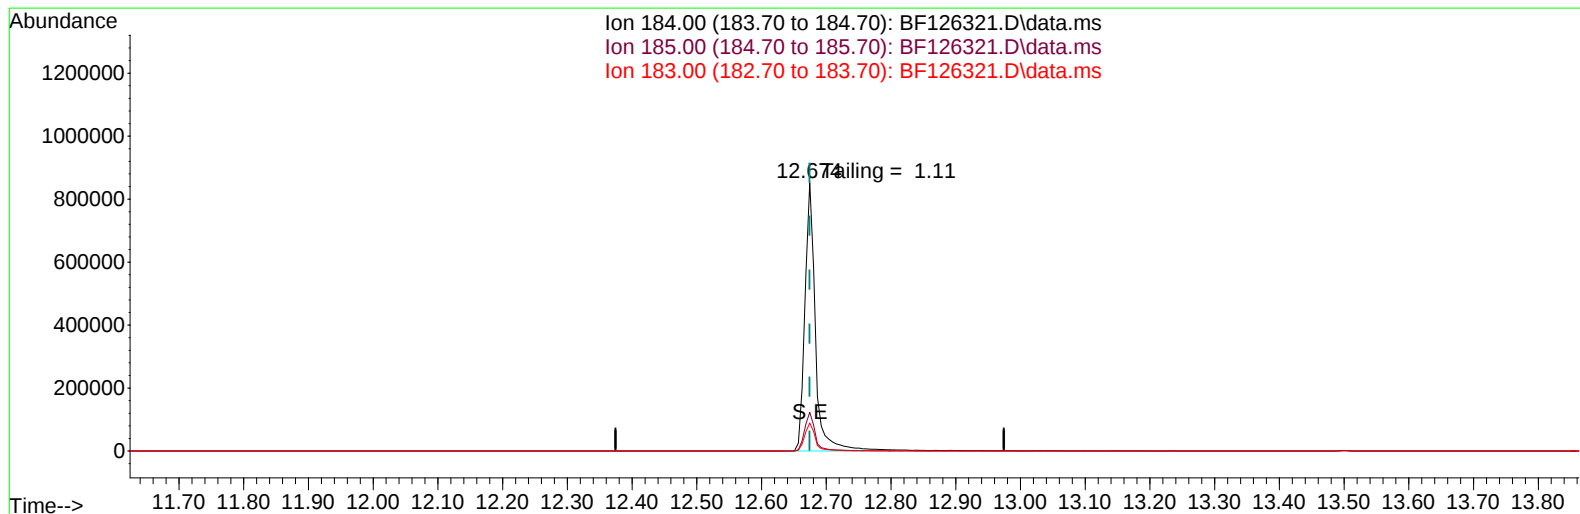

TIC: BF126321.D\data.ms

(77) Benzidine

12.674min (+ 0.000) 0.00 ng

response 973874

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.45
183.00	10.10	10.46
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/22/2021	BNA_F	<u>BF126321.D</u>
Compound Name	Response	Retention Time
DDT	436472	13.5
DDD	8175	13.19
DDE	1100	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9275	445747	2.08

Instrument :
BNA_F
ClientSampleId :
DFTPP