
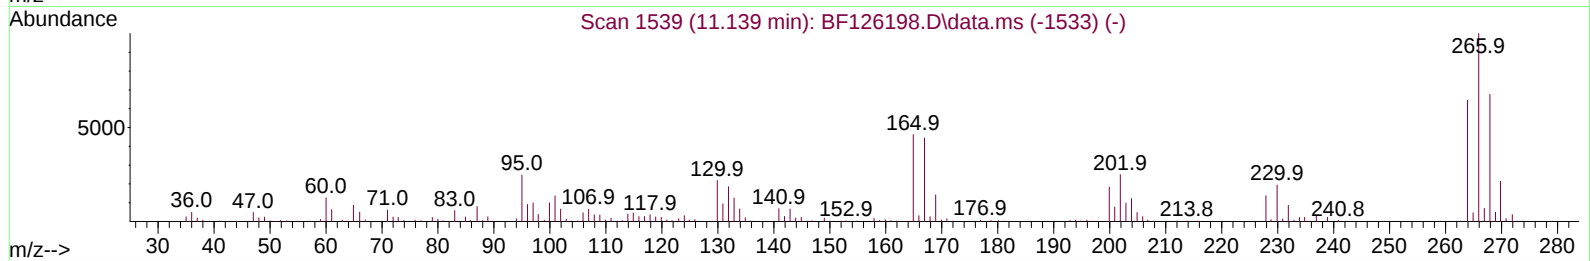
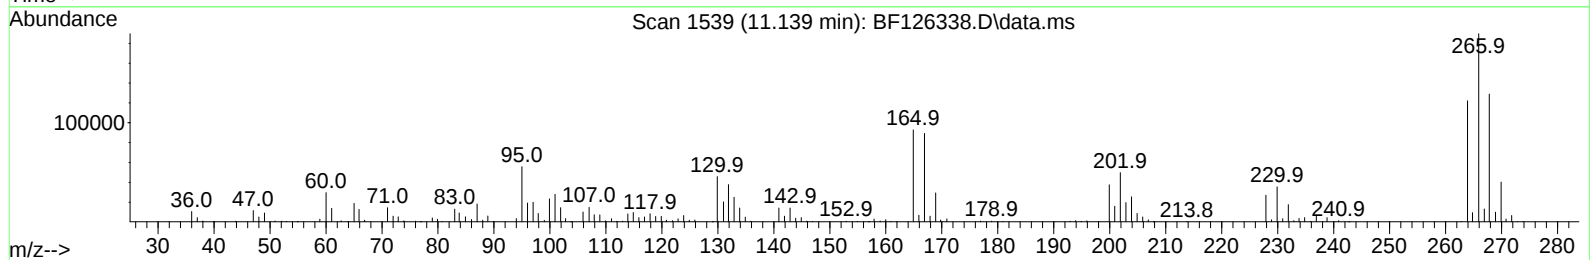


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126338.D
Acq On : 23 Dec 2021 11:59
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 04:10:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 13:00:11 2021
Response via : Initial Calibration

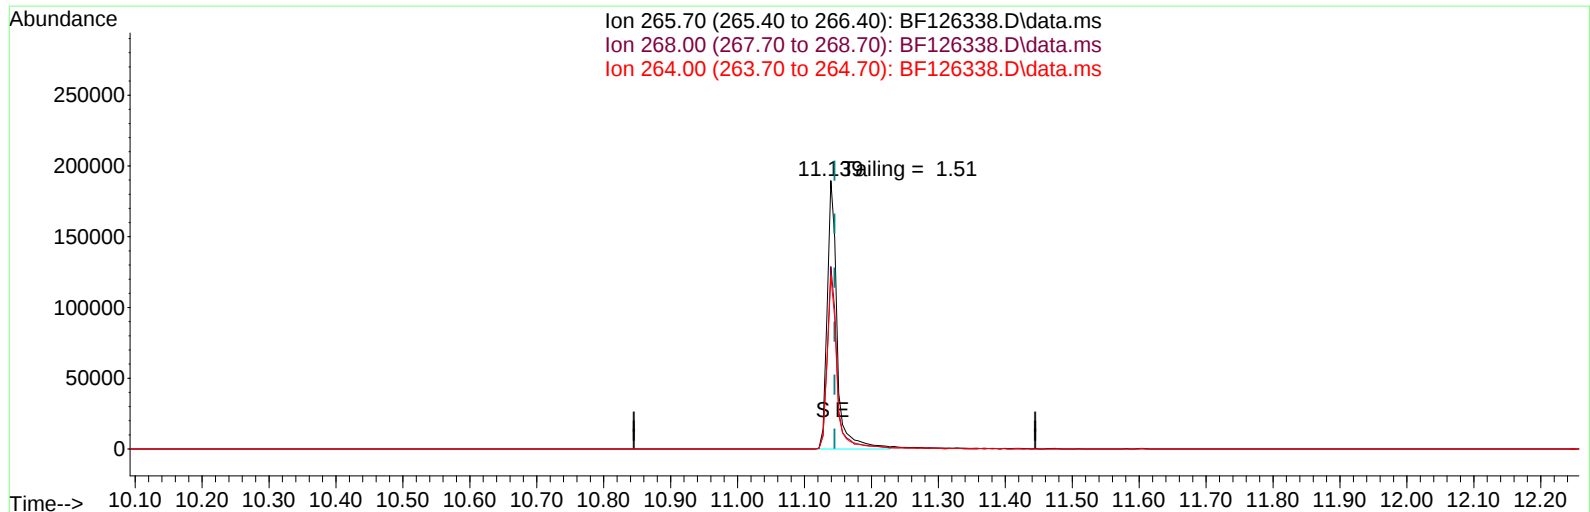

TIC: BF126338.D\data.ms

(70) Pentachlorophenol (C)




11.139min (-0.006) 46160.06 ng

response 199298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.99
264.00	69.90	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
 Data File : BF126338.D
 Acq On : 23 Dec 2021 11:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 25 04:10:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 22 13:00:11 2021
 Response via : Initial Calibration

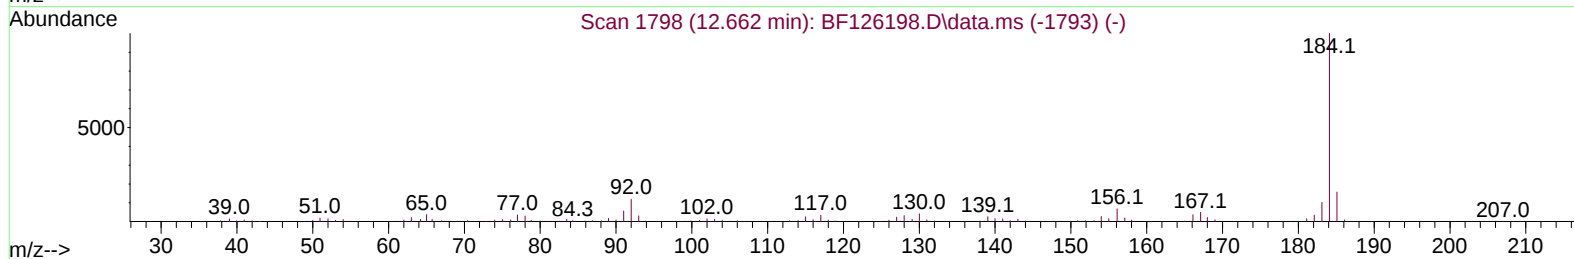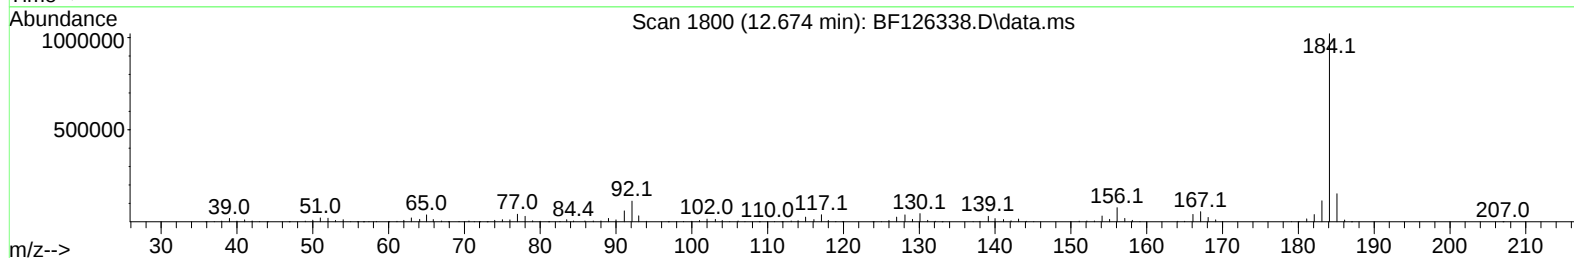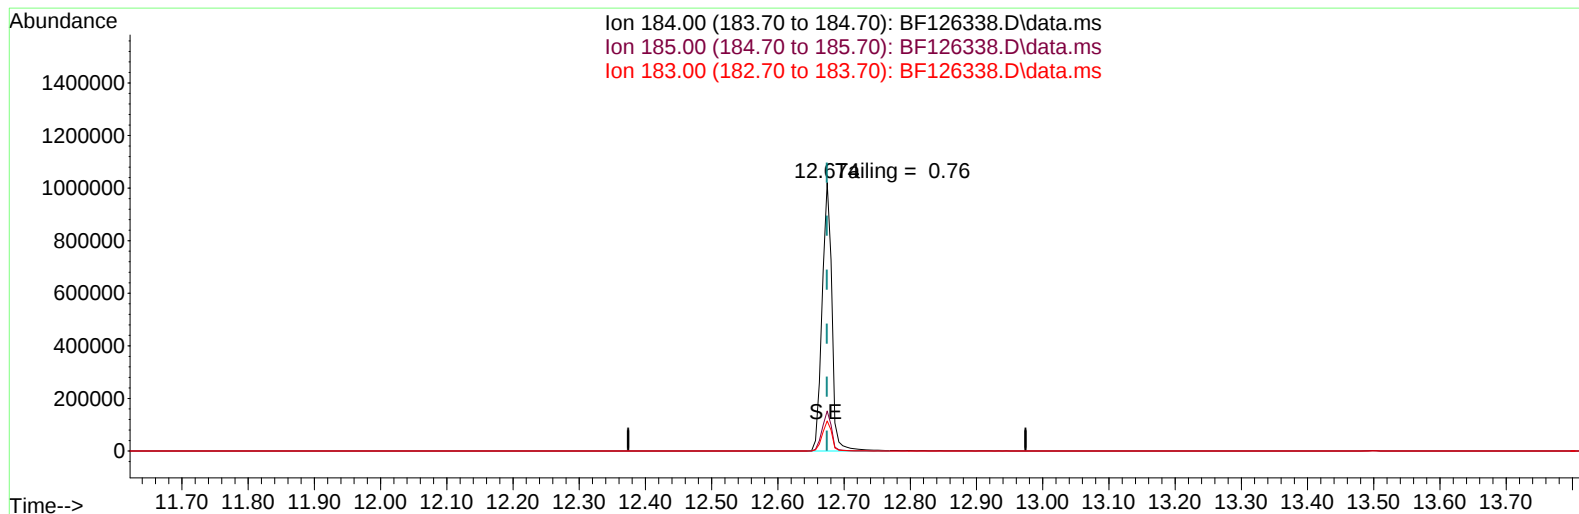

TIC: BF126338.D\data.ms

(77) Benzidine**12.674min (+ 0.000) 0.00 ng****response 1050851**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.94
183.00	10.10	11.21
0.00	0.00	0.00