

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
 Data File : BF126340.D
 Acq On : 23 Dec 2021 13:02
 Operator : JU/CG
 Sample : PB141629BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB141629BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126340.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.040	498	502	509	rVB	39040	52115	1.35%	0.206%
2	5.434	563	569	572	rBV	3619120	3838898	99.58%	15.181%
3	6.439	735	740	743	rBV	3194450	3855091	100.00%	15.245%
4	6.810	800	803	807	rBV	997316	863547	22.40%	3.415%
5	7.375	894	899	902	rBV	2572387	2620158	67.97%	10.361%
6	8.092	1017	1021	1029	rBV	1138213	1183840	30.71%	4.682%
7	9.175	1200	1205	1208	rBV	4074471	3771385	97.83%	14.914%
8	9.851	1316	1320	1331	rVB	1340049	1221069	31.67%	4.829%
9	10.639	1449	1454	1457	rBV	2212600	2080889	53.98%	8.229%
10	11.333	1568	1572	1588	rVB	1208593	1110900	28.82%	4.393%
11	12.927	1838	1843	1846	rBV	3145150	3025819	78.49%	11.966%
12	13.974	2017	2021	2031	rBV	792436	729666	18.93%	2.885%
13	14.068	2033	2037	2045	rBV	87036	104504	2.71%	0.413%
14	15.421	2262	2267	2273	rBV	610798	766653	19.89%	3.032%
15	16.739	2481	2491	2493	rBV6	27206	62982	1.63%	0.249%




Sum of corrected areas: 25287516

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126340.D
Acq On : 23 Dec 2021 13:02
Operator : JU/CG
Sample : PB141629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

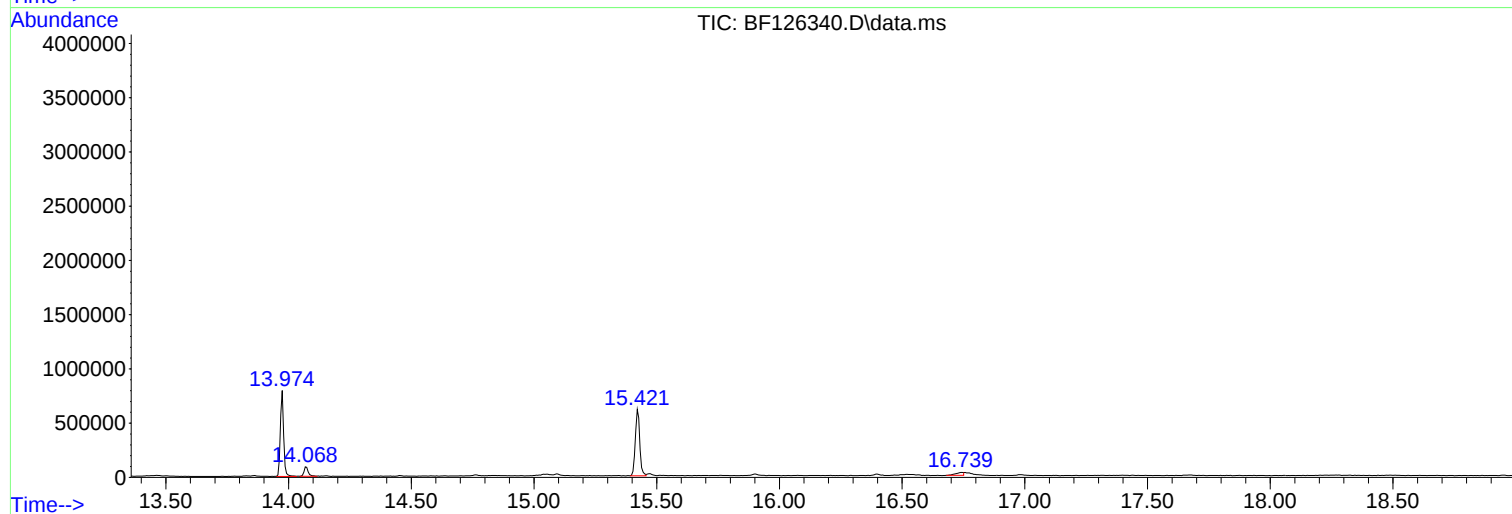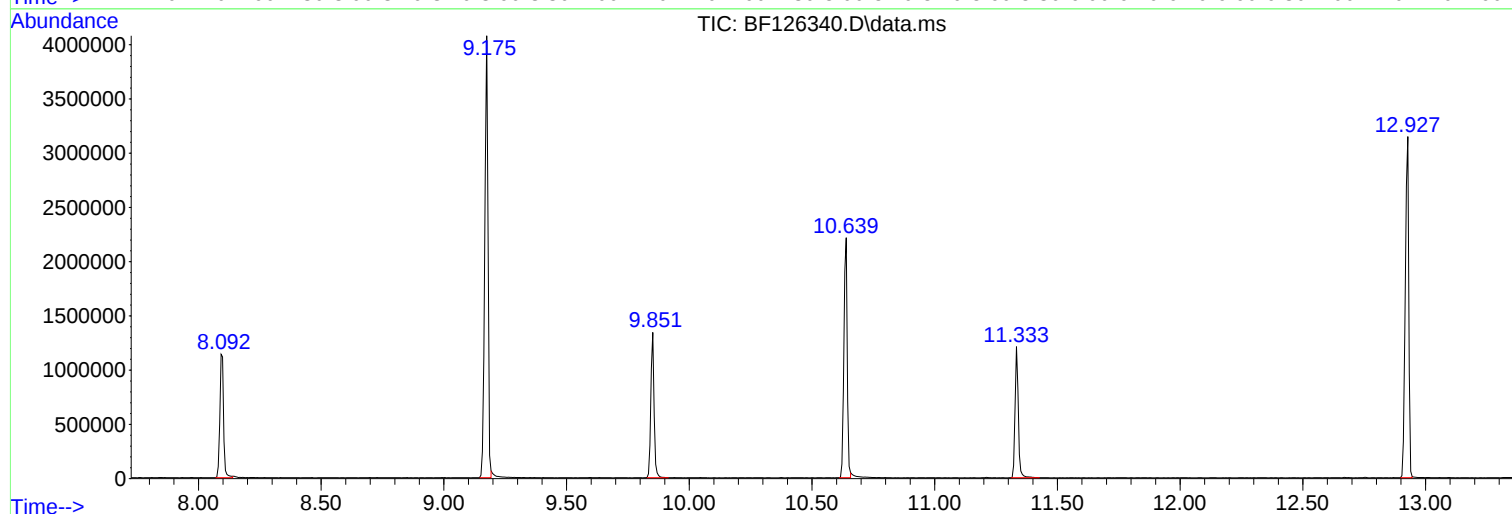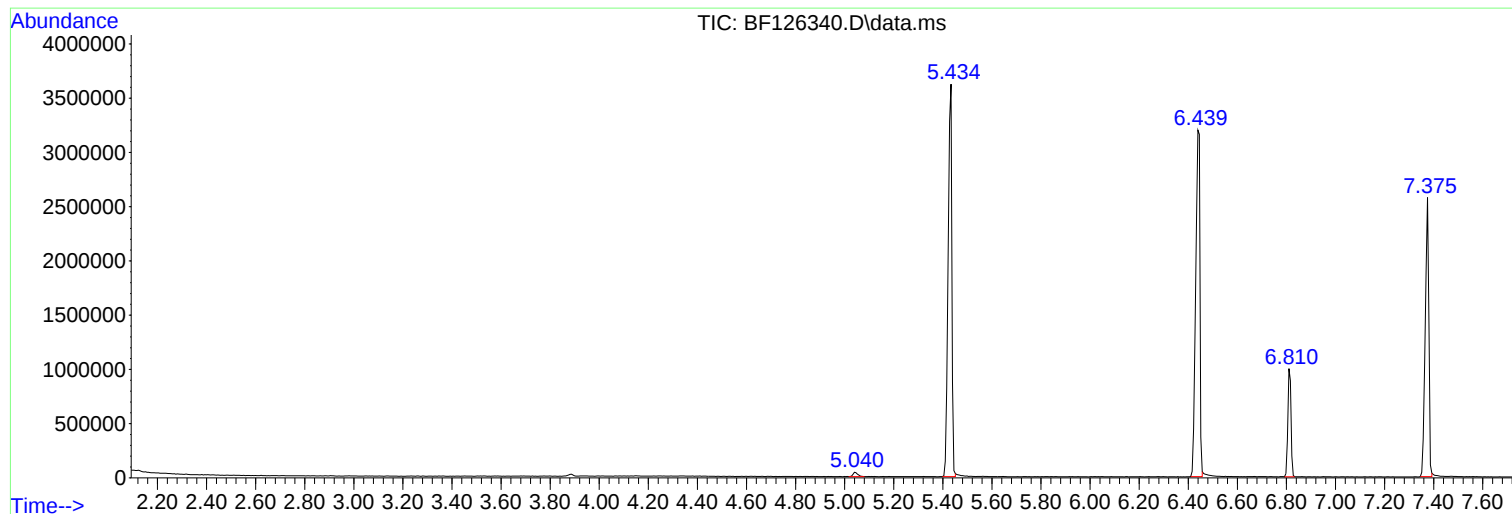

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126340.D
Acq On : 23 Dec 2021 13:02
Operator : JU/CG
Sample : PB141629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141629BL









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.068	2.86 ng	104504	Chrysene-d12	13.974

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	58
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	50
4			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	38
5			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	32

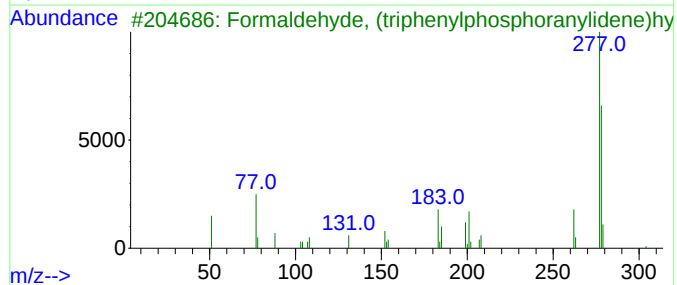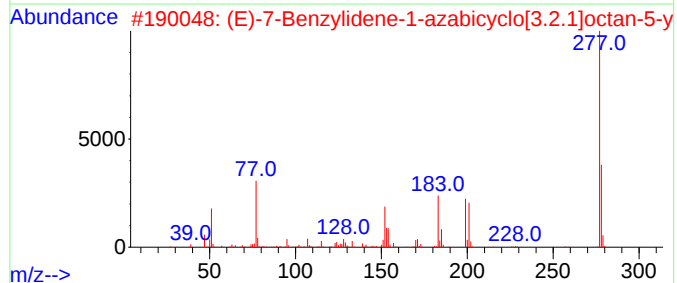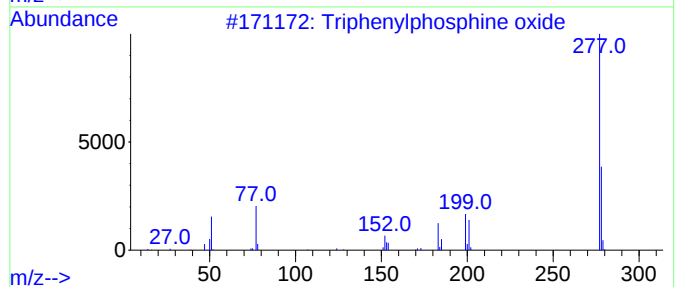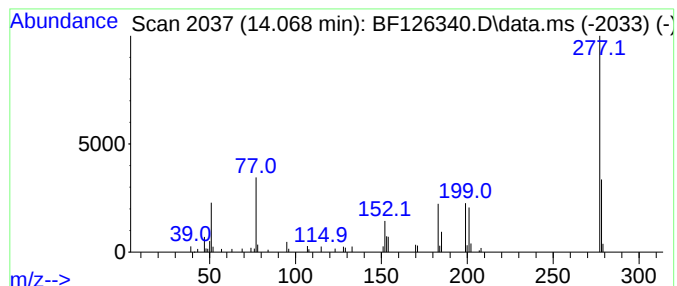

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126340.D
Acq On : 23 Dec 2021 13:02
Operator : JU/CG
Sample : PB141629BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB141629BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Triphenylphosph...	14.068	2.9	ng	104504	5	13.974	729666	20.0