

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
 Data File : BF126345.D
 Acq On : 23 Dec 2021 15:38
 Operator : JU/CG
 Sample : M5187-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SASP2-119-1-40-57

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.028	493	500	508	rVB	29219	40033	1.30%	0.190%
2	5.428	563	568	571	rBV	2871897	2792876	90.48%	13.255%
3	6.439	735	740	743	rBV	2682564	2866394	92.87%	13.604%
4	6.810	800	803	807	rBV	878442	754911	24.46%	3.583%
5	7.375	894	899	902	rBV	1993688	1877090	60.81%	8.908%
6	8.092	1017	1021	1039	rVB	1026542	1062174	34.41%	5.041%
7	8.692	1120	1123	1127	rVB	47448	38076	1.23%	0.181%
8	9.175	1200	1205	1208	rBV	3495904	3086610	100.00%	14.649%
9	9.257	1216	1219	1224	rBV2	79128	69444	2.25%	0.330%
10	9.851	1316	1320	1327	rVB	1376251	1208994	39.17%	5.738%
11	10.639	1449	1454	1463	rBV	1771110	1808385	58.59%	8.582%
12	11.298	1563	1566	1569	rBV2	40243	38907	1.26%	0.185%
13	11.333	1569	1572	1578	rVB	1304821	1096077	35.51%	5.202%
14	11.504	1598	1601	1608	rVB	39401	38319	1.24%	0.182%
15	11.869	1660	1663	1666	rBV	47023	43843	1.42%	0.208%
16	11.904	1666	1669	1672	rVB	67737	60889	1.97%	0.289%
17	12.321	1735	1740	1742	rBV	36575	38361	1.24%	0.182%
18	12.374	1746	1749	1754	rVB	60187	52459	1.70%	0.249%
19	12.921	1838	1842	1846	rBV	2508071	2372763	76.87%	11.261%
20	13.580	1951	1954	1957	rVB	52655	49474	1.60%	0.235%
21	13.892	2003	2007	2009	rBV	42773	42968	1.39%	0.204%
22	13.974	2017	2021	2032	rVB	812487	810992	26.27%	3.849%
23	14.068	2033	2037	2042	rVB	61989	66104	2.14%	0.314%
24	15.421	2262	2267	2273	rBV	593596	754743	24.45%	3.582%




Sum of corrected areas: 21070886

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126345.D
Acq On : 23 Dec 2021 15:38
Operator : JU/CG
Sample : M5187-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-40-57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

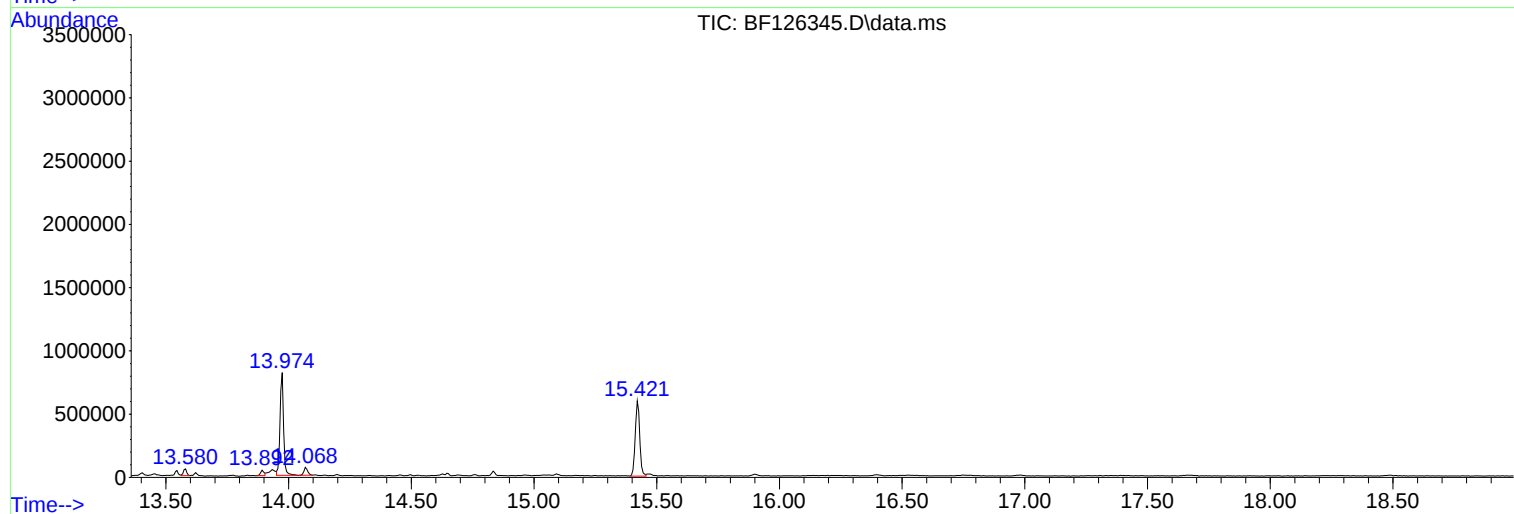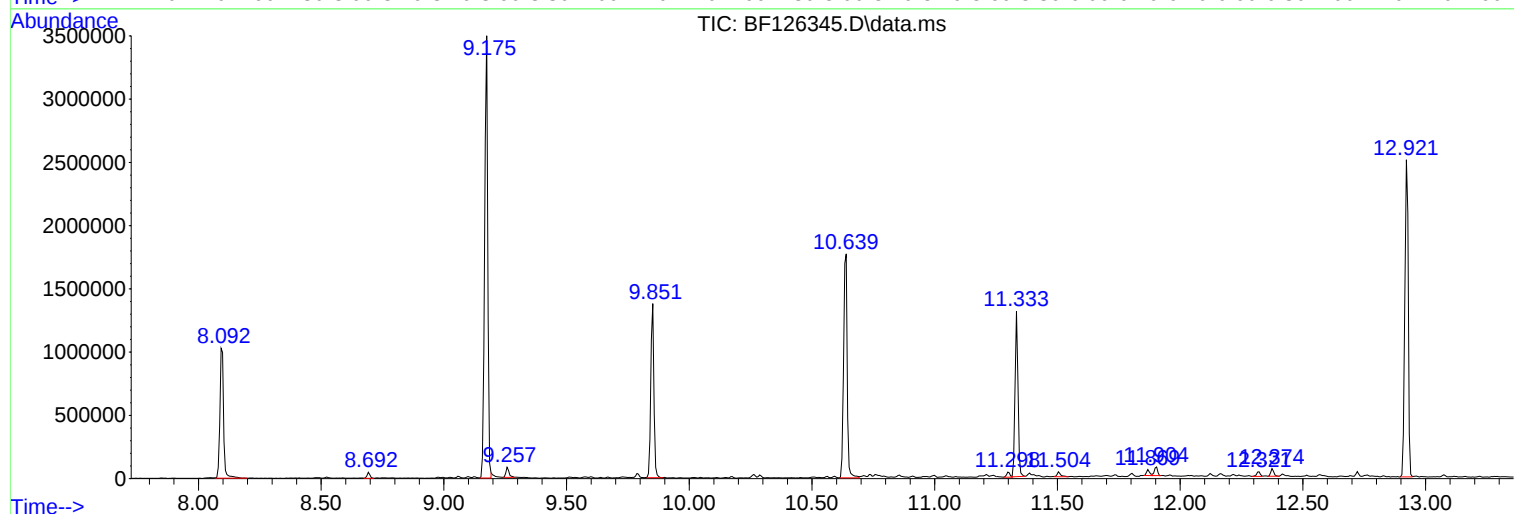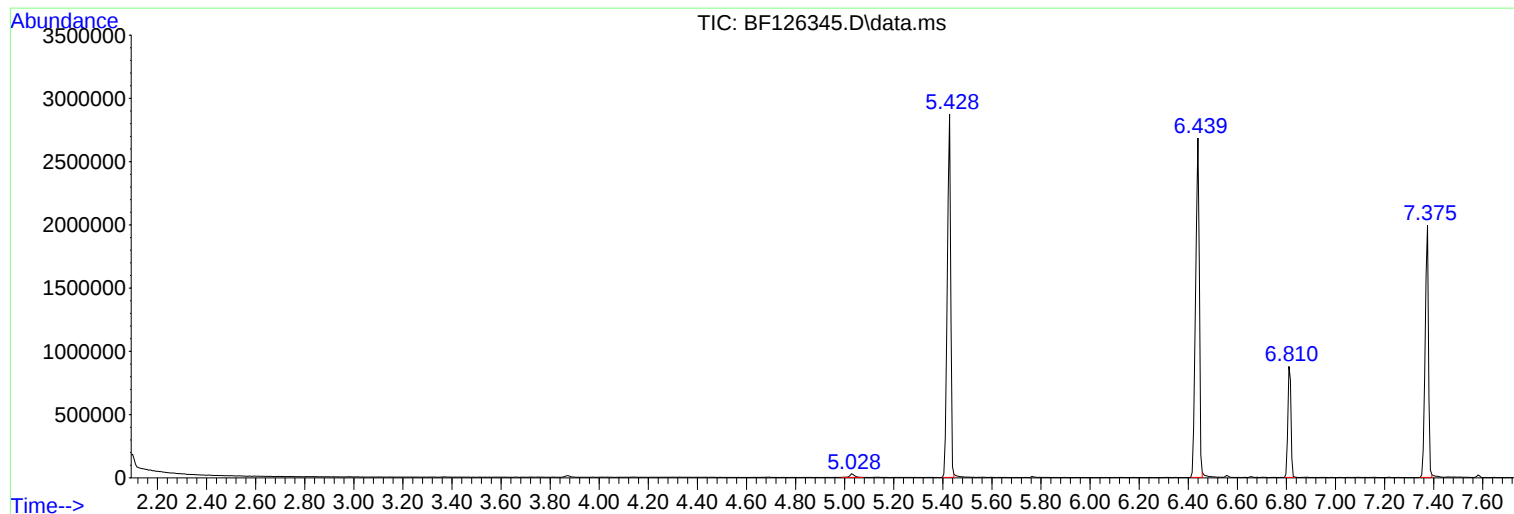

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126345.D
Acq On : 23 Dec 2021 15:38
Operator : JU/CG
Sample : M5187-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-40-57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126345.D
Acq On : 23 Dec 2021 15:38
Operator : JU/CG
Sample : M5187-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SASP2-119-1-40-57

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------