


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
 Data File : BF126338.D
 Acq On : 23 Dec 2021 11:59
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 22 13:00:11 2021

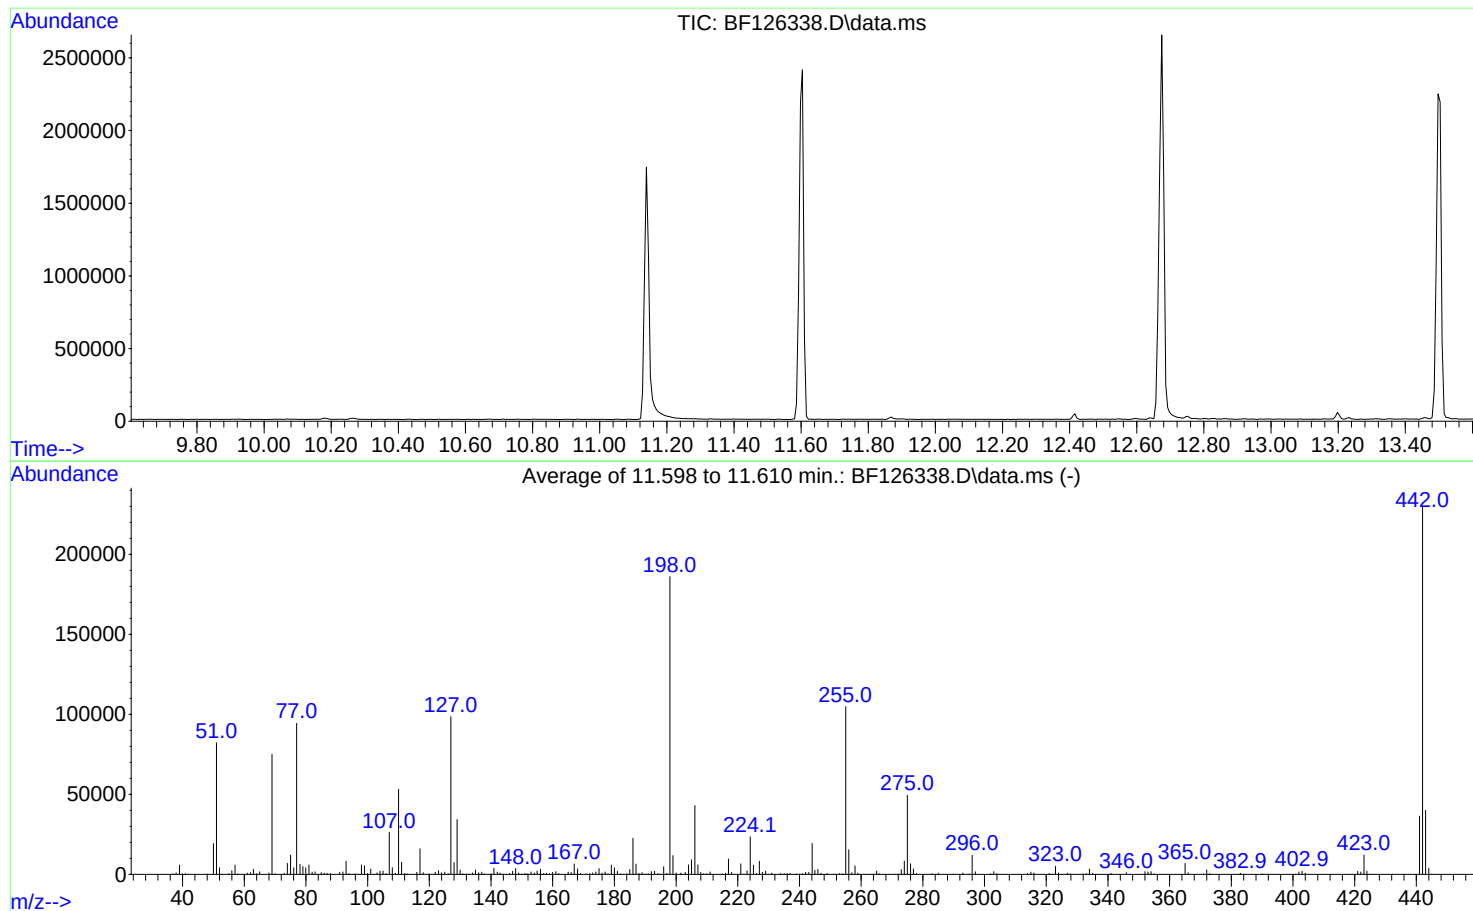




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.2	82209	PASS
68	69	0.00	2	1.3	954	PASS
69	198	0.00	100	40.4	75108	PASS
70	69	0.00	2	0.6	419	PASS
127	198	10	80	52.9	98539	PASS
197	198	0.00	2	0.4	721	PASS
198	198	100	100	100.0	186099	PASS
199	198	5	9	6.3	11701	PASS
275	198	10	60	26.6	49453	PASS
365	198	1	100	3.6	6777	PASS
441	198	0.01	100	19.6	36405	PASS
442	442	50	100	100.0	229888	PASS
443	442	15	24	17.4	39973	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126338.D
Acq On : 23 Dec 2021 11:59
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 25 04:10:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 13:00:11 2021
Response via : Initial Calibration

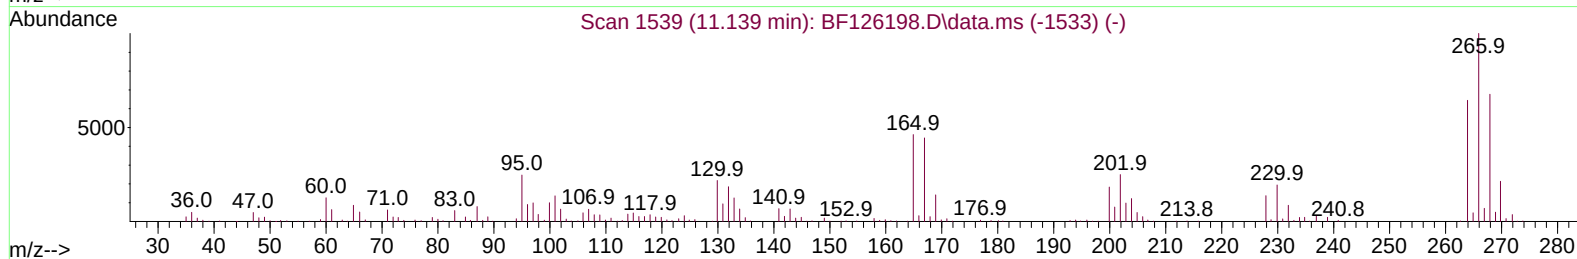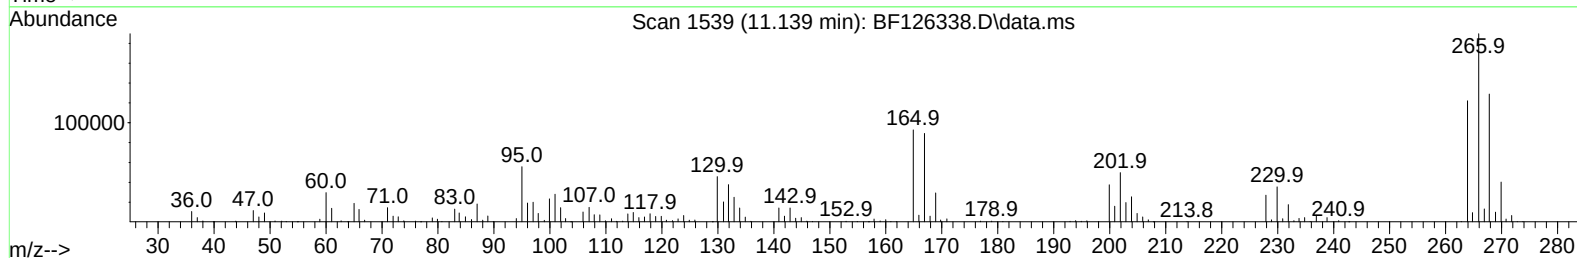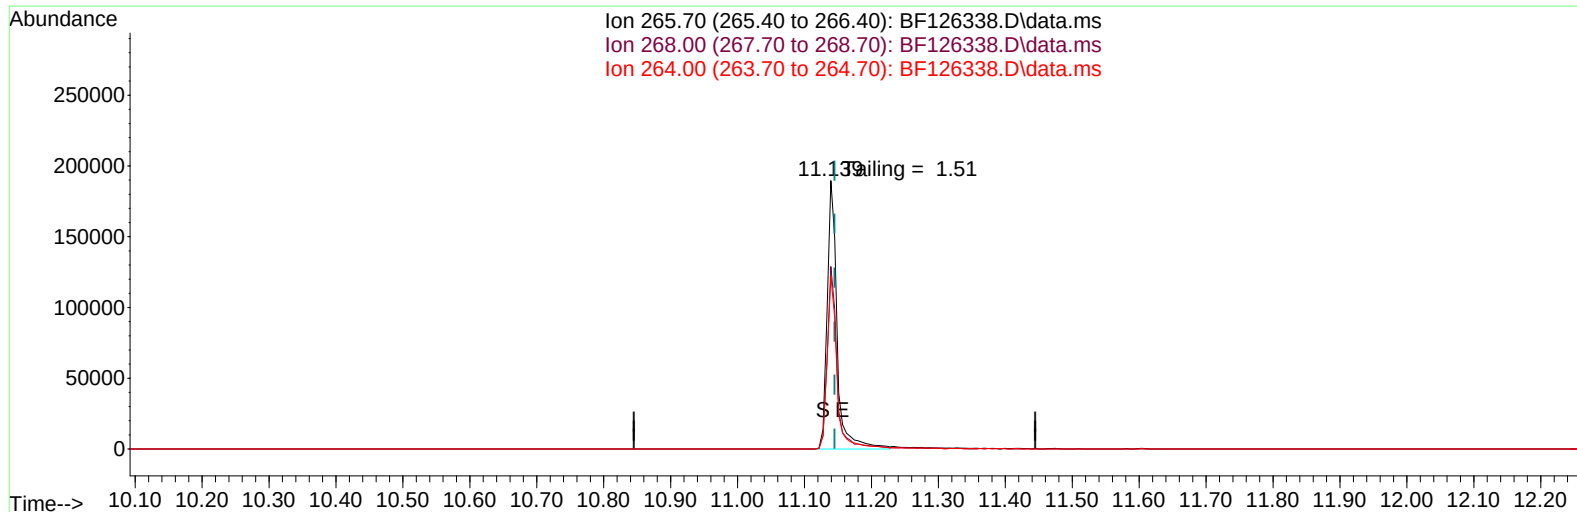

TIC: BF126338.D\data.ms

(70) Pentachlorophenol (C)

11.139min (-0.006) 46160.06 ng




response 199298

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	67.99
264.00	69.90	64.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122321\
Data File : BF126338.D
Acq On : 23 Dec 2021 11:59
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 25 04:10:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 22 13:00:11 2021
Response via : Initial Calibration

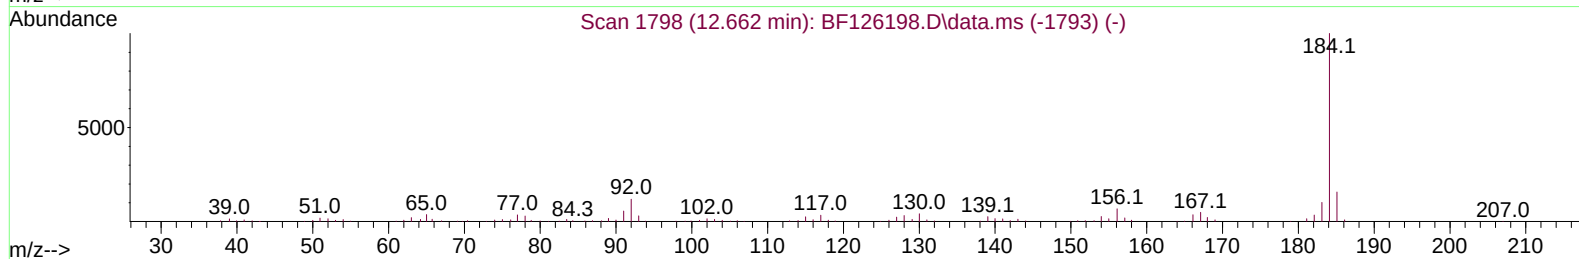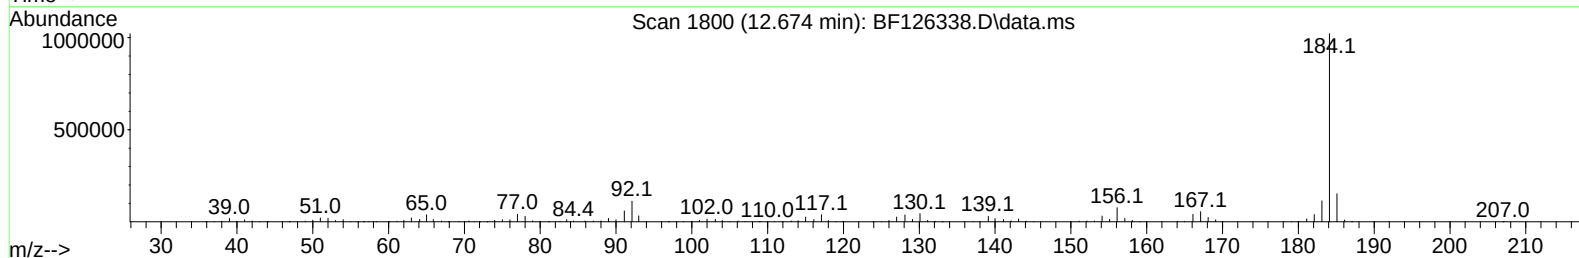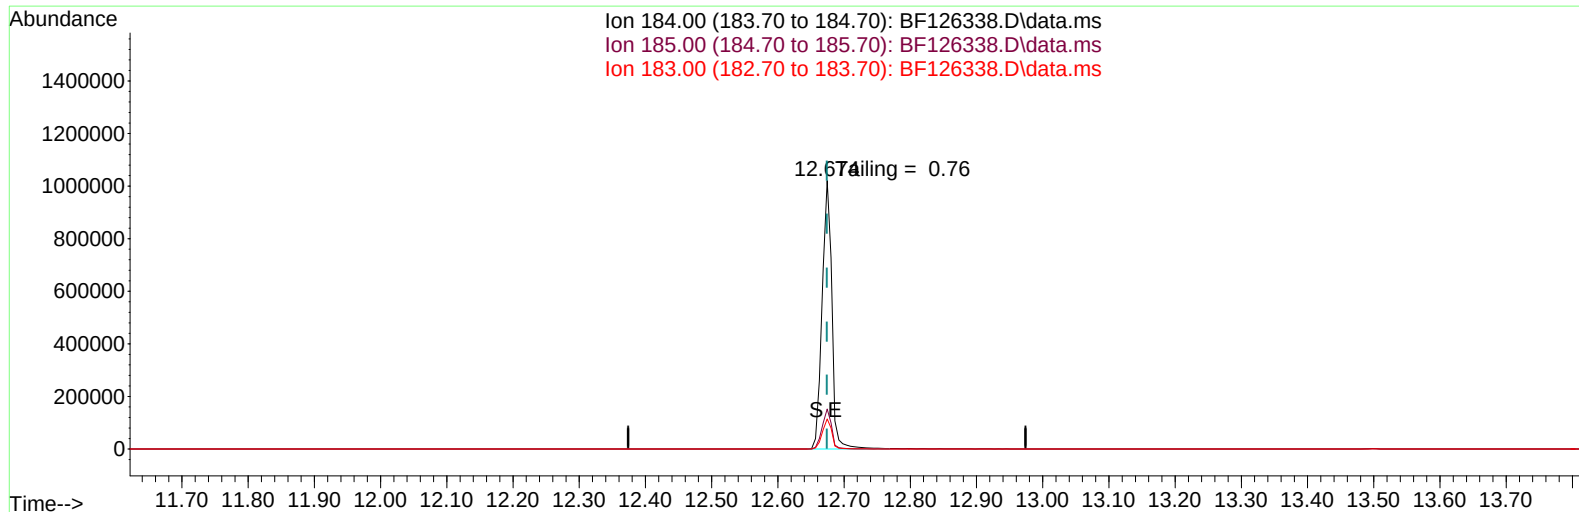

TIC: BF126338.D\data.ms

(77) Benzidine

12.674min (+ 0.000) 0.00 ng

response 1050851

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.94
183.00	10.10	11.21
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
12/23/2021	BNA_F	<u>BF126338.D</u>
Compound Name	Response	Retention Time
DDT	423460	13.504
DDD	11838	13.198
DDE	837	12.863
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12675	436135	2.91

Instrument :
BNA_F
ClientSampleId :
DFTPP