
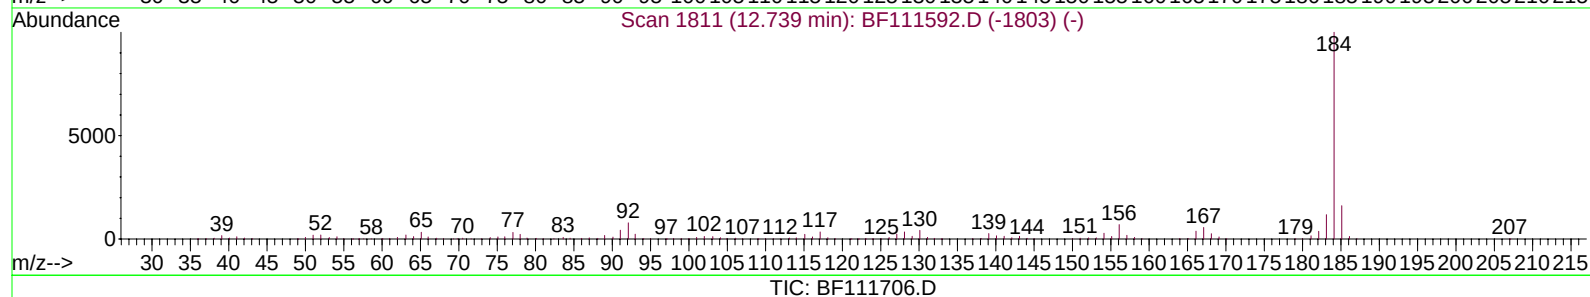
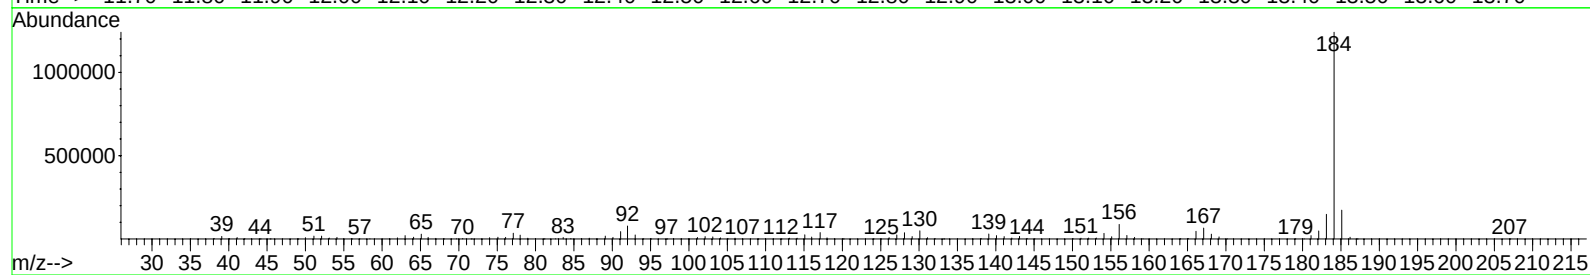


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122618\
 Data File : BF111706.D
 Acq On : 26 Dec 2018 10:38
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 17:37:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 19 17:39:39 2018
 Response via : Initial Calibration

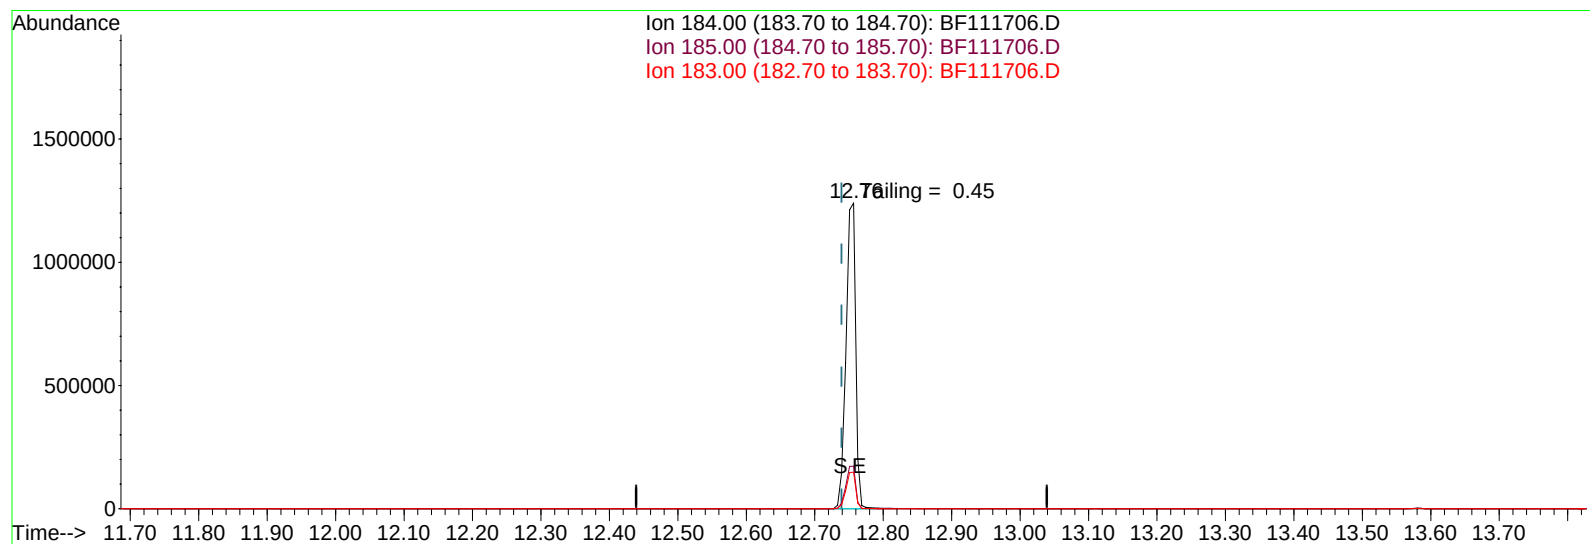

(77) Benzidine




12.757min (+0.018) 0.00ng

response 1217420

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	13.93
183.00	11.60	11.96
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF122618\
Data File : BF111706.D
Acq On : 26 Dec 2018 10:38
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 26 17:37:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 19 17:39:39 2018
Response via : Initial Calibration

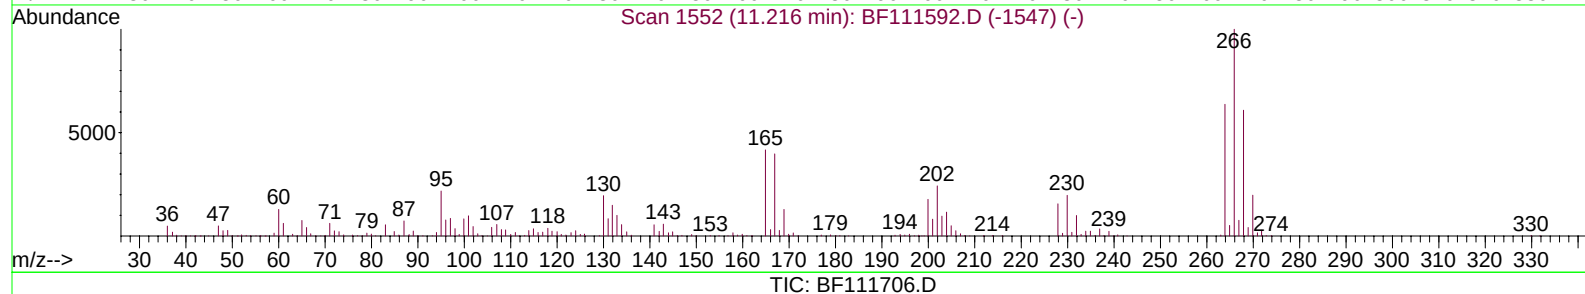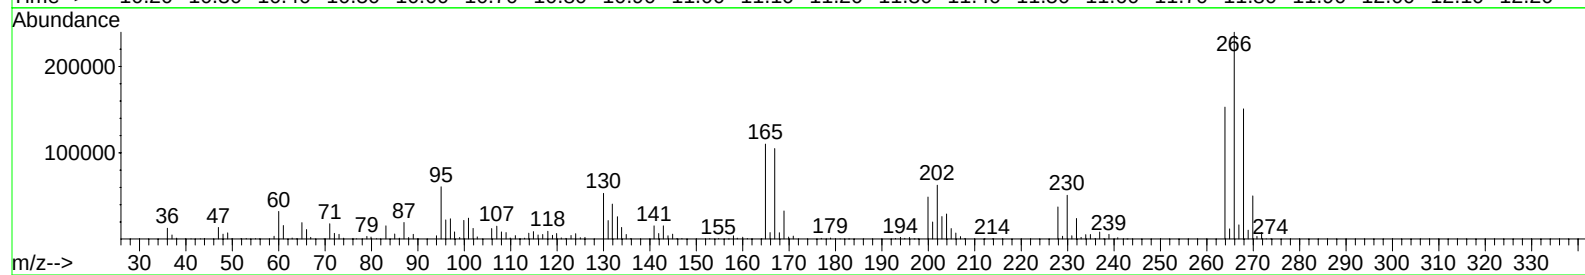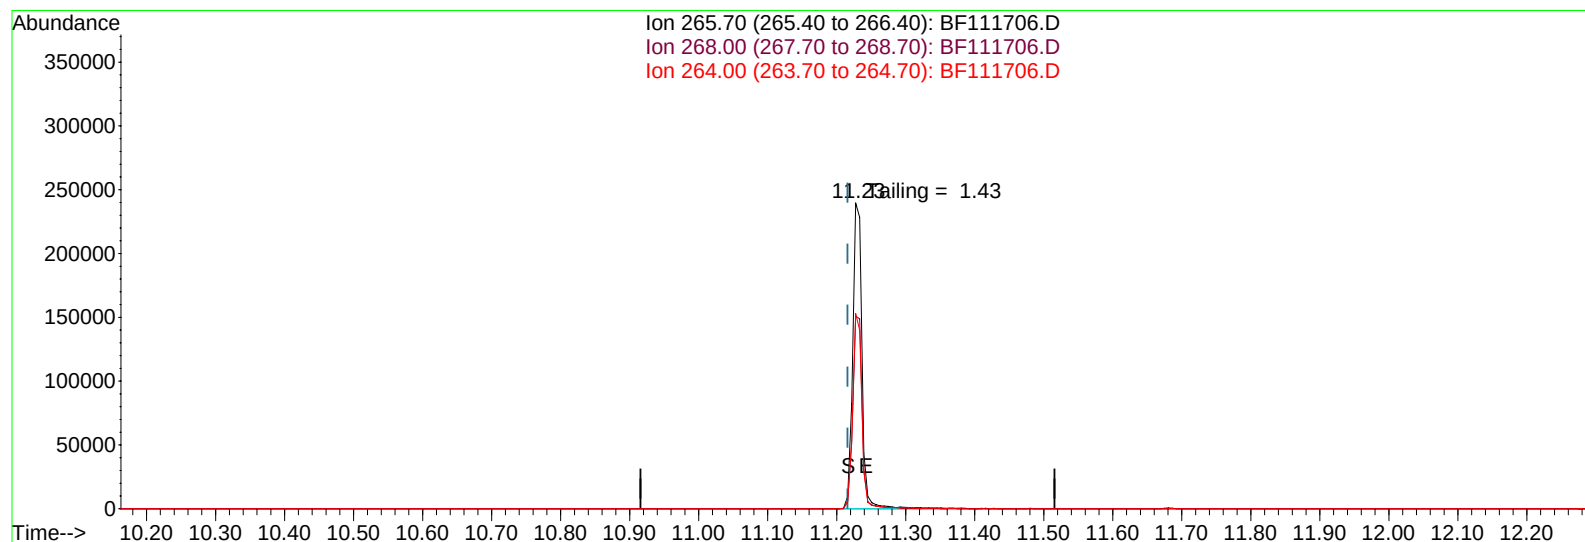

(70) Pentachlorophenol (C)

11.227min (+0.012) 33086.11ng

response 222335

Ion	Exp%	Act%
265.70	100	100
268.00	59.90	63.01
264.00	61.40	63.84
0.00	0.00	0.00