

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122618\
 Data File : BF111739.D
 Acq On : 27 Dec 2018 2:56
 Operator : JU/SJ
 Sample : J6547-04 2X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 COMP-1B

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.181	11	16	22	rVB	64103	83632	4.75%	0.437%
2	5.116	511	515	522	rVB	83982	90091	5.12%	0.470%
3	5.534	582	586	590	rBV	1806070	1637543	93.03%	8.549%
4	6.540	753	757	767	rBV	1950226	1760162	100.00%	9.190%
5	6.675	776	780	784	rBV	1848596	1694423	96.27%	8.846%
6	6.904	815	819	823	rBV	1166092	913218	51.88%	4.768%
7	7.063	842	846	849	rBV	1656081	1353427	76.89%	7.066%
8	7.457	909	913	916	rBV	1174737	979610	55.65%	5.114%
9	8.187	1032	1037	1040	rBV	1314214	1034326	58.76%	5.400%
10	9.257	1215	1219	1222	rBV	2212066	1690253	96.03%	8.825%
11	9.645	1282	1285	1290	rVB	229455	192327	10.93%	1.004%
12	9.939	1332	1335	1339	rVB	1220916	1018454	57.86%	5.317%
13	10.486	1425	1428	1434	rBV2	23657	25027	1.42%	0.131%
14	10.728	1465	1469	1474	rBV	1251522	1035371	58.82%	5.406%
15	10.845	1486	1489	1497	rVB4	29129	56966	3.24%	0.297%
16	11.322	1568	1570	1574	rVB	27770	24361	1.38%	0.127%
17	11.428	1584	1588	1590	rBV	1304053	1057714	60.09%	5.522%
18	11.451	1590	1592	1595	rVV	302445	241059	13.70%	1.259%
19	11.504	1598	1601	1603	rVB	78416	68962	3.92%	0.360%
20	11.927	1671	1673	1675	rBV	36859	38514	2.19%	0.201%
21	11.951	1675	1677	1681	rVB2	83840	89594	5.09%	0.468%
22	12.004	1684	1686	1689	rVB2	29500	23251	1.32%	0.121%
23	12.039	1689	1692	1695	rBV	67582	76301	4.33%	0.398%
24	12.222	1721	1723	1725	rBV	49026	39792	2.26%	0.208%
25	12.516	1770	1773	1776	rBV3	51750	55355	3.14%	0.289%
26	12.639	1791	1794	1798	rBV	540541	450456	25.59%	2.352%
27	12.869	1828	1833	1839	rBV	457479	495047	28.13%	2.585%
28	13.010	1853	1857	1860	rBV	1877175	1550051	88.06%	8.093%
29	14.069	2033	2037	2039	rBV2	867390	902508	51.27%	4.712%
30	15.557	2287	2290	2293	rBV	431405	476066	27.05%	2.485%


Sum of corrected areas: 19153861

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122618\
Data File : BF111739.D
Acq On : 27 Dec 2018 2:56
Operator : JU/SJ
Sample : J6547-04 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
COMP-1B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

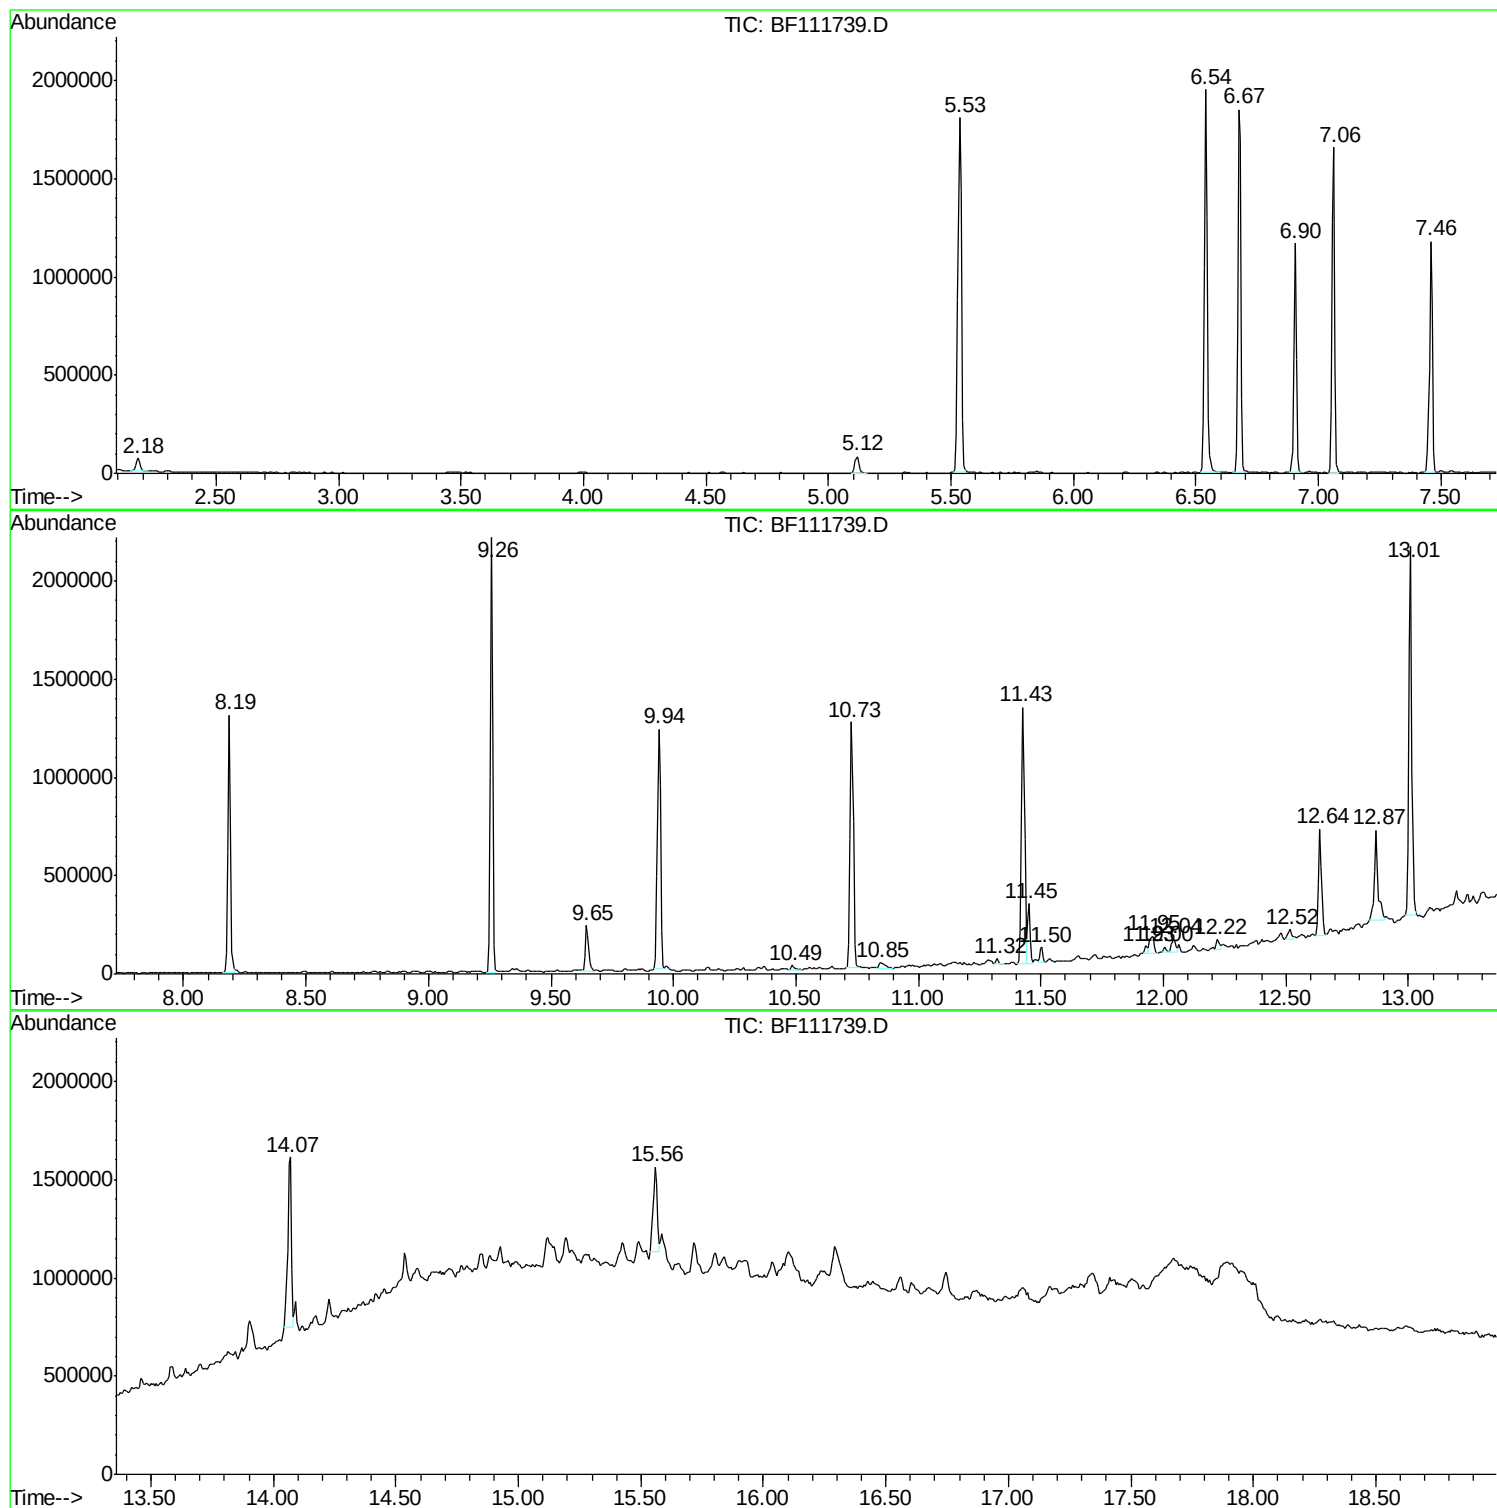

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF122618\
Data File : BF111739.D
Acq On : 27 Dec 2018 2:56
Operator : JU/SJ
Sample : J6547-04 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1B










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.67 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.67	37.11 ng	1694420	1,4-Dichlorobenzene-d4	6.90

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10
4		1,3,5-Trifluorobenzene	132	C6H3F3	000372-38-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

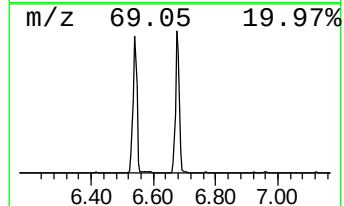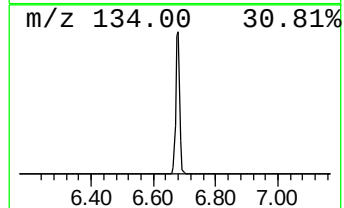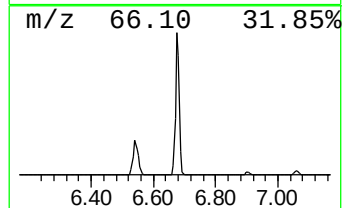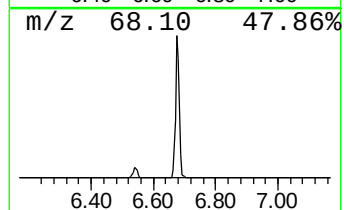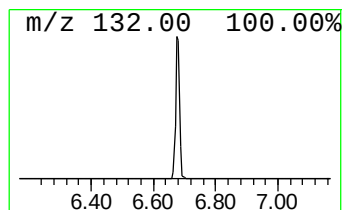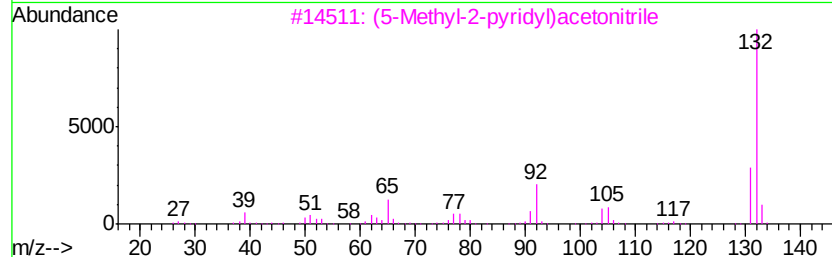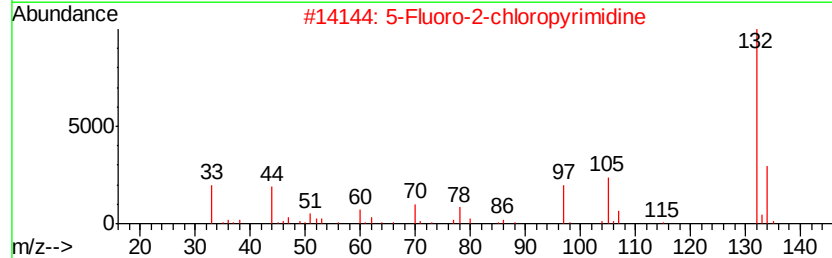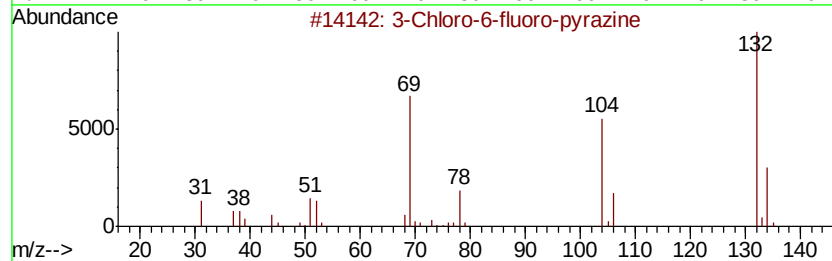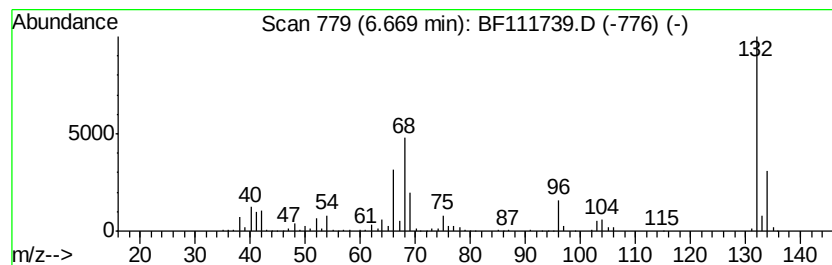

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122618\
Data File : BF111739.D
Acq On : 27 Dec 2018 2:56
Operator : JU/SJ
Sample : J6547-04 2X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
COMP-1B

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.67	6.67	37.1	ng	1694420	1	6.90	913218	20.0