


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF122618\  
 Data File : BF111706.D  
 Acq On : 26 Dec 2018 10:38  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF121918.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Dec 19 17:39:39 2018

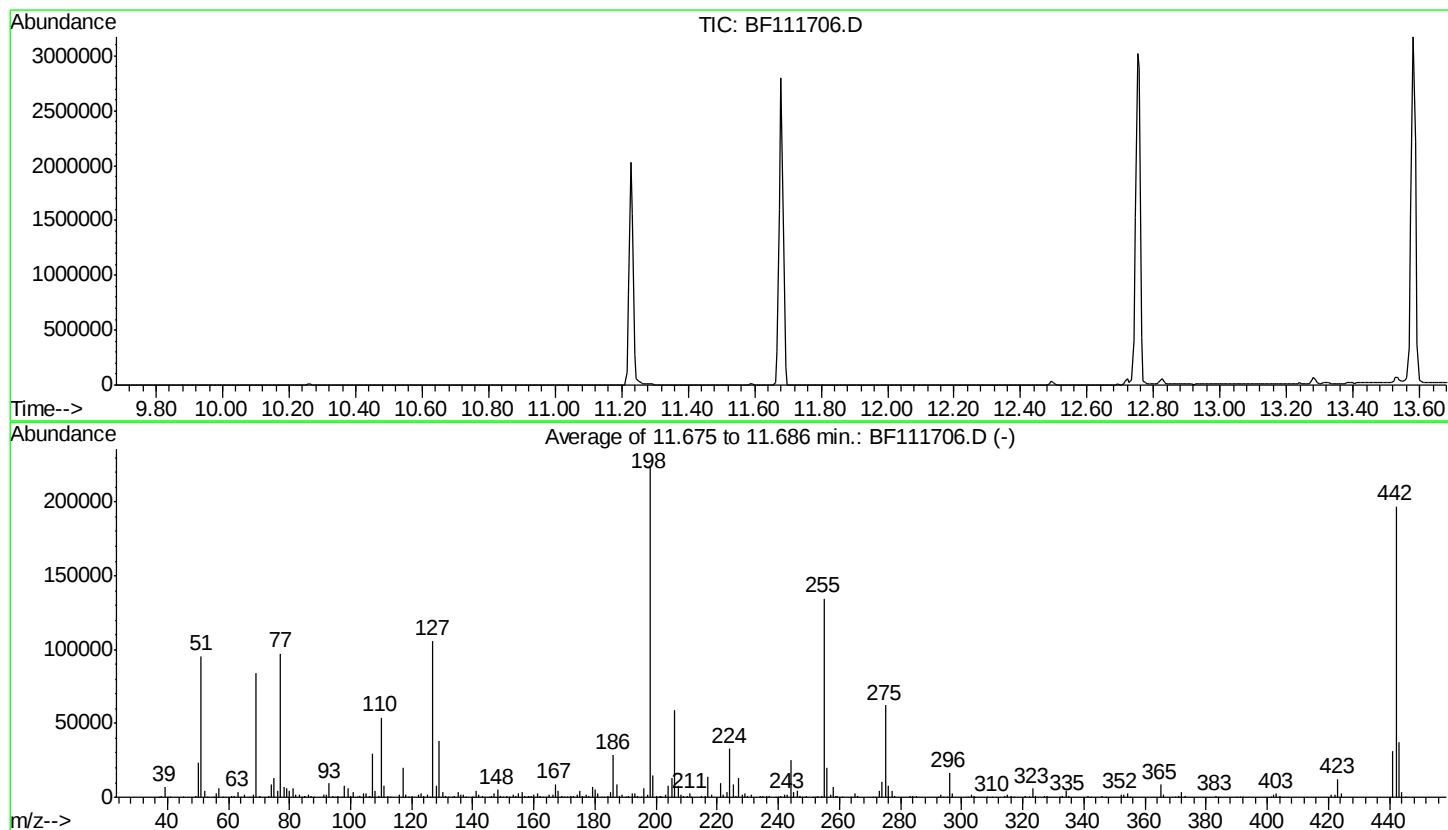

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1625

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 42.6      | 95616   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.9       | 1600    | PASS             |
| 69          | 198          | 0.00         | 100          | 37.6      | 84381   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 502     | PASS             |
| 127         | 198          | 10           | 80           | 47.1      | 105893  | PASS             |
| 197         | 198          | 0.00         | 2            | 0.7       | 1622    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 224661  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 15144   | PASS             |
| 275         | 198          | 10           | 60           | 27.7      | 62306   | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 8431    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.8      | 31042   | PASS             |
| 442         | 198          | 50           | 100          | 87.7      | 197056  | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 37661   | PASS             |