


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF122618\
 Data File : BF111719.D
 Acq On : 26 Dec 2018 17:48
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

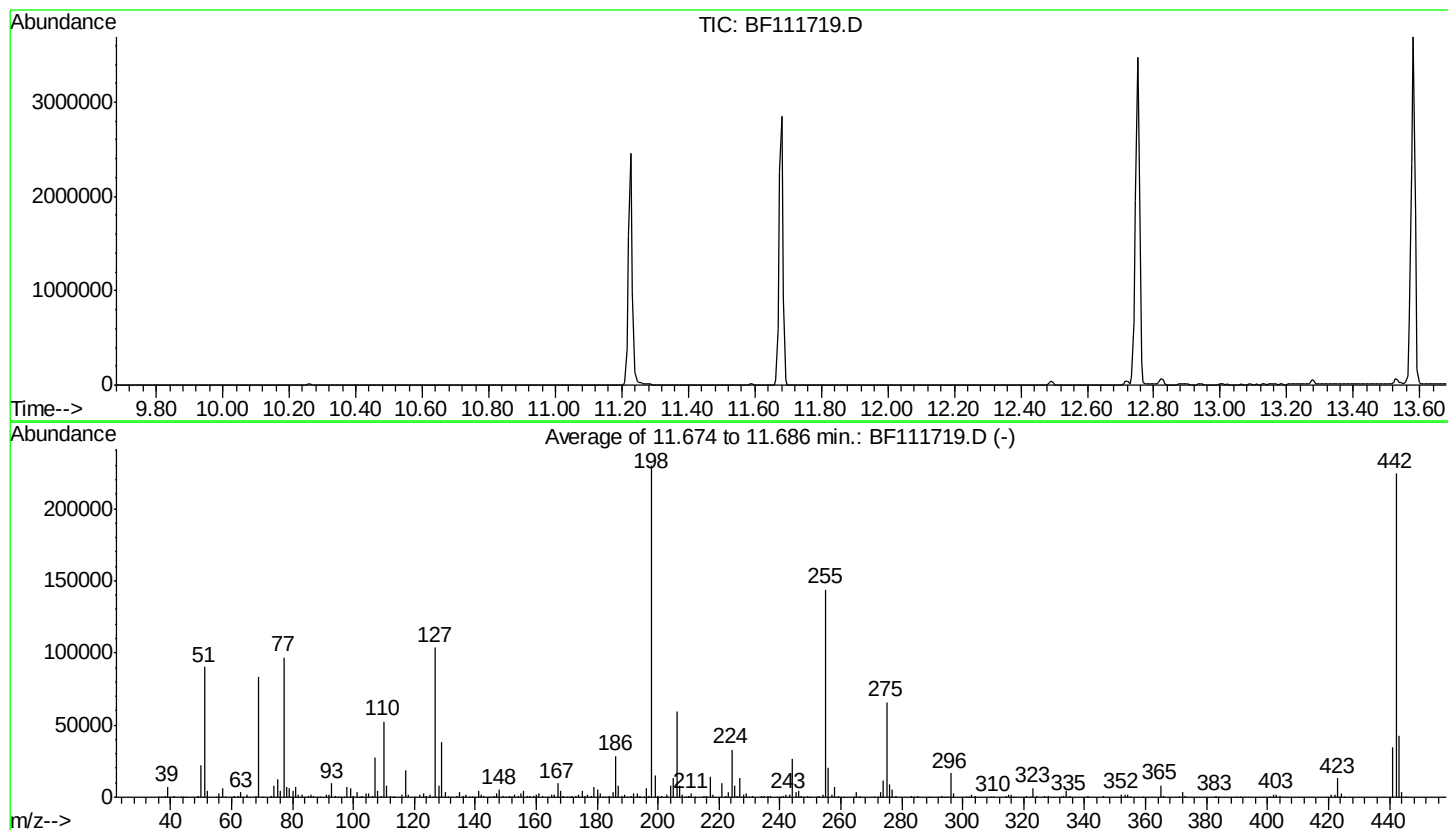

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1624

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.2	90069	PASS
68	69	0.00	2	1.6	1300	PASS
69	198	0.00	100	36.2	83117	PASS
70	69	0.00	2	0.4	364	PASS
127	198	10	80	45.1	103512	PASS
197	198	0.00	2	0.5	1170	PASS
198	198	100	100	100.0	229762	PASS
199	198	5	9	6.7	15336	PASS
275	198	10	60	28.7	66034	PASS
365	198	1	100	3.6	8338	PASS
441	198	0.01	100	15.2	34893	PASS
442	198	50	100	97.5	224064	PASS
443	442	15	24	19.0	42610	PASS