


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF122618\
 Data File : BF111745.D
 Acq On : 27 Dec 2018 6:07
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF121918.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Dec 19 17:39:39 2018

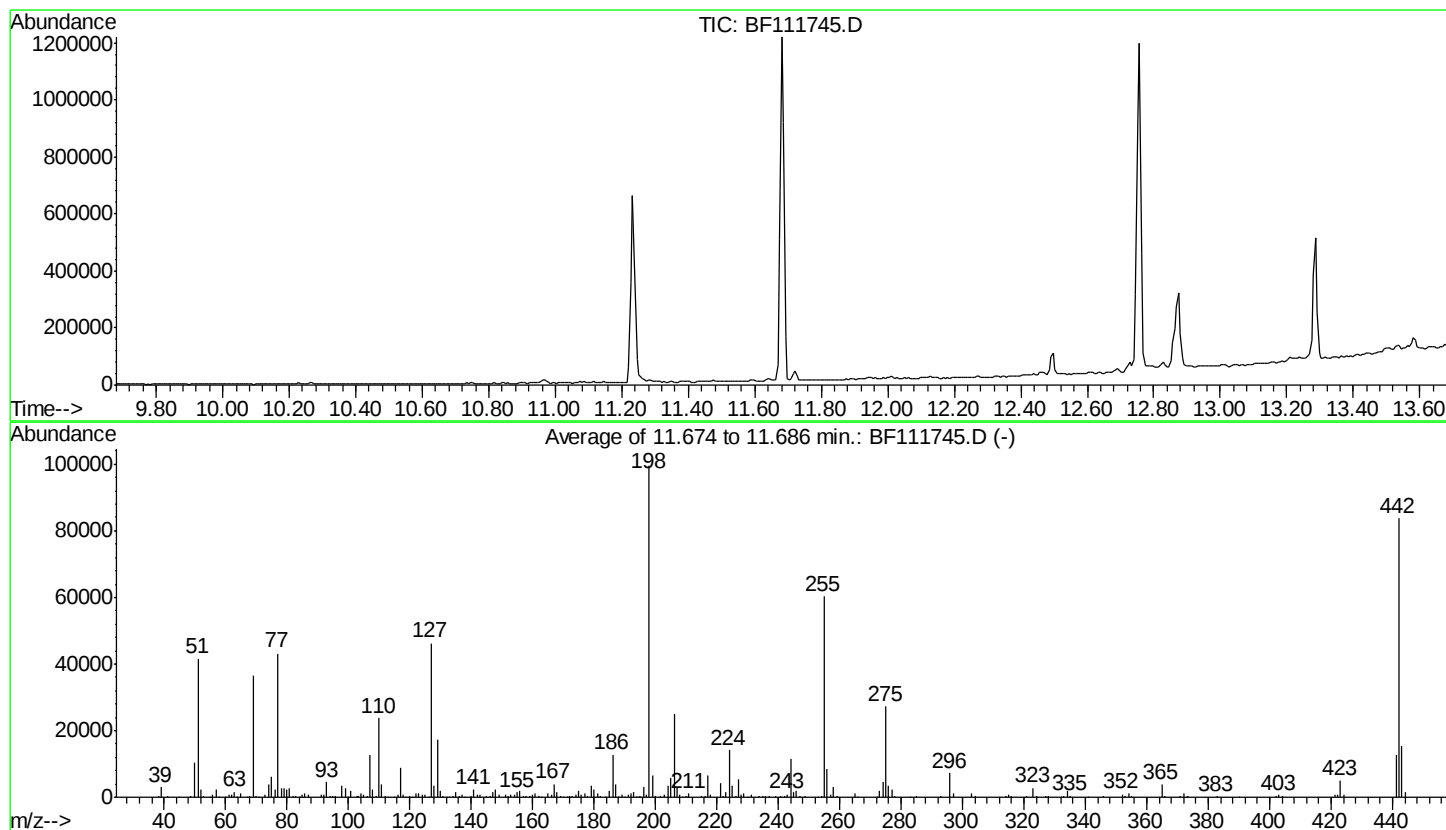

AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	41705	PASS
68	69	0.00	2	1.3	485	PASS
69	198	0.00	100	36.8	36604	PASS
70	69	0.00	2	1.2	433	PASS
127	198	10	80	46.4	46197	PASS
197	198	0.00	2	0.7	742	PASS
198	198	100	100	100.0	99562	PASS
199	198	5	9	6.7	6699	PASS
275	198	10	60	27.3	27224	PASS
365	198	1	100	3.7	3733	PASS
441	198	0.01	100	12.8	12784	PASS
442	198	50	100	84.1	83754	PASS
443	442	15	24	18.3	15287	PASS